

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121721\
 Data File : PP042052.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2021 18:59
 Operator : AJ\MA
 Sample : M5080-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CONCRETE-PAD

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/17/2021
 Supervised By :mohammad ahmed 12/17/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 03:42:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 06:21:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.068	331296	575387	25.677m	23.454
2) SA Decachlor...	10.923	9.428	355618	452484	26.985	22.505

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121721\
Data File : PP042052.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2021 18:59
Operator : AJ\MA
Sample : M5080-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CONCRETE-PAD


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/17/2021
Supervised By :mohammad ahmed 12/17/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 03:42:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 06:21:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

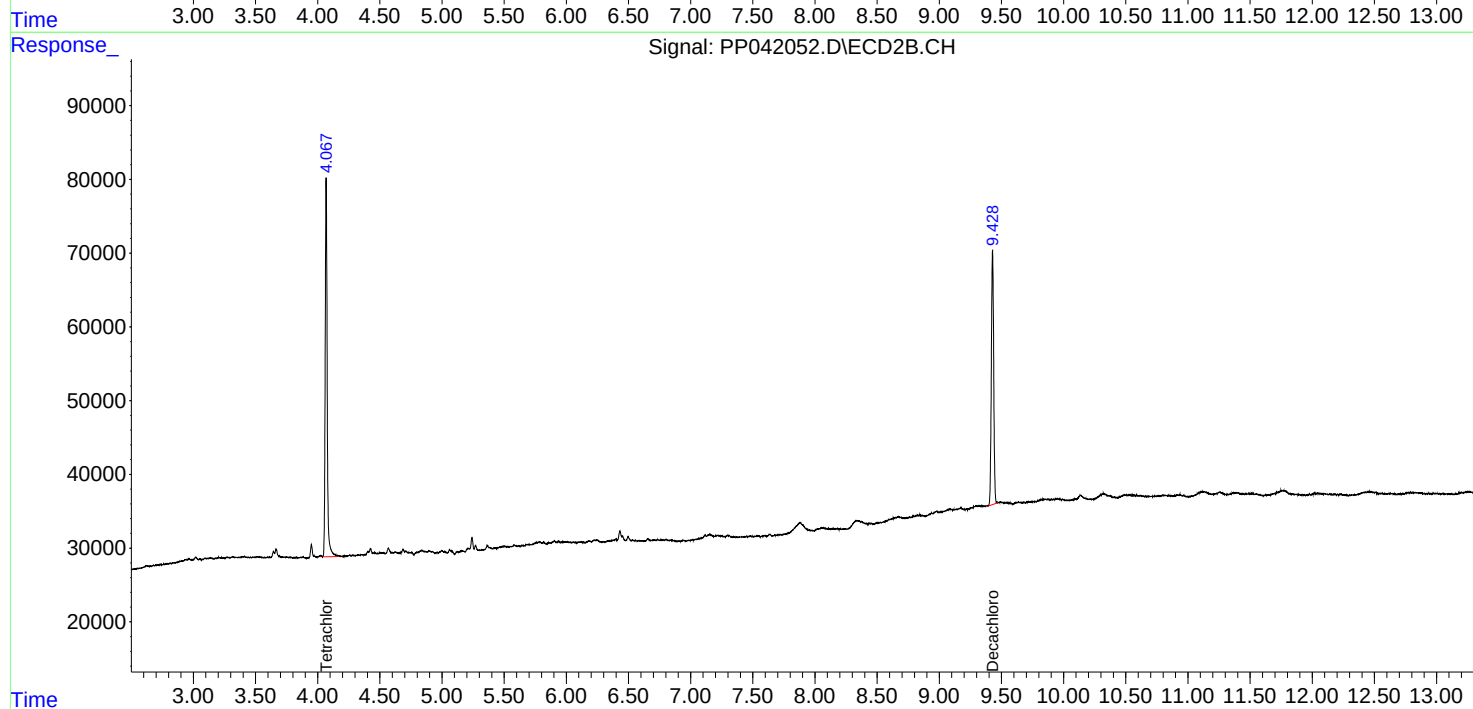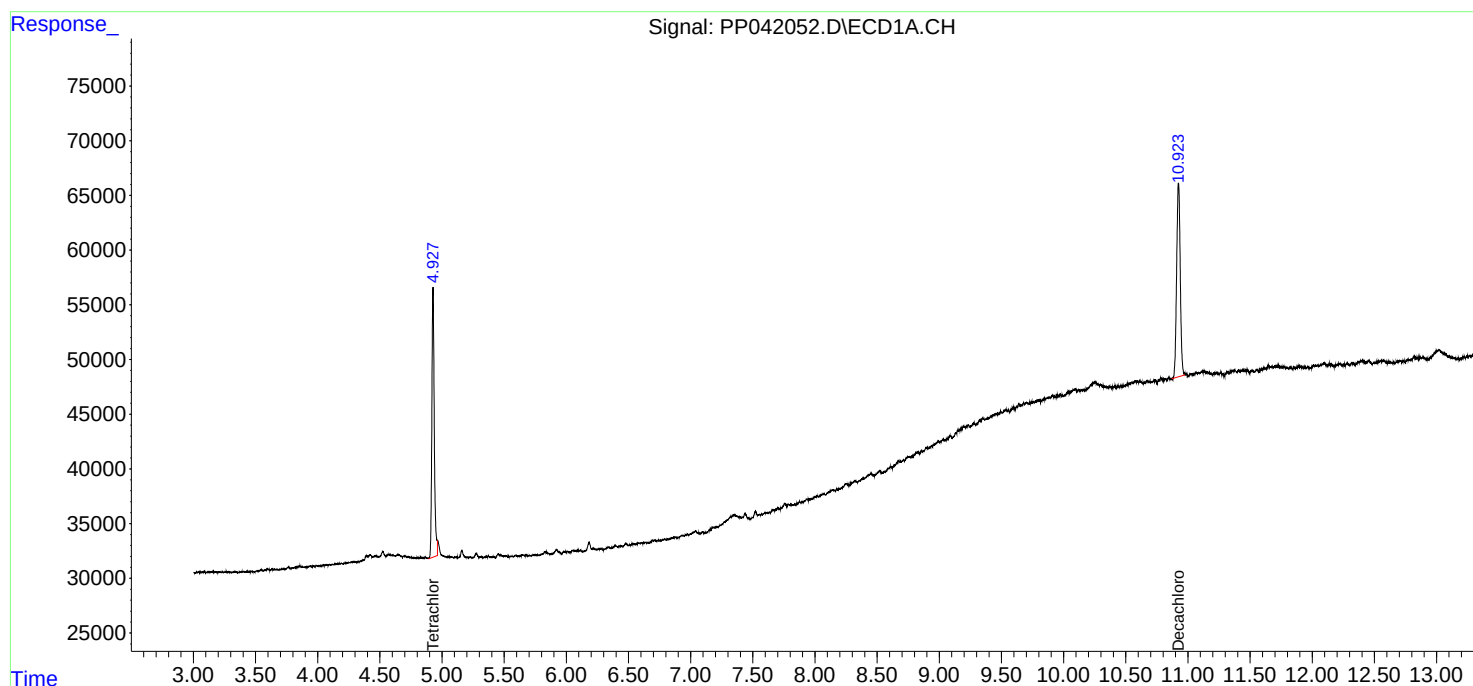

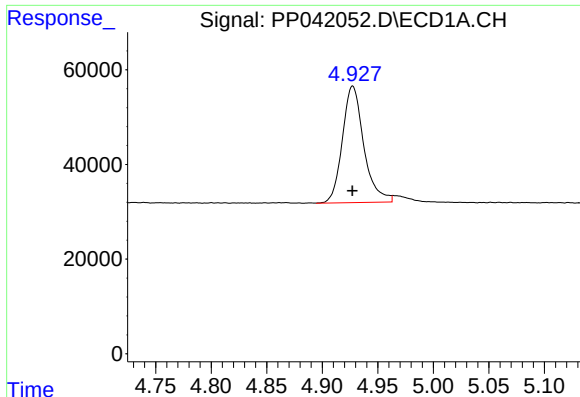


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 331296
Conc: 25.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-PAD


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/17/2021
Supervised By :mohammad ahmed 12/17/2021

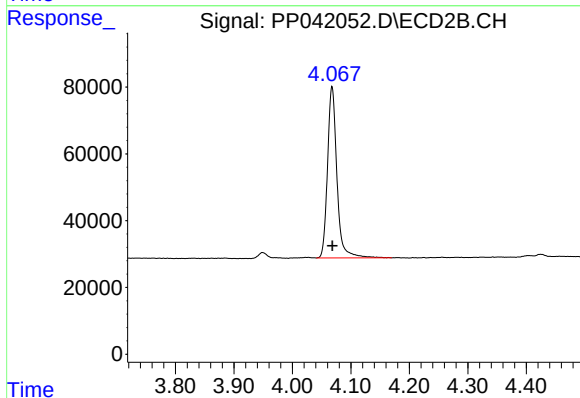


#1 Tetrachloro-m-xylene

R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 575387
Conc: 23.45 ng/ml

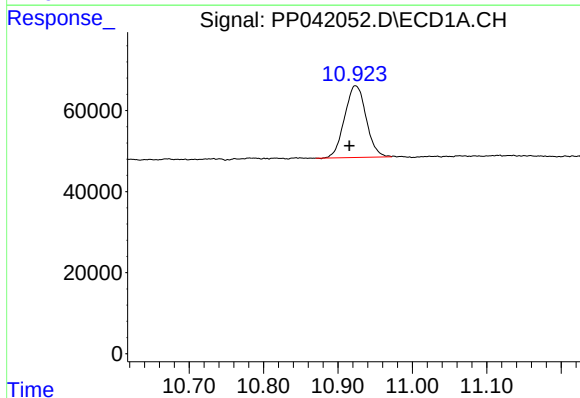

#2 Decachlorobiphenyl

R.T.: 10.923 min
Delta R.T.: 0.008 min
Response: 355618
Conc: 26.99 ng/ml

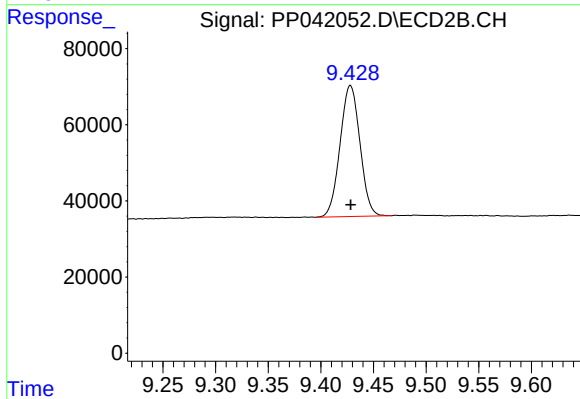

#2 Decachlorobiphenyl

R.T.: 9.428 min
Delta R.T.: 0.000 min
Response: 452484
Conc: 22.50 ng/ml