

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121721\
 Data File : PP042060.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2021 21:13
 Operator : AJ\MA
 Sample : M5082-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SASP2-121-1(65-77.7)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 03:45:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 06:21:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.928	4.068	279928	482315	21.696	19.660
2)	SA Decachlor...	10.924	9.427	239267	330537	18.156	16.440

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121721\
Data File : PP042060.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2021 21:13
Operator : AJ\MA
Sample : M5082-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SASP2-121-1(65-77.7)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 03:45:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 06:21:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

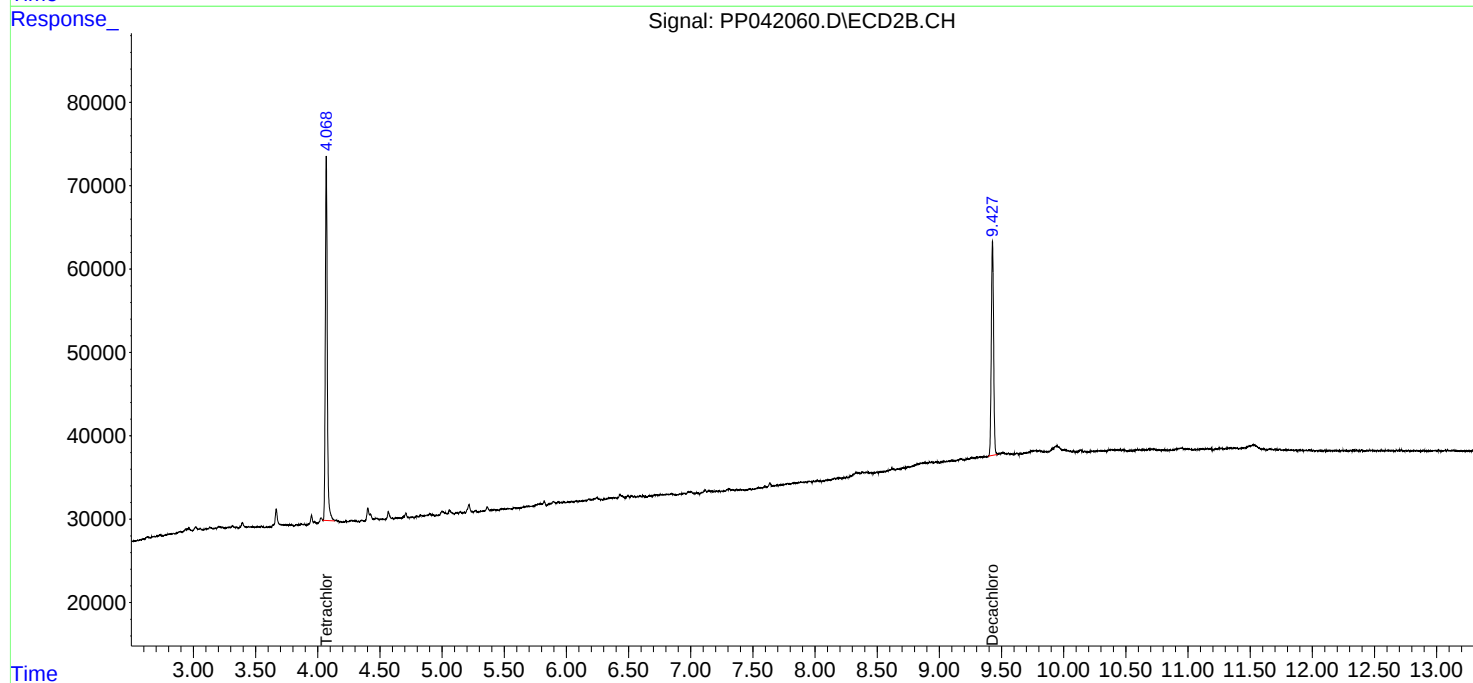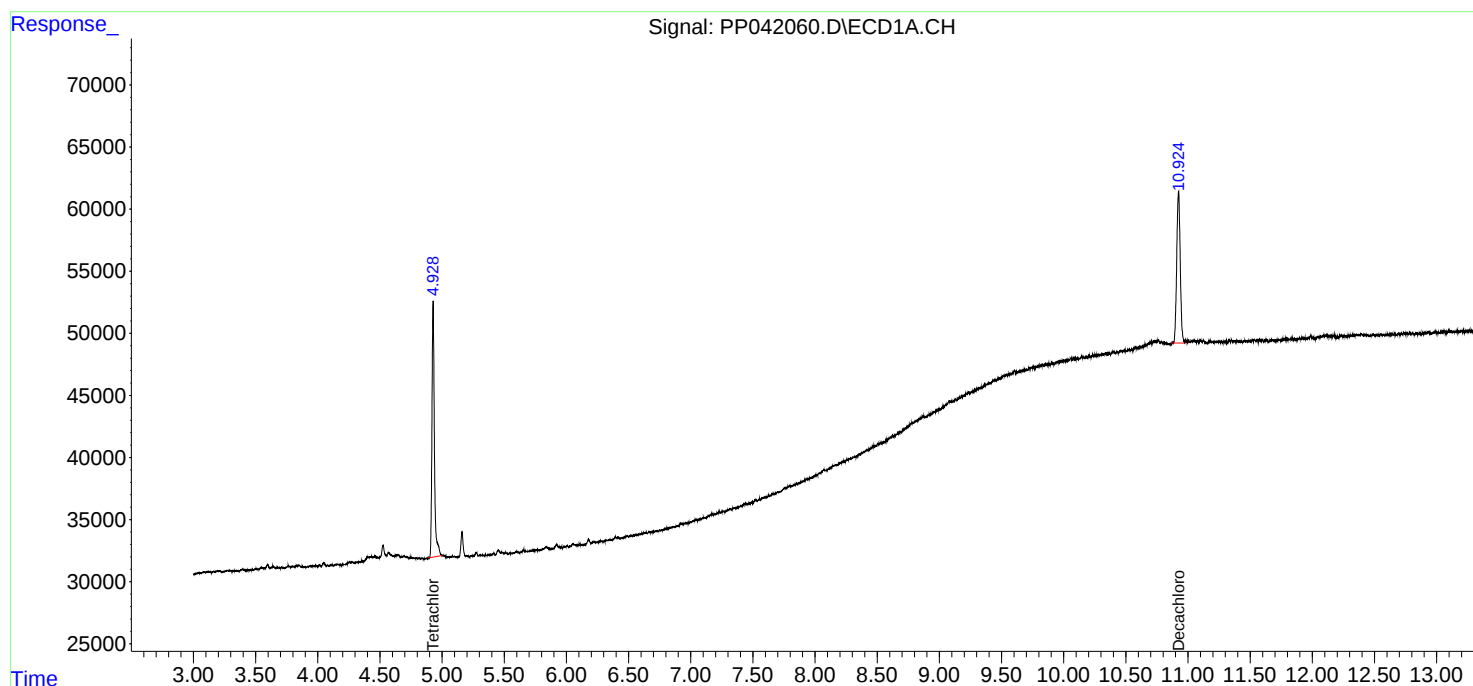


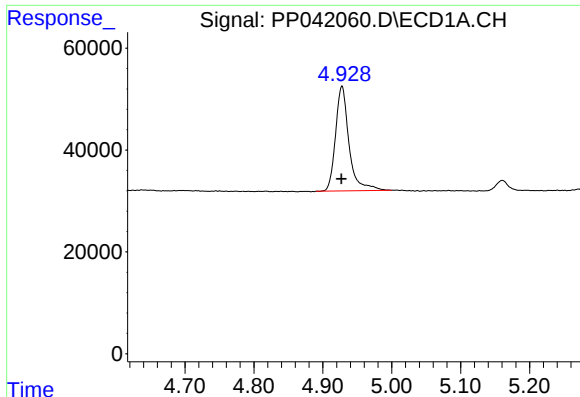

#1 Tetrachloro-m-xylene


R.T.: 4.928 min
Delta R.T.: 0.000 min
Response: 279928
Conc: 21.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
SASP2-121-1(65-77.7)

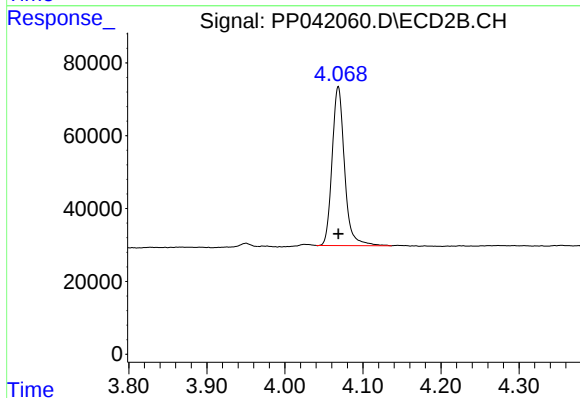


#1 Tetrachloro-m-xylene

R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 482315
Conc: 19.66 ng/ml

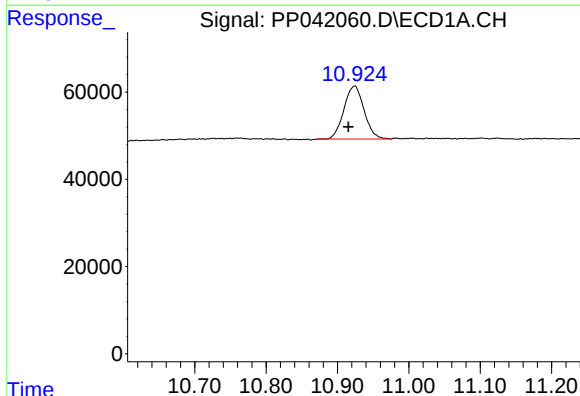

#2 Decachlorobiphenyl

R.T.: 10.924 min
Delta R.T.: 0.009 min
Response: 239267
Conc: 18.16 ng/ml

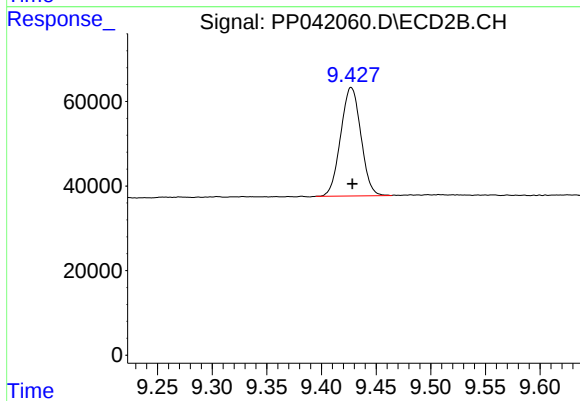

#2 Decachlorobiphenyl

R.T.: 9.427 min
Delta R.T.: -0.001 min
Response: 330537
Conc: 16.44 ng/ml