

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121823\
 Data File : PP062484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2023 14:24
 Operator : YP\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/19/2023
 Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 14:38:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 18 14:38:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.689	9963608	15954199	4.956	4.653
2) SA Decachlor...	10.159	8.801	6431488	12088763	4.832	5.104
Target Compounds						
21) L5 AR-1248-1	5.577	4.799	1908907	3491808	50.727	52.997
22) L5 AR-1248-2	5.851	5.041	3083158	5148410	52.332	53.452
23) L5 AR-1248-3	6.056	5.084	3452521	5445780	52.587	53.710
24) L5 AR-1248-4	6.462	5.258	3363935	6531196	50.127	54.447m
25) L5 AR-1248-5	6.501	5.659	3341941	5923638	50.907	54.693

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121823\
Data File : PP062484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2023 14:24
Operator : YP\AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 14:38:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 18 14:38:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

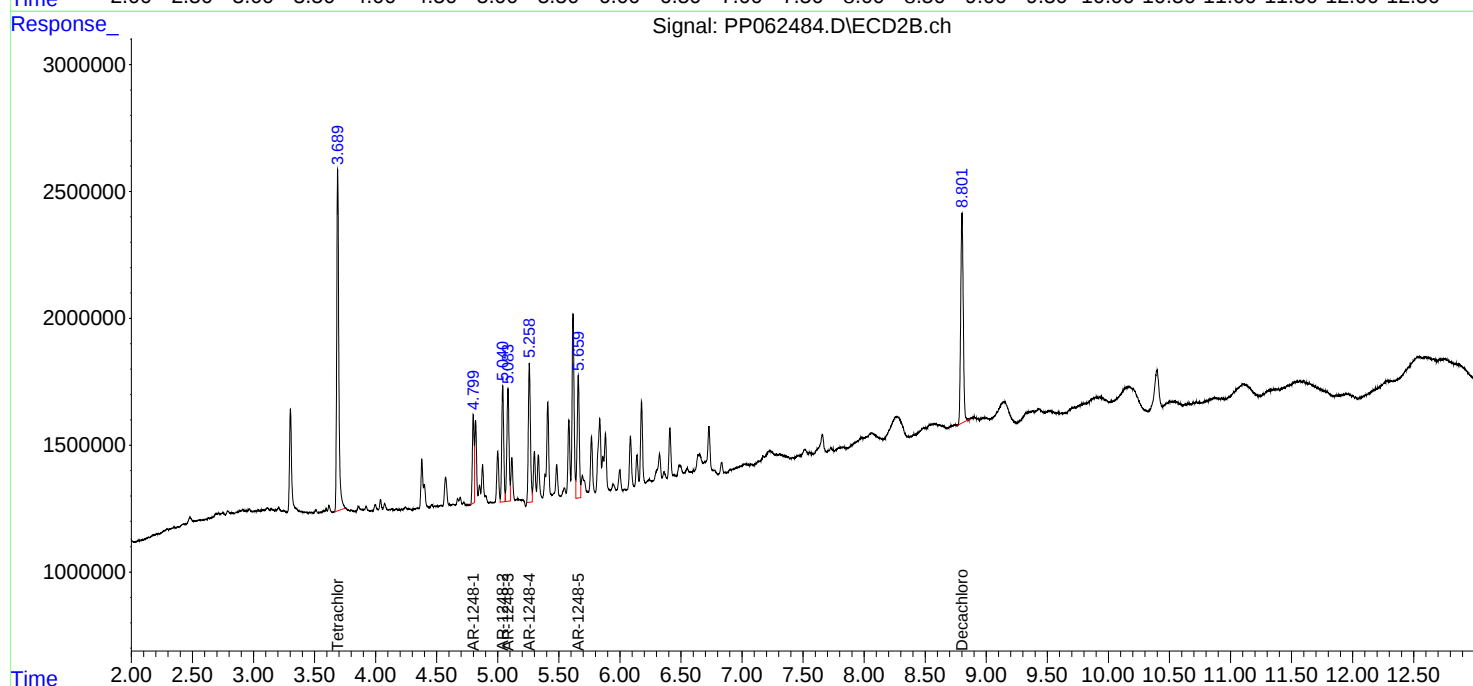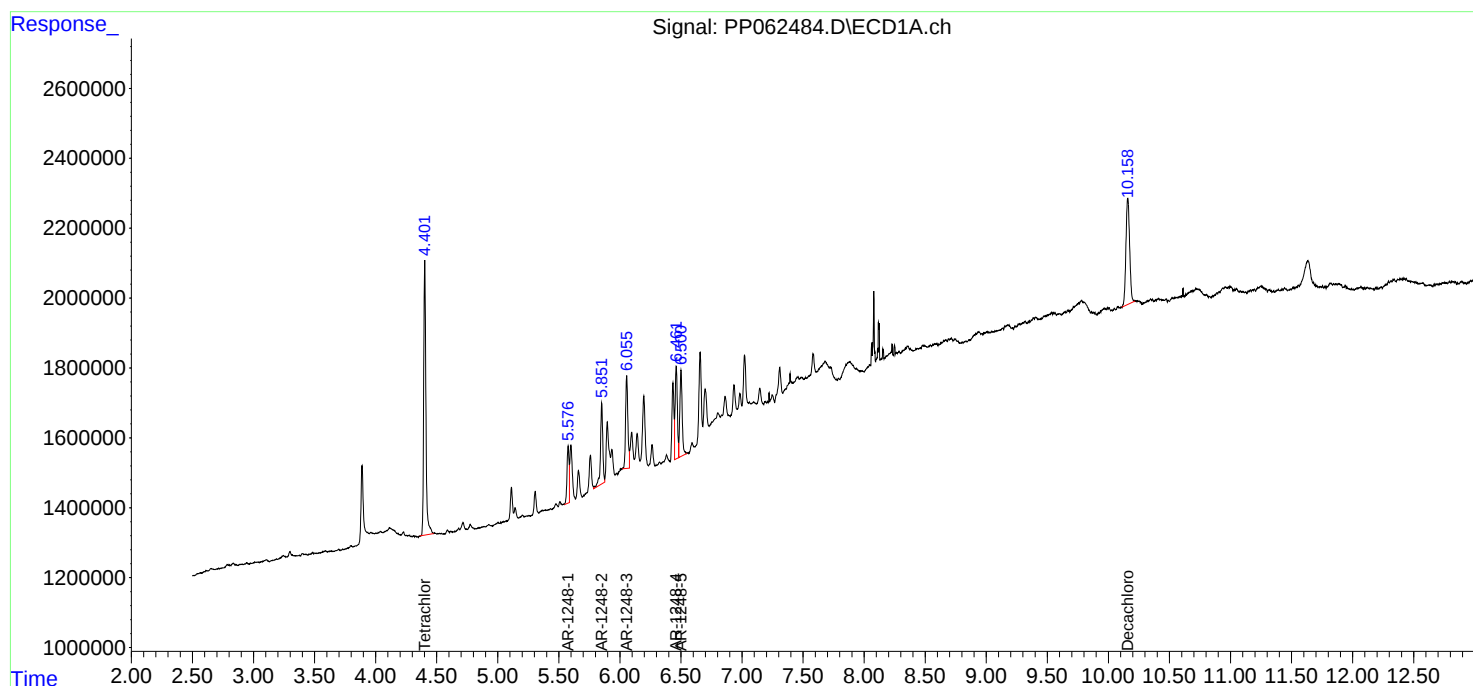

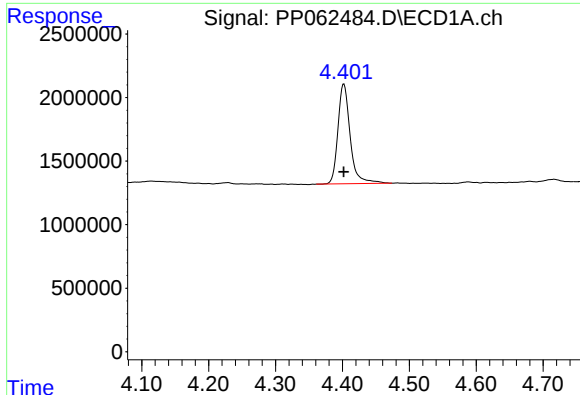


#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: 0.000 min
Response: 9963608
Conc: 4.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

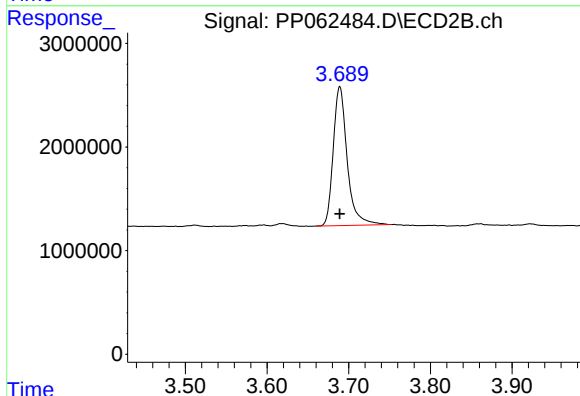


#1 Tetrachloro-m-xylene

R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 15954199
Conc: 4.65 ng/ml

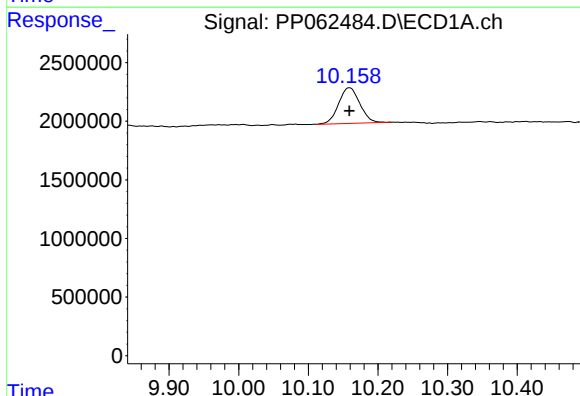


#2 Decachlorobiphenyl

R.T.: 10.159 min
Delta R.T.: 0.000 min
Response: 6431488
Conc: 4.83 ng/ml

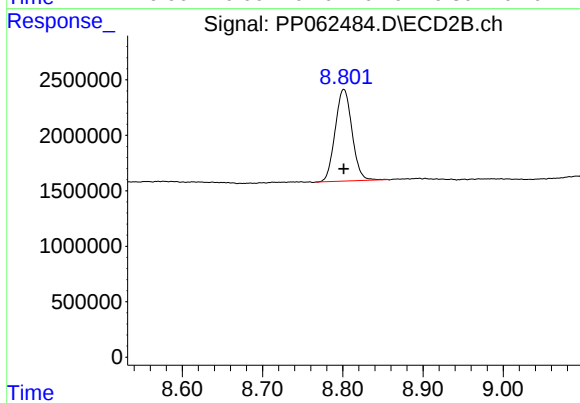

#2 Decachlorobiphenyl

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 12088763
Conc: 5.10 ng/ml

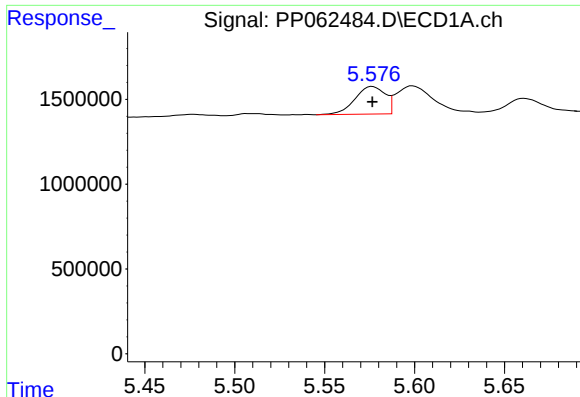


#21 AR-1248-1

R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 1908907
Conc: 50.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

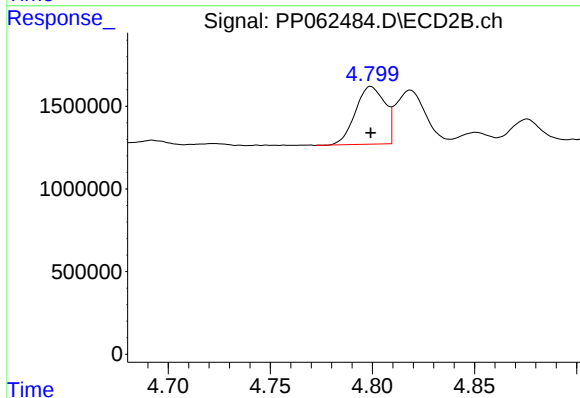


#21 AR-1248-1

R.T.: 4.799 min
Delta R.T.: 0.000 min
Response: 3491808
Conc: 53.00 ng/ml

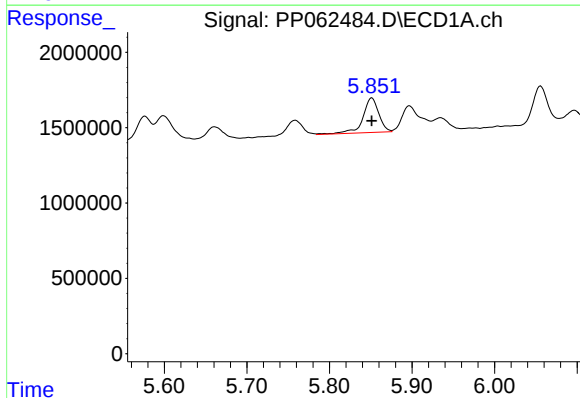


#22 AR-1248-2

R.T.: 5.851 min
Delta R.T.: 0.000 min
Response: 3083158
Conc: 52.33 ng/ml

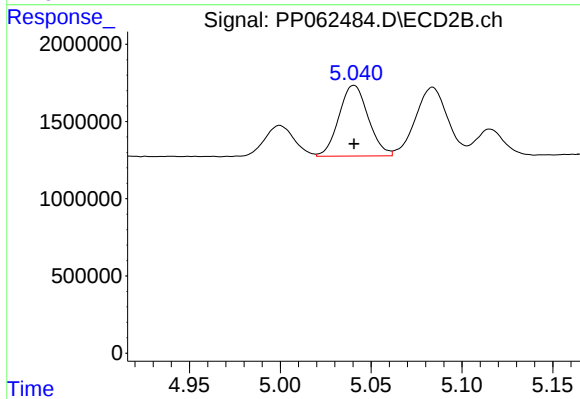

#22 AR-1248-2

R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 5148410
Conc: 53.45 ng/ml

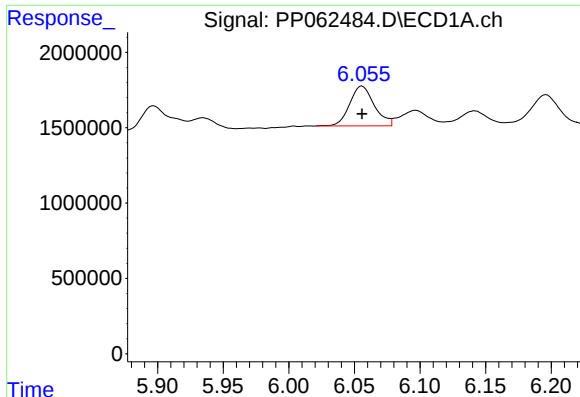


#23 AR-1248-3

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 3452521
Conc: 52.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

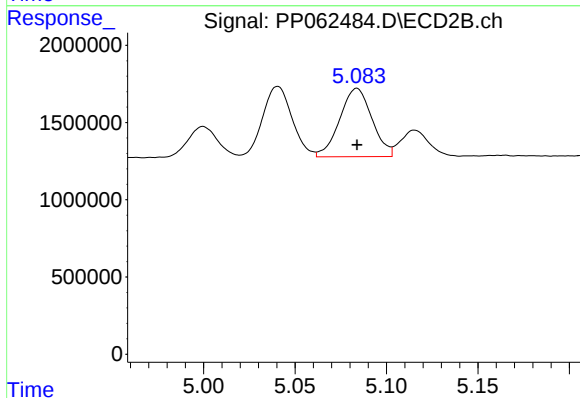


#23 AR-1248-3

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 5445780
Conc: 53.71 ng/ml

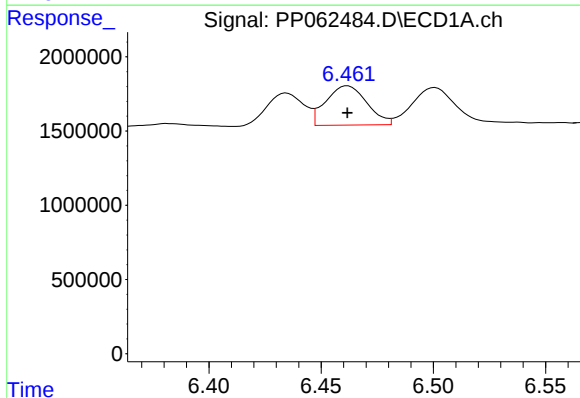


#24 AR-1248-4

R.T.: 6.462 min
Delta R.T.: 0.000 min
Response: 3363935
Conc: 50.13 ng/ml

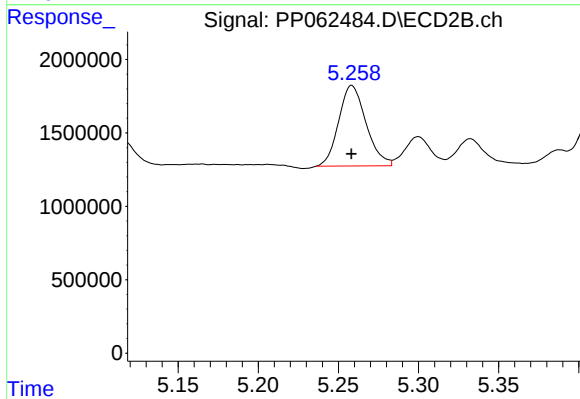

#24 AR-1248-4

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 6531196
Conc: 54.45 ng/ml m

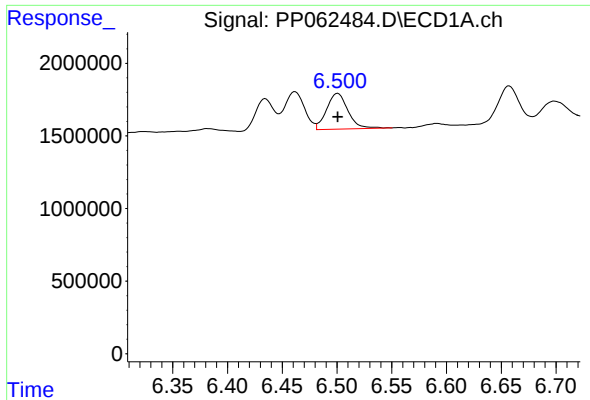


#25 AR-1248-5

R.T.: 6.501 min
Delta R.T.: 0.000 min
Response: 3341941
Conc: 50.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

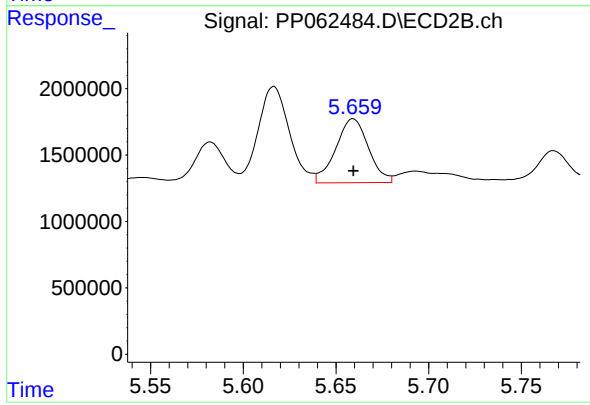

#25 AR-1248-5

R.T.: 5.659 min
Delta R.T.: 0.000 min
Response: 5923638
Conc: 54.69 ng/ml