

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121823\
 Data File : PP062489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2023 15:45
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/19/2023
 Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 16:00:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 18 16:00:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.689	10395034	16706040	5.055	4.754
2) SA Decachlor...	10.157	8.800	6462870	12688093	4.750	5.180
Target Compounds						
26) L6 AR-1254-1	6.434	5.617	3910278	9645402	52.201	54.383
27) L6 AR-1254-2	6.653	5.766	5937791	8508818	52.227m	55.091
28) L6 AR-1254-3	7.020	6.177	5676566	12871617	48.662m	53.346
29) L6 AR-1254-4	7.307	6.409	3469646	6826503	46.212m	52.378
30) L6 AR-1254-5	7.726	6.832	3425311	10257618	43.472m	51.182

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121823\
Data File : PP062489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2023 15:45
Operator : YP\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 16:00:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 18 16:00:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

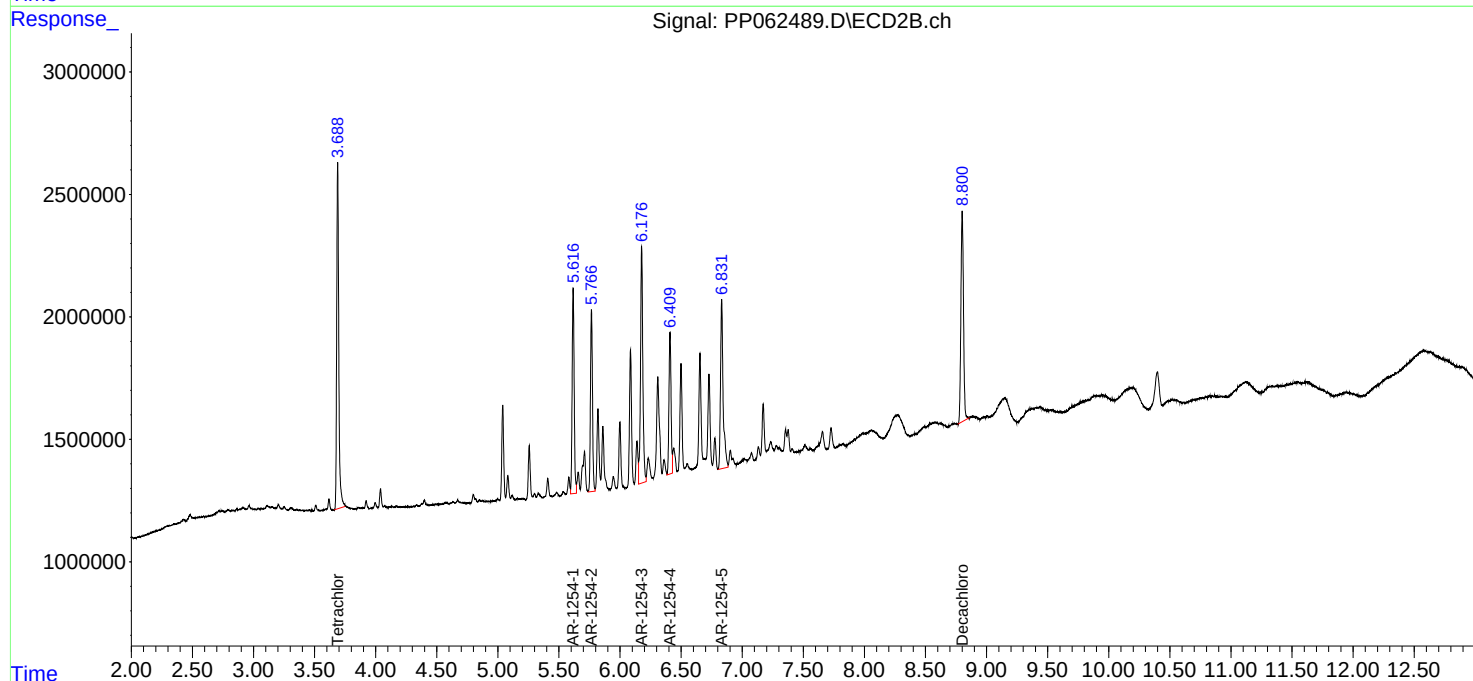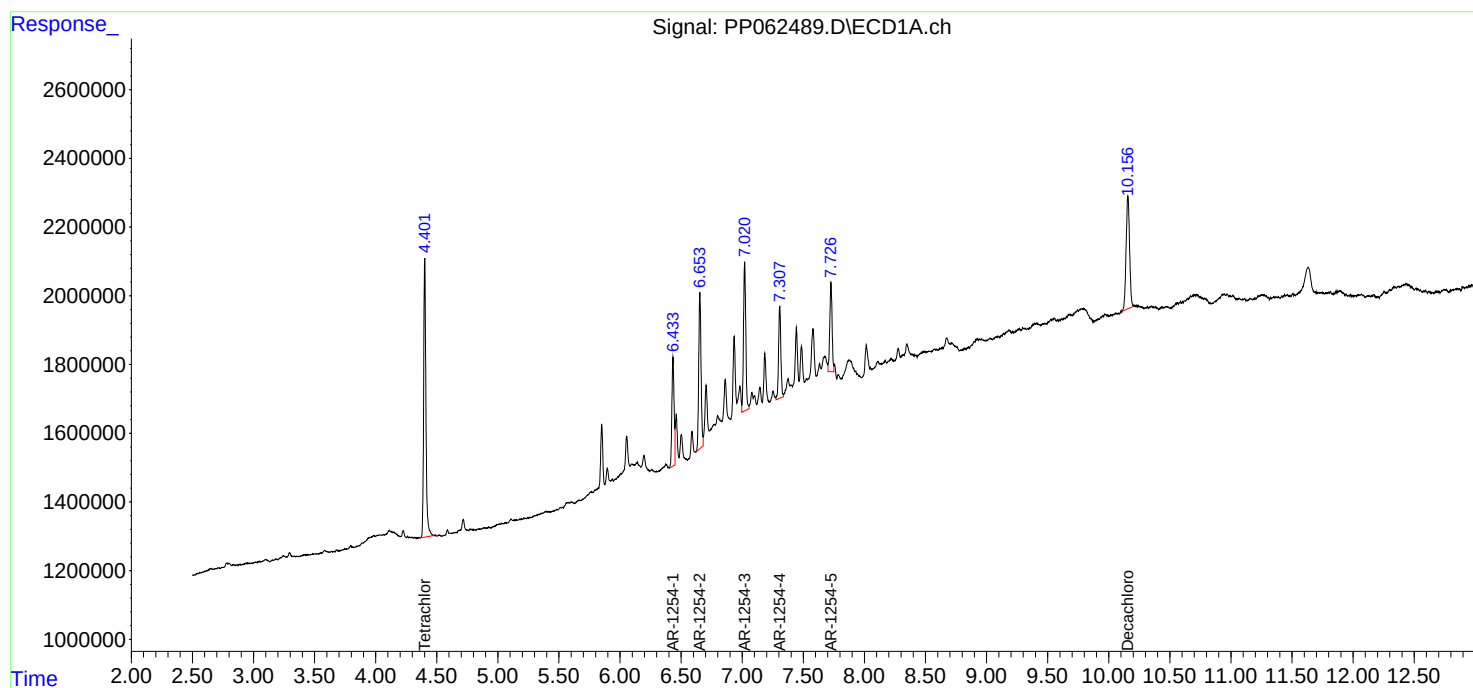

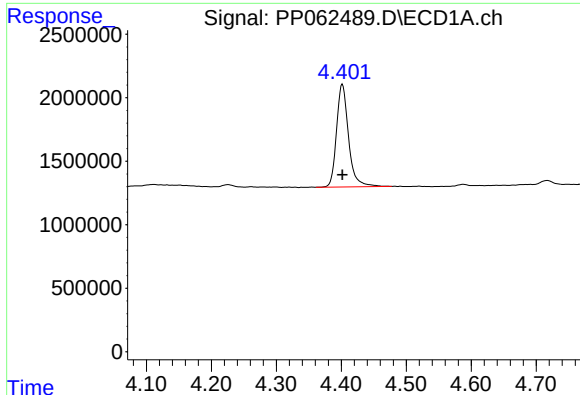


#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: 0.000 min
Response: 10395034
Conc: 5.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

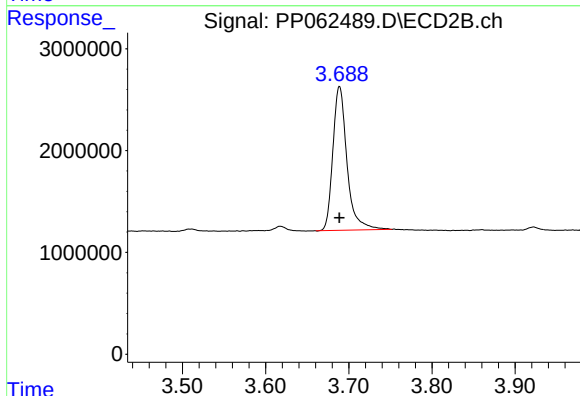


#1 Tetrachloro-m-xylene

R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 16706040
Conc: 4.75 ng/ml

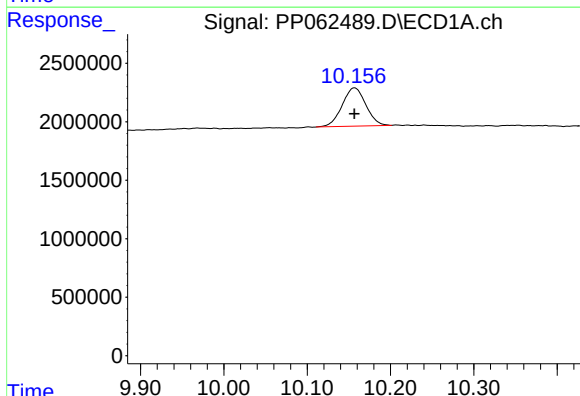


#2 Decachlorobiphenyl

R.T.: 10.157 min
Delta R.T.: 0.000 min
Response: 6462870
Conc: 4.75 ng/ml

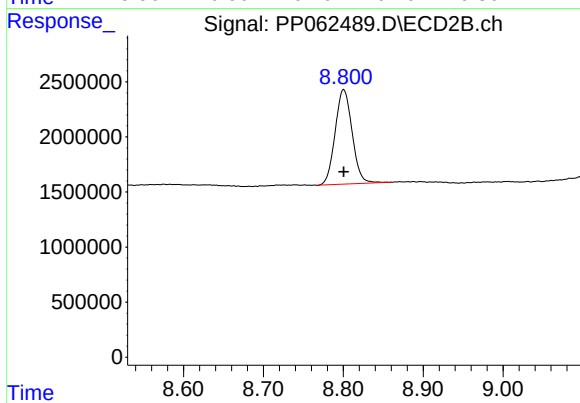

#2 Decachlorobiphenyl

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 12688093
Conc: 5.18 ng/ml

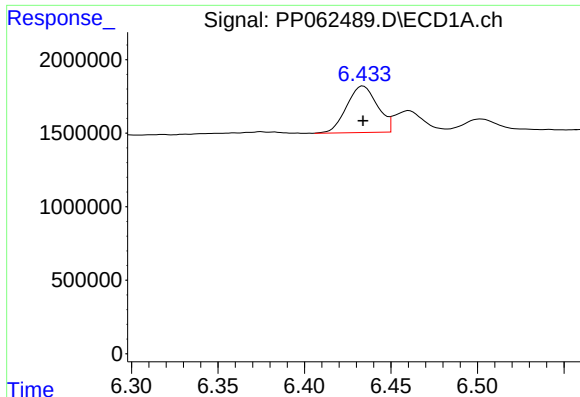


#26 AR-1254-1

R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 3910278
Conc: 52.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

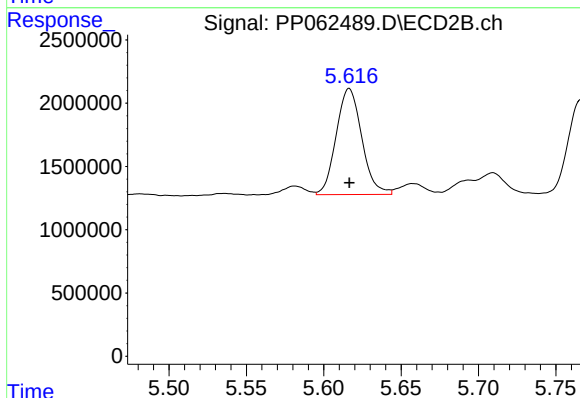


#26 AR-1254-1

R.T.: 5.617 min
Delta R.T.: 0.000 min
Response: 9645402
Conc: 54.38 ng/ml

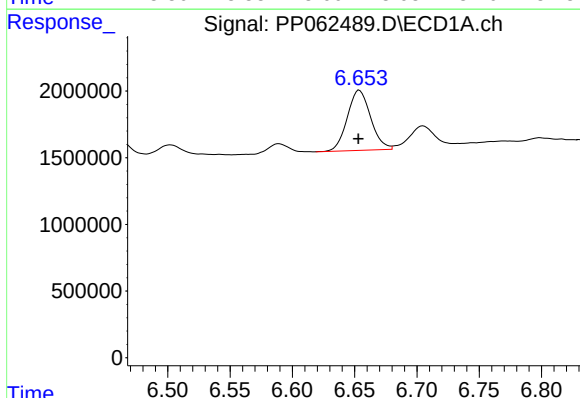


#27 AR-1254-2

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 5937791
Conc: 52.23 ng/ml m

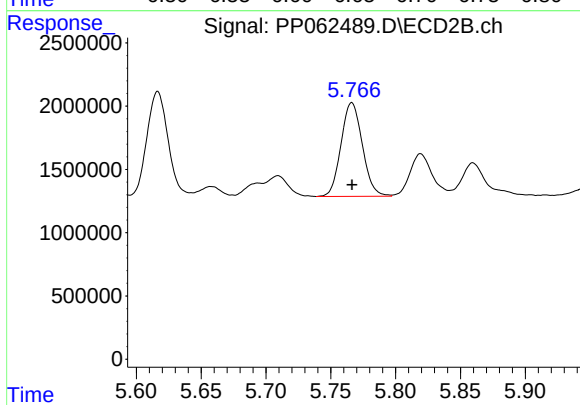

#27 AR-1254-2

R.T.: 5.766 min
Delta R.T.: 0.000 min
Response: 8508818
Conc: 55.09 ng/ml

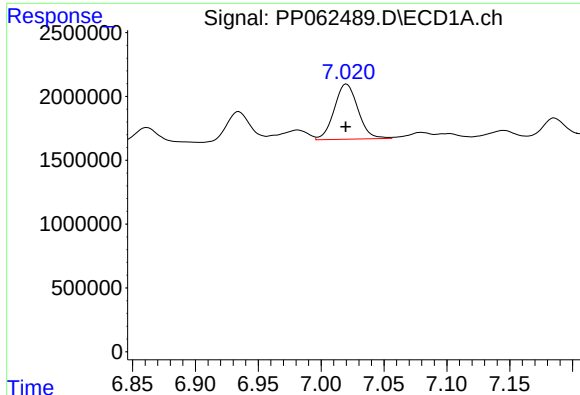


#28 AR-1254-3

R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 5676566
Conc: 48.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

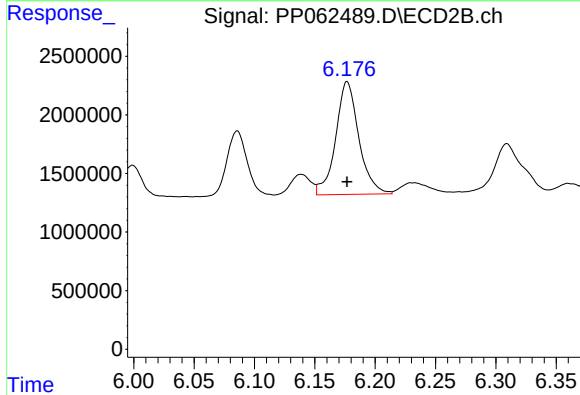


#28 AR-1254-3

R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 12871617
Conc: 53.35 ng/ml

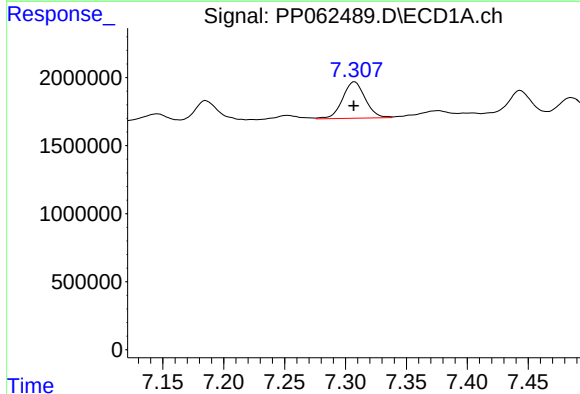


#29 AR-1254-4

R.T.: 7.307 min
Delta R.T.: 0.000 min
Response: 3469646
Conc: 46.21 ng/ml m

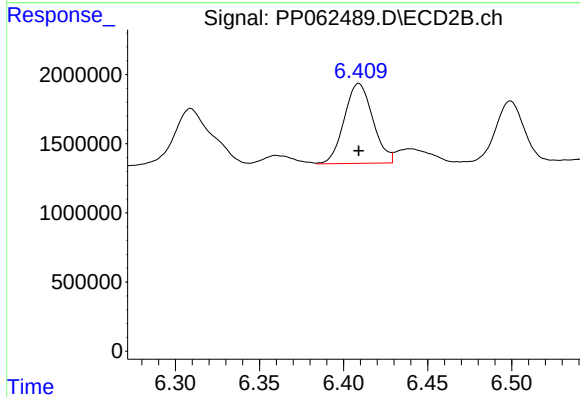

#29 AR-1254-4

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 6826503
Conc: 52.38 ng/ml

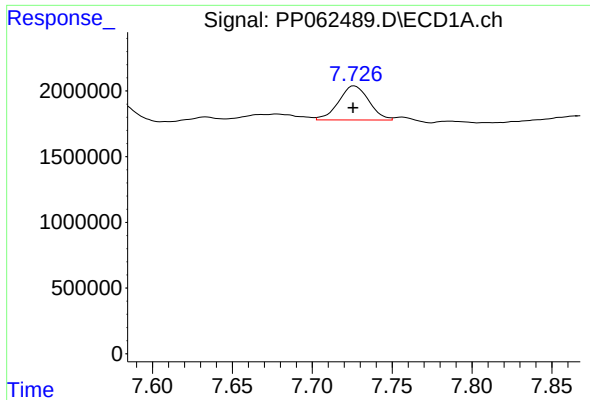


#30 AR-1254-5

R.T.: 7.726 min
Delta R.T.: 0.000 min
Response: 3425311
Conc: 43.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

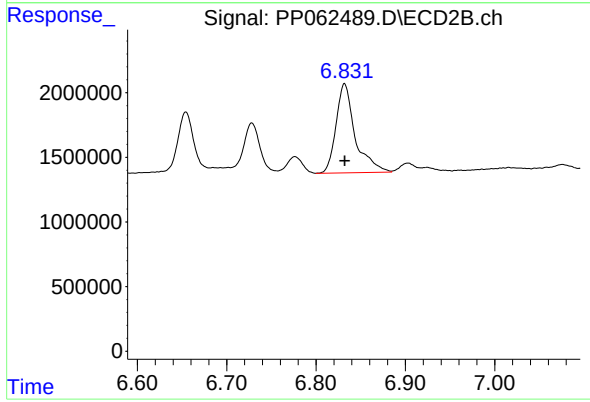

#30 AR-1254-5

R.T.: 6.832 min
Delta R.T.: 0.000 min
Response: 10257618
Conc: 51.18 ng/ml