

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121922\
 Data File : PP053839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2022 17:46
 Operator : YP\AJ
 Sample : N6098-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FVSUB-TP6-COMP-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 03:24:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 14 05:38:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.339	3.591	41756512	30251306	19.886	19.370
2)	SA Decachlor...	10.100	8.627	25482221	20894069	15.009	14.959

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121922\
Data File : PP053839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2022 17:46
Operator : YP\AJ
Sample : N6098-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FVSUB-TP6-COMP-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 03:24:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 14 05:38:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

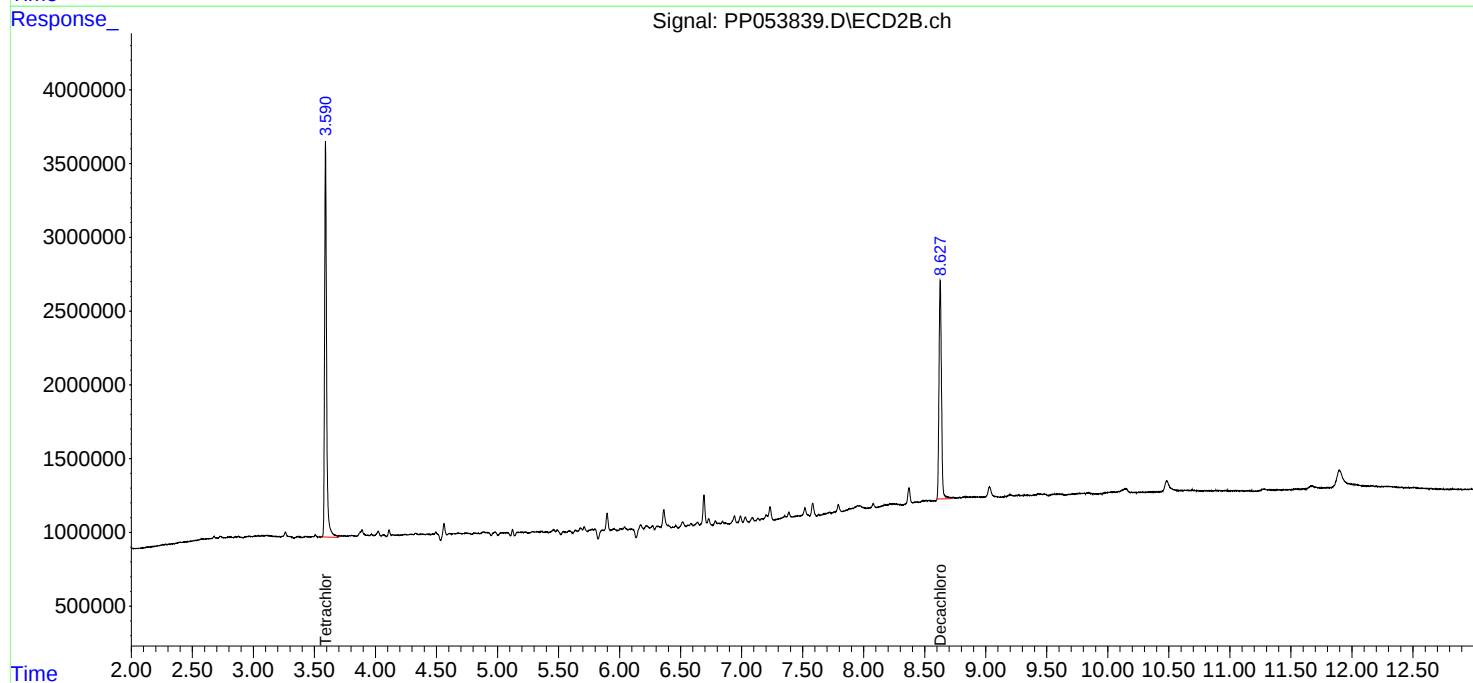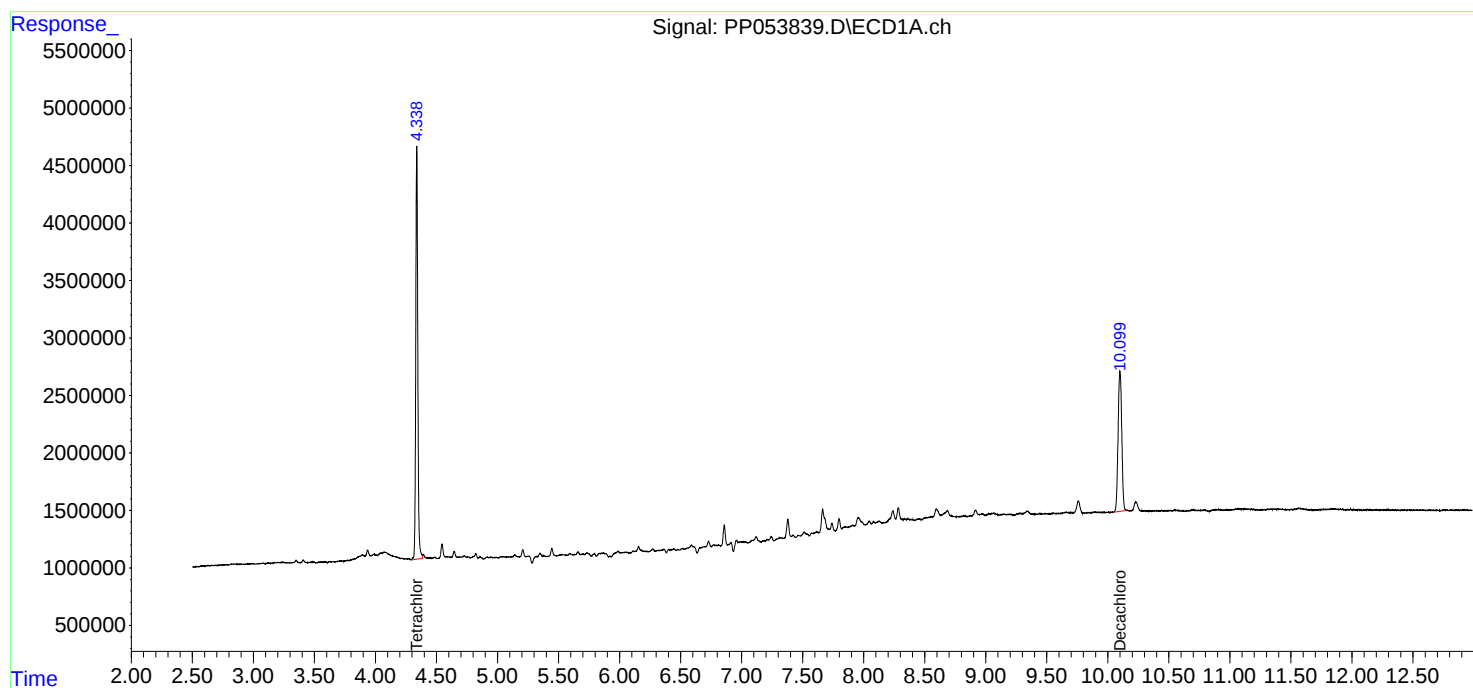


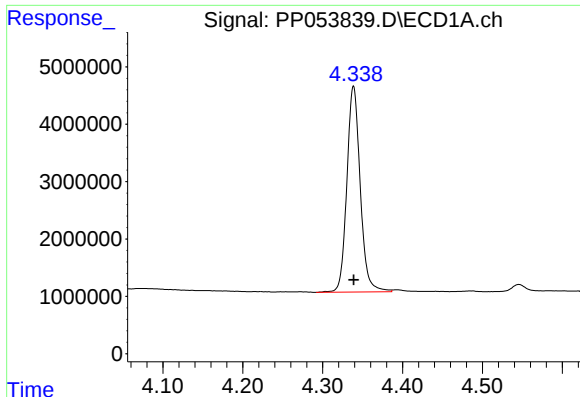

#1 Tetrachloro-m-xylene


R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 41756512
Conc: 19.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
FVSUB-TP6-COMP-06

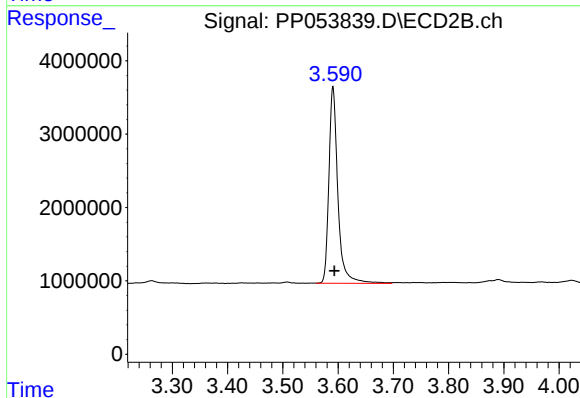


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.003 min
Response: 30251306
Conc: 19.37 ng/ml

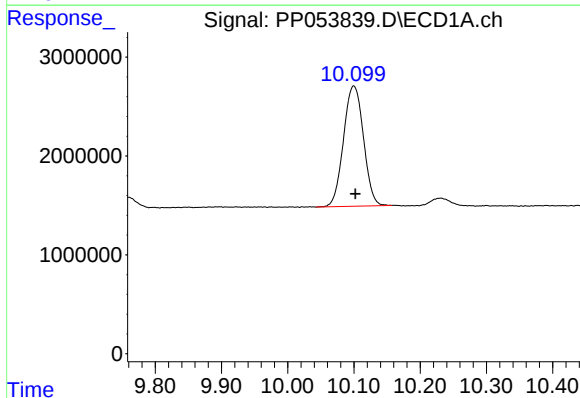

#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: -0.002 min
Response: 25482221
Conc: 15.01 ng/ml

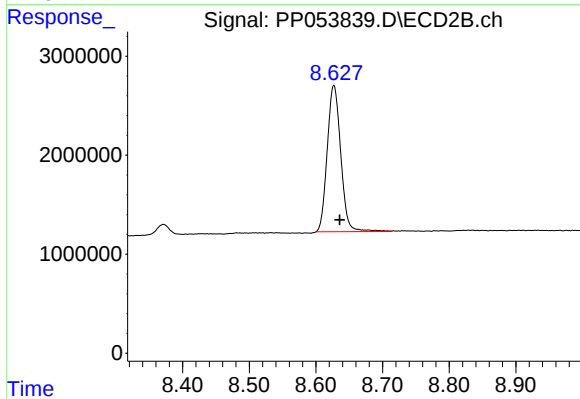

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.009 min
Response: 20894069
Conc: 14.96 ng/ml