

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121923\
 Data File : PP062538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2023 20:41
 Operator : YP\AJ
 Sample : 05911-04 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH3861(1-2)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :Ankita Jodhani 12/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 23:43:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 19 06:30:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.685	2753287	4092200	1.353m	1.193m
2) SA Decachlor...	10.141	8.788	3286184	3440916	2.641m	1.536 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121923\
Data File : PP062538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2023 20:41
Operator : YP\AJ
Sample : 05911-04 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH3861I(1-2)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/20/2023
Supervised By :Ankita Jodhani 12/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 23:43:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 19 06:30:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

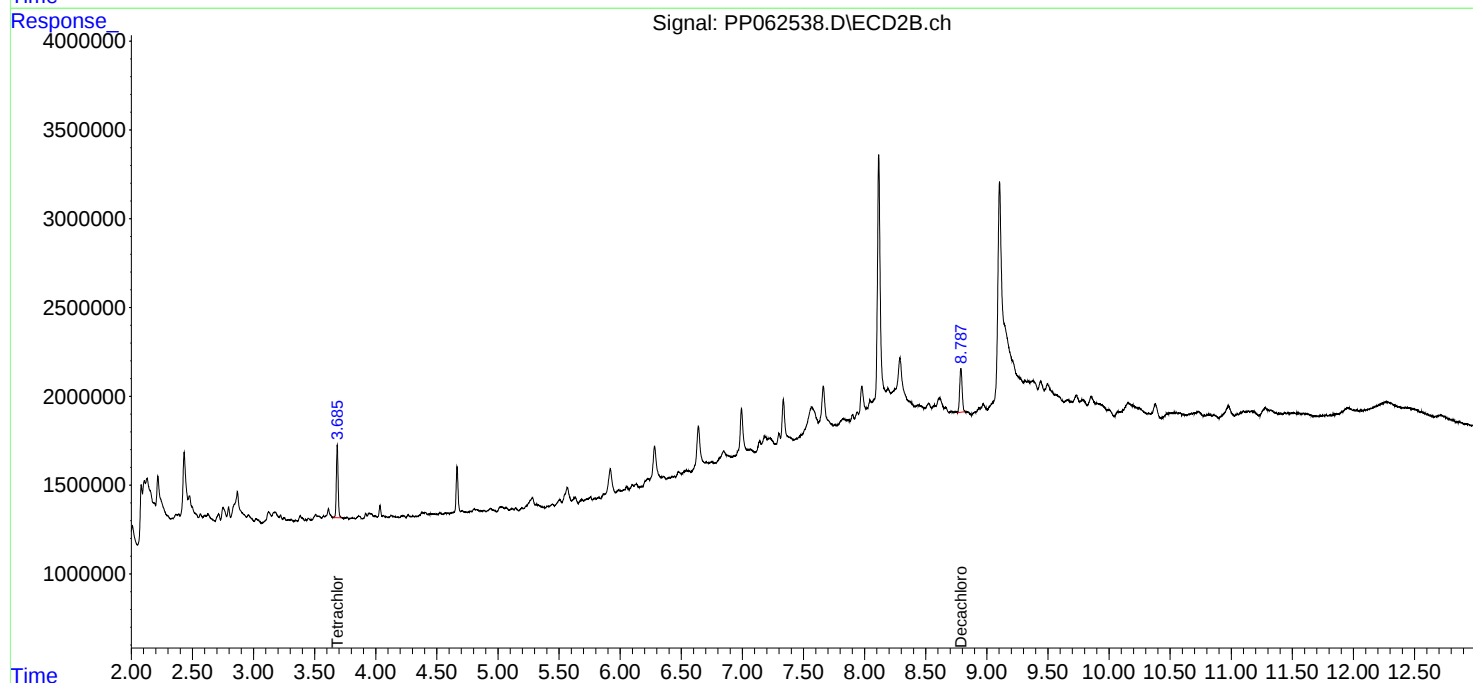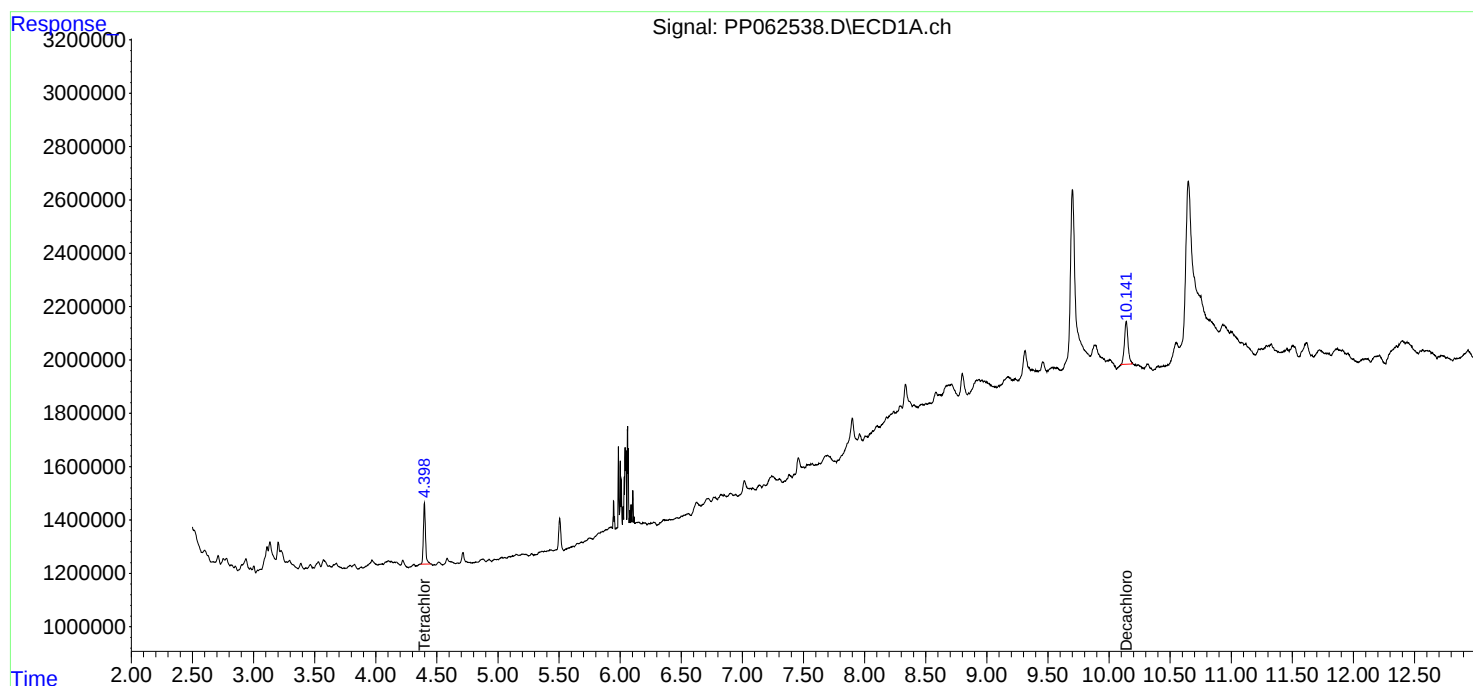

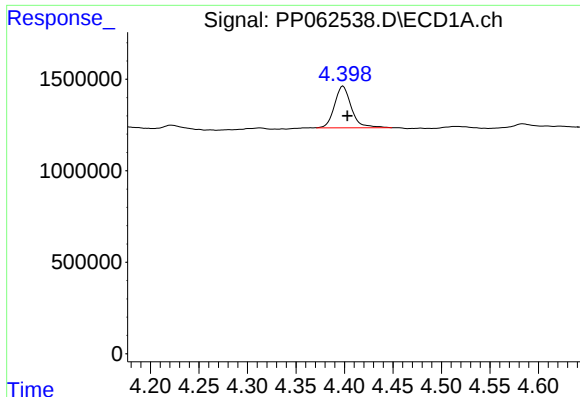


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: -0.005 min
Response: 2753287
Conc: 1.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMH3861I(1-2)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/20/2023
Supervised By :Ankita Jodhani 12/20/2023

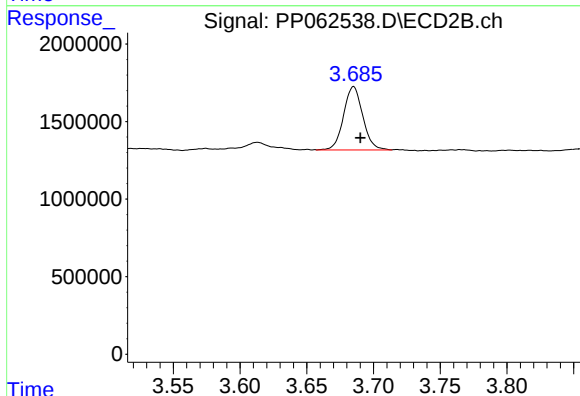


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: -0.005 min
Response: 4092200
Conc: 1.19 ng/ml m

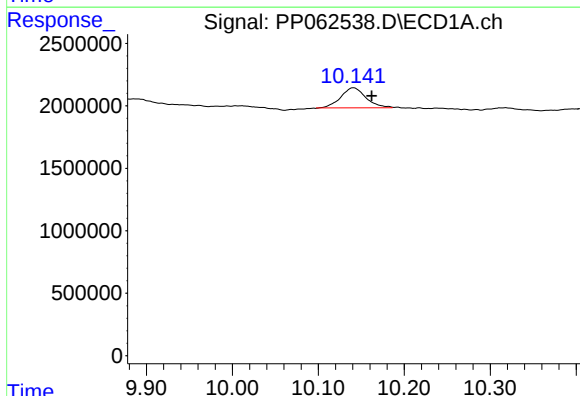

#2 Decachlorobiphenyl

R.T.: 10.141 min
Delta R.T.: -0.021 min
Response: 3286184
Conc: 2.64 ng/ml m

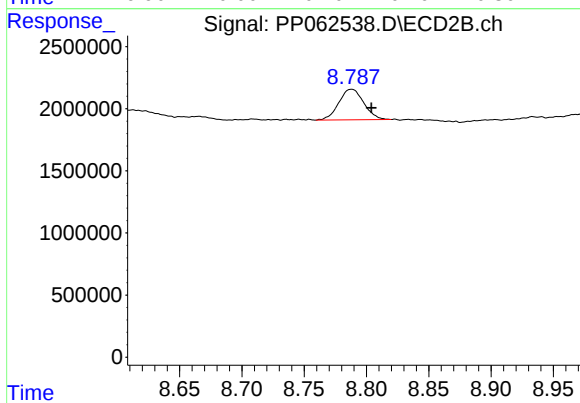

#2 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: -0.016 min
Response: 3440916
Conc: 1.54 ng/ml