

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122022\
 Data File : PP053889.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 17:14
 Operator : YP\AJ
 Sample : N6149-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PARAM-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/21/2022
 Supervised By :Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 20:48:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 14 05:38:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.588	26901434	43796982	12.812	28.044 #
2) SA Decachlor...	10.098	8.623	39205316	32328297	23.092	23.145m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122022\
Data File : PP053889.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 17:14
Operator : YP\AJ
Sample : N6149-02
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PARAM-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 20:48:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 14 05:38:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

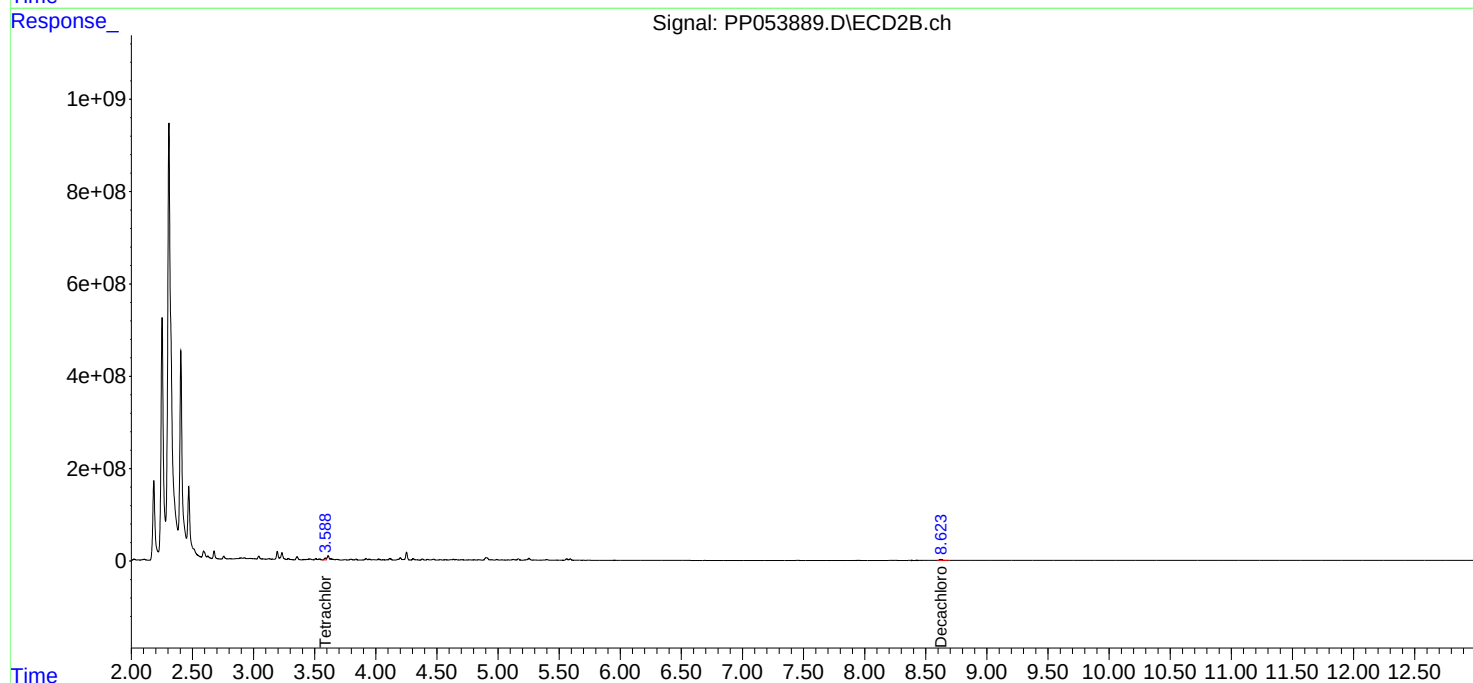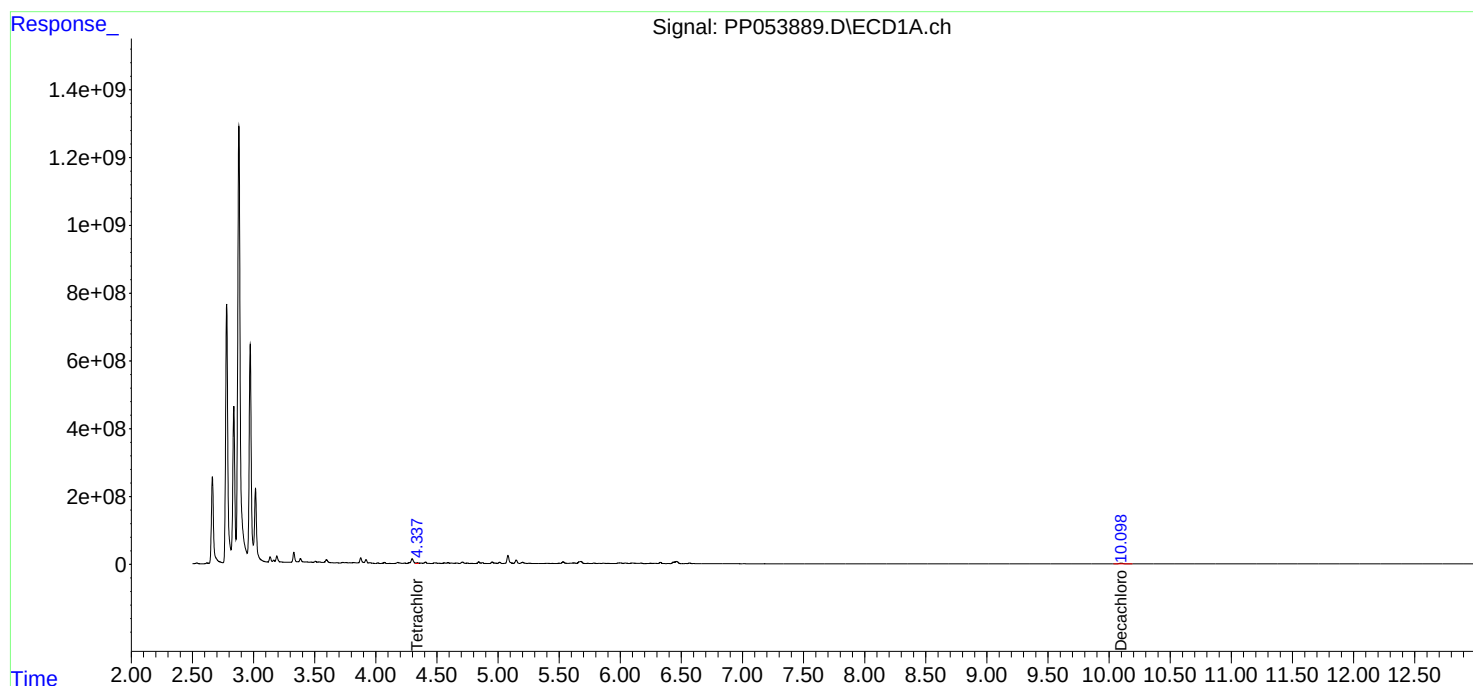

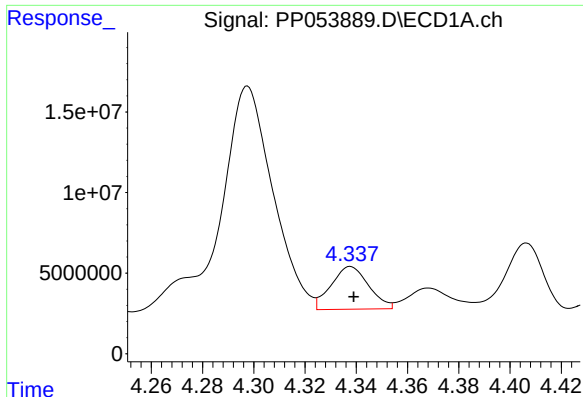


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.001 min
Response: 26901434
Conc: 12.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
PARAM-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

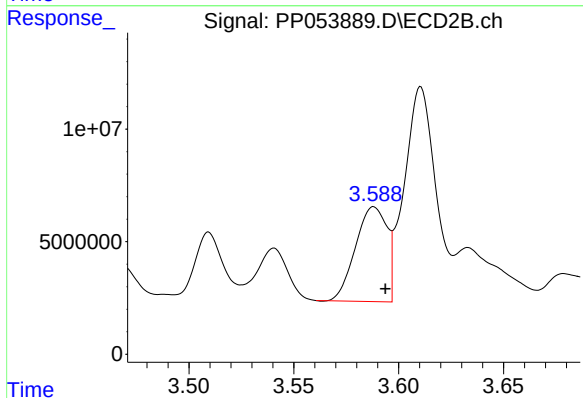


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: -0.005 min
Response: 43796982
Conc: 28.04 ng/ml

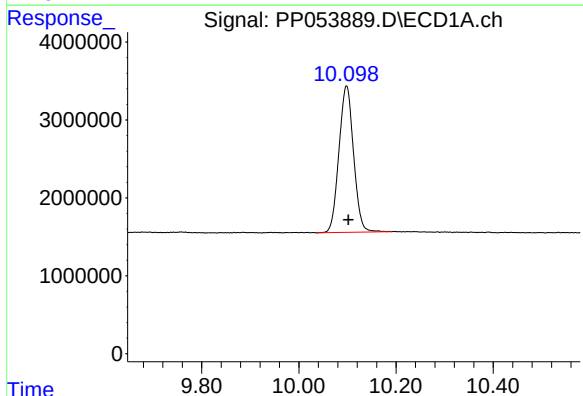

#2 Decachlorobiphenyl

R.T.: 10.098 min
Delta R.T.: -0.004 min
Response: 39205316
Conc: 23.09 ng/ml

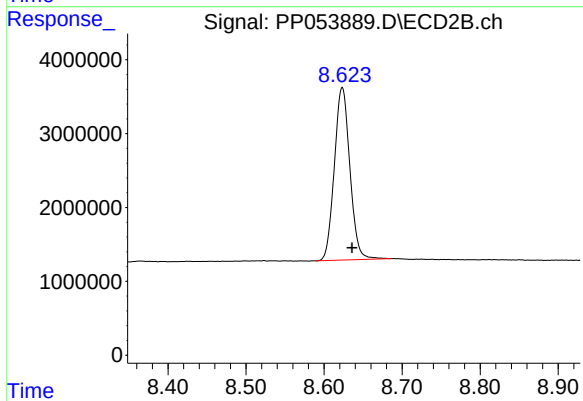

#2 Decachlorobiphenyl

R.T.: 8.623 min
Delta R.T.: -0.013 min
Response: 32328297
Conc: 23.15 ng/ml m