

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122022\
 Data File : PP053897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 19:25
 Operator : YP\AJ
 Sample : N6149-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HAN-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/21/2022
 Supervised By :Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 20:52:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 14 05:38:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.331	3.595	36351997	138.1E6	17.312m	88.400m#
2) SA Decachlor...	10.097	8.622	35049268	28877433	20.644	20.675m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122022\
Data File : PP053897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 19:25
Operator : YP\AJ
Sample : N6149-10
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HAN-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 20:52:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 14 05:38:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

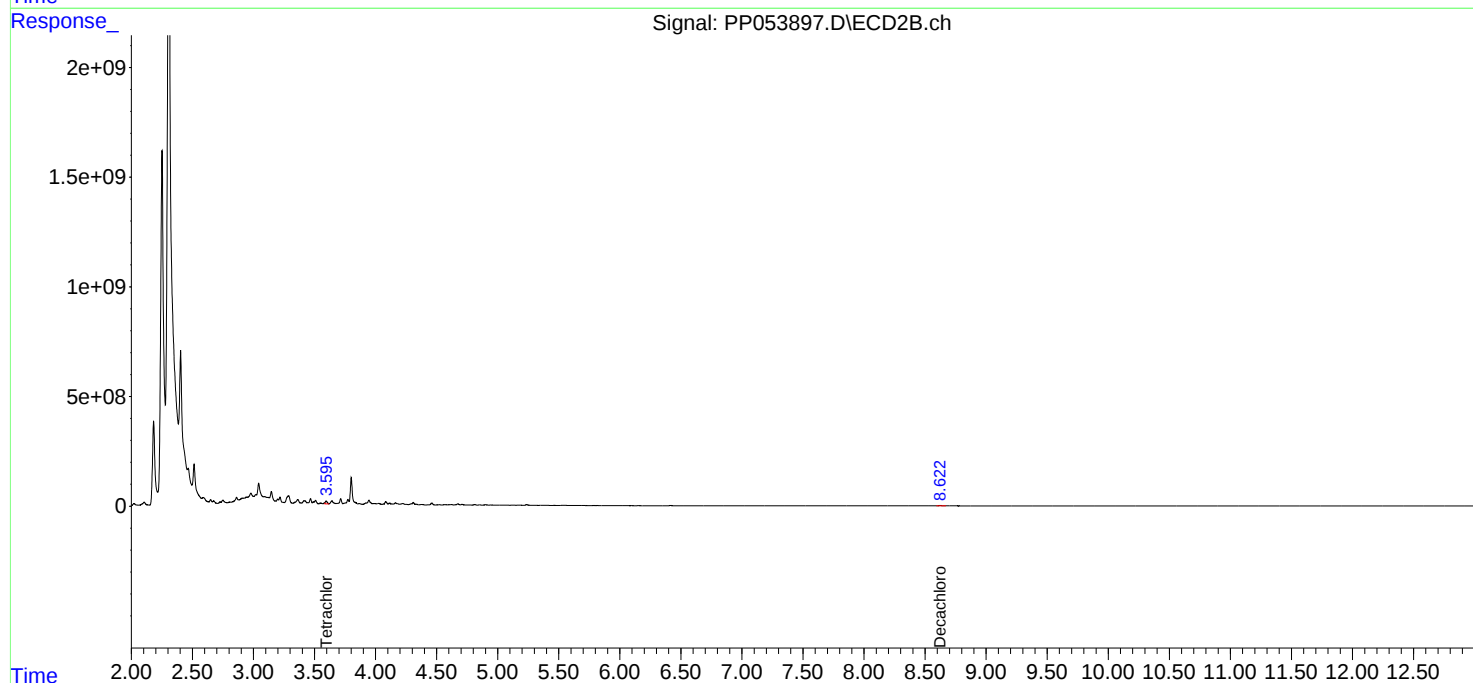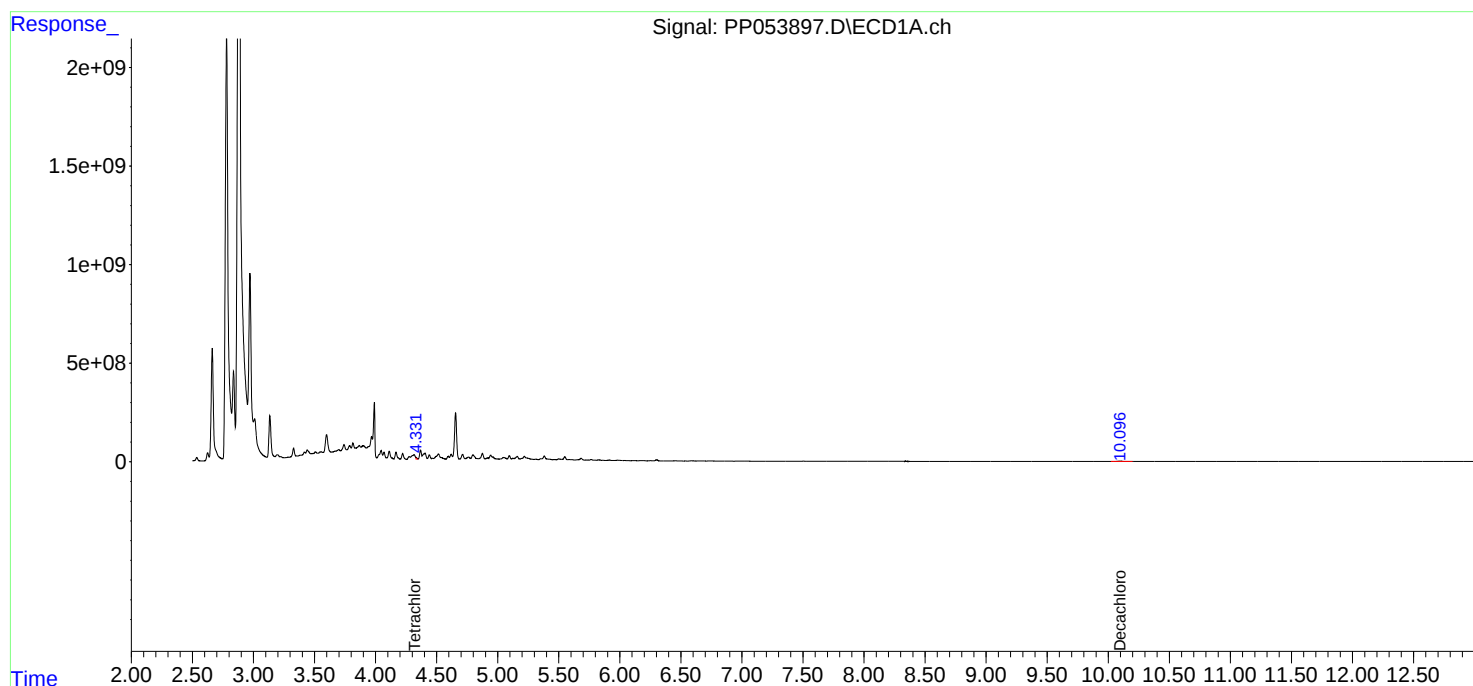

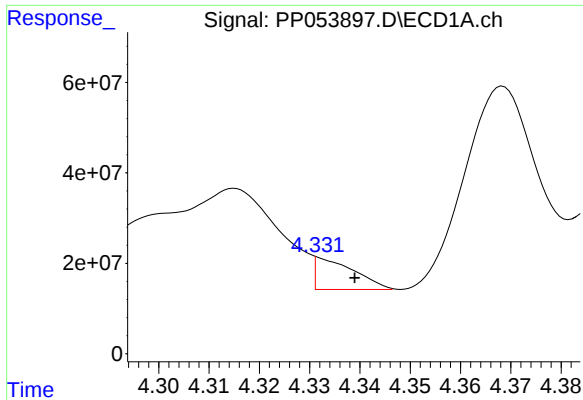


#1 Tetrachloro-m-xylene

R.T.: 4.331 min
Delta R.T.: -0.008 min
Response: 36351997
Conc: 17.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
HAN-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

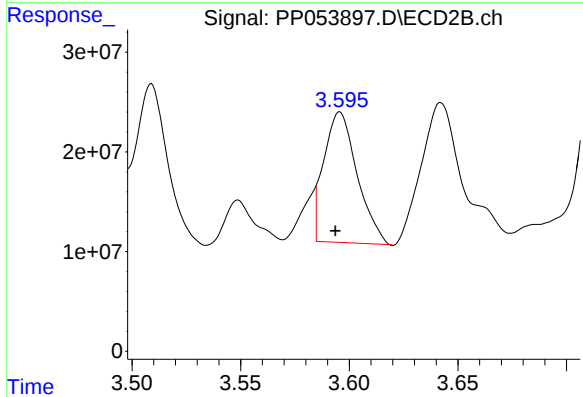


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.002 min
Response: 138056741
Conc: 88.40 ng/ml m

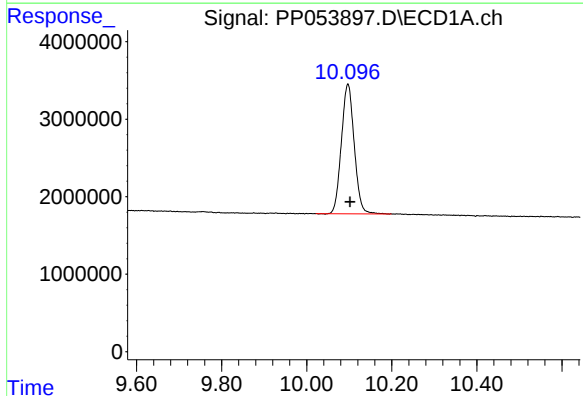

#2 Decachlorobiphenyl

R.T.: 10.097 min
Delta R.T.: -0.005 min
Response: 35049268
Conc: 20.64 ng/ml

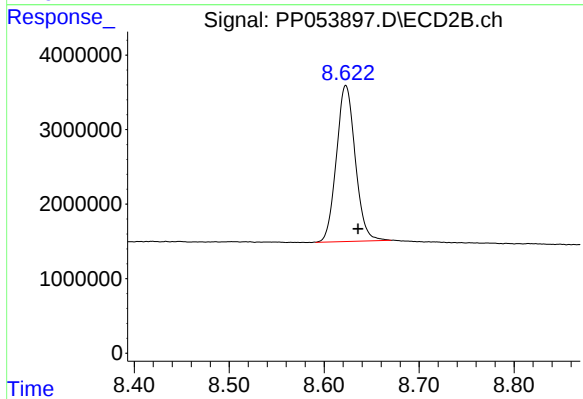

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: -0.013 min
Response: 28877433
Conc: 20.67 ng/ml m