

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
 Data File : PP032260.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2020 13:27
 Operator : DD\AJ
 Sample : L5159-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CGP-1

Manual Integrations
 APPROVED

Ankita
 12/22/2020 12:17:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 05:16:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.769	4.047	2192191	1014504	42.556m	21.450m#
2) SA Decachlor...	10.640	9.338	945666	920339	30.156	27.443

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
Data File : PP032260.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2020 13:27
Operator : DD\AJ
Sample : L5159-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CGP-1


Manual Integrations
APPROVED

Ankita
12/22/2020 12:17:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 05:16:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

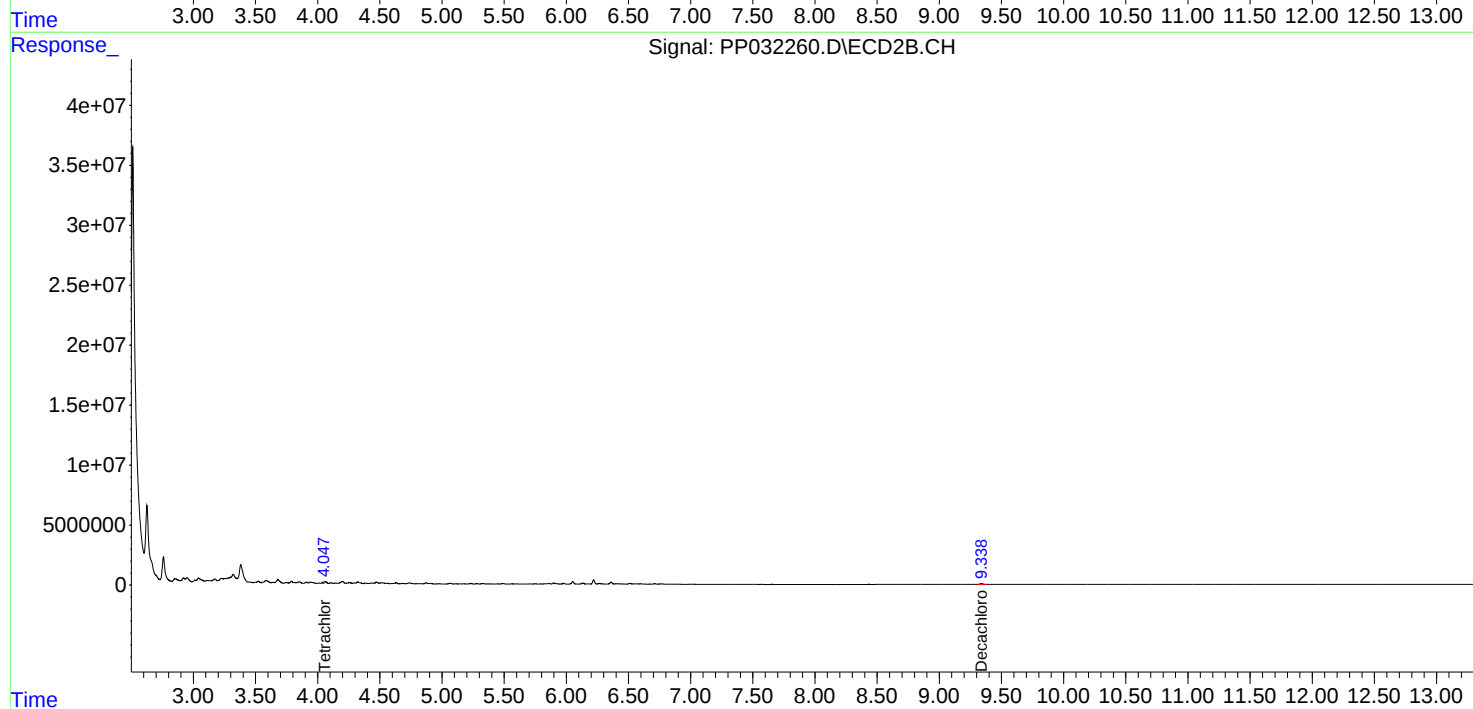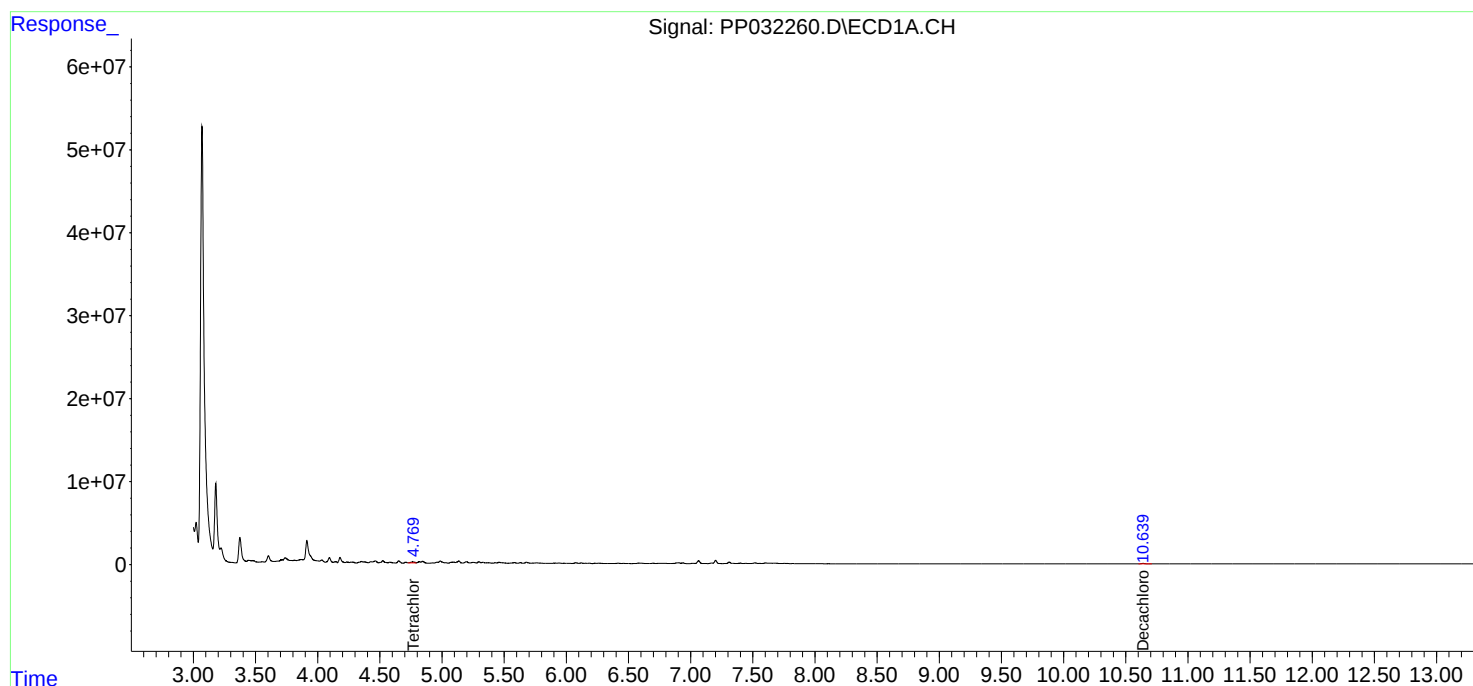

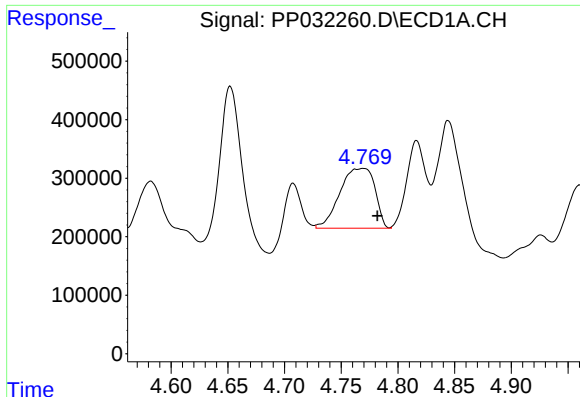


#1 Tetrachloro-m-xylene

R.T.: 4.769 min
Delta R.T.: -0.013 min
Response: 2192191
Conc: 42.56 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CGP-1


Manual Integrations
APPROVED

Ankita
12/22/2020 12:17:04 PM

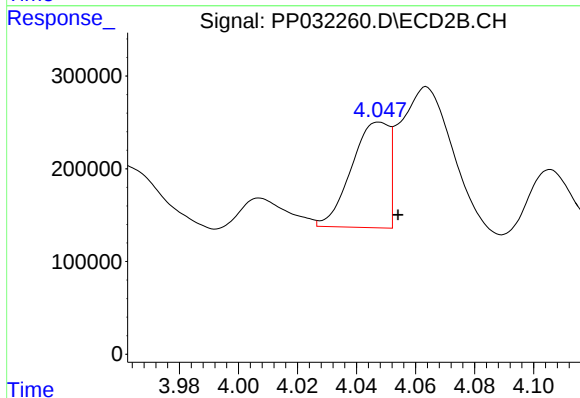


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: -0.007 min
Response: 1014504
Conc: 21.45 ng/ml m

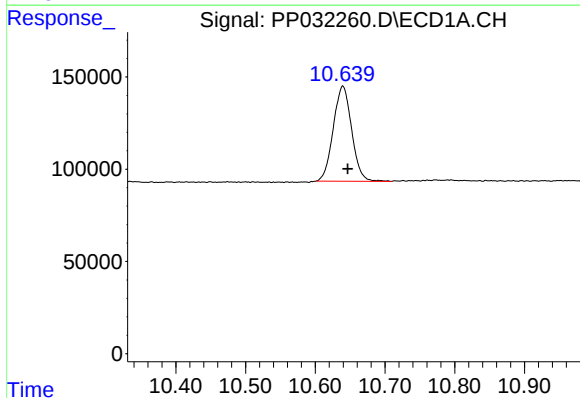

#2 Decachlorobiphenyl

R.T.: 10.640 min
Delta R.T.: -0.007 min
Response: 945666
Conc: 30.16 ng/ml

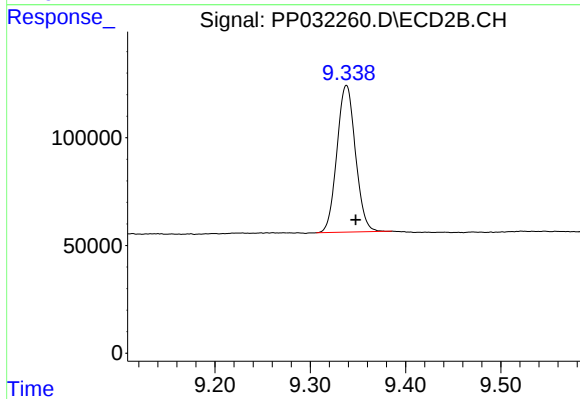

#2 Decachlorobiphenyl

R.T.: 9.338 min
Delta R.T.: -0.010 min
Response: 920339
Conc: 27.44 ng/ml