

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
 Data File : PP032261.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2020 13:44
 Operator : DD\AJ
 Sample : L5159-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CGP-2

Manual Integrations
 APPROVED

Ankita
 12/22/2020 12:17:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 05:16:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.764f	4.045	1721621	1351580	33.421m	28.577m
2) SA Decachlor...	10.640	9.338	995917	978729	31.758	29.184

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
Data File : PP032261.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2020 13:44
Operator : DD\AJ
Sample : L5159-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CGP-2


Manual Integrations
APPROVED

Ankita
12/22/2020 12:17:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 05:16:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

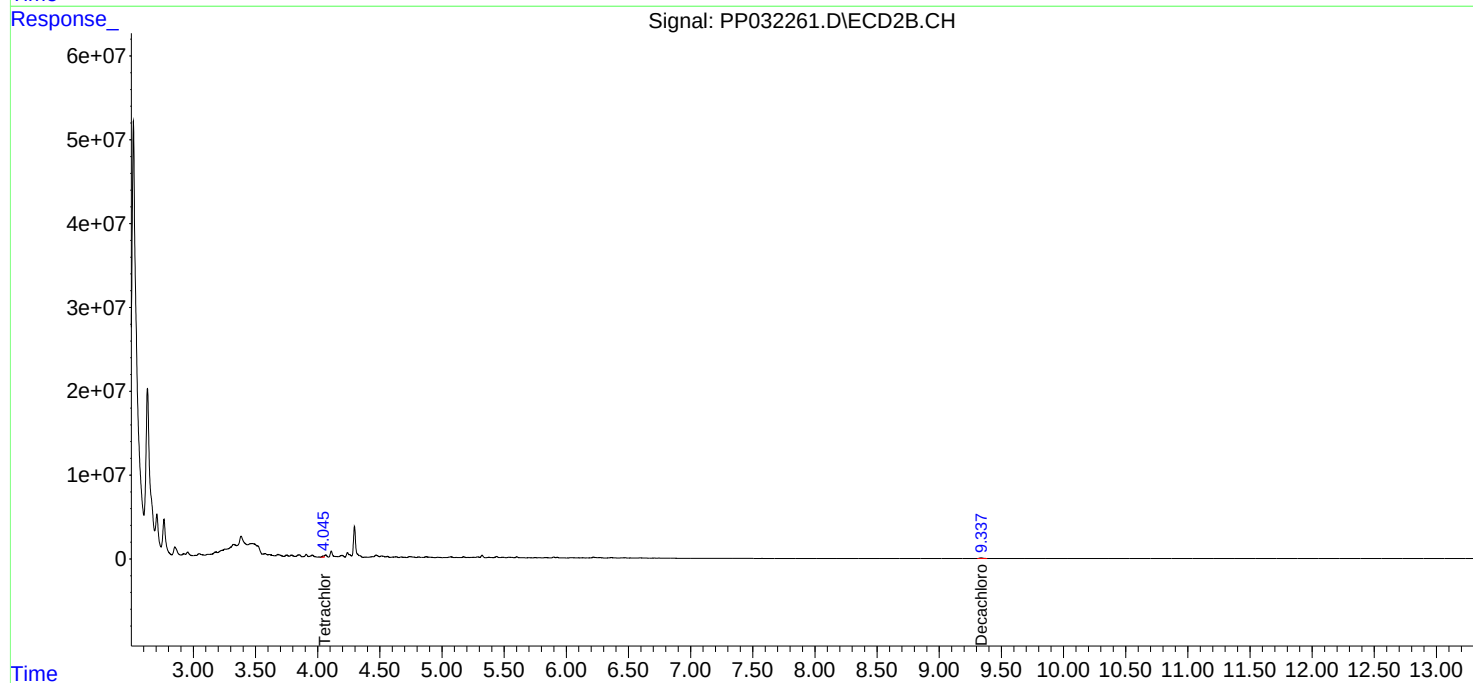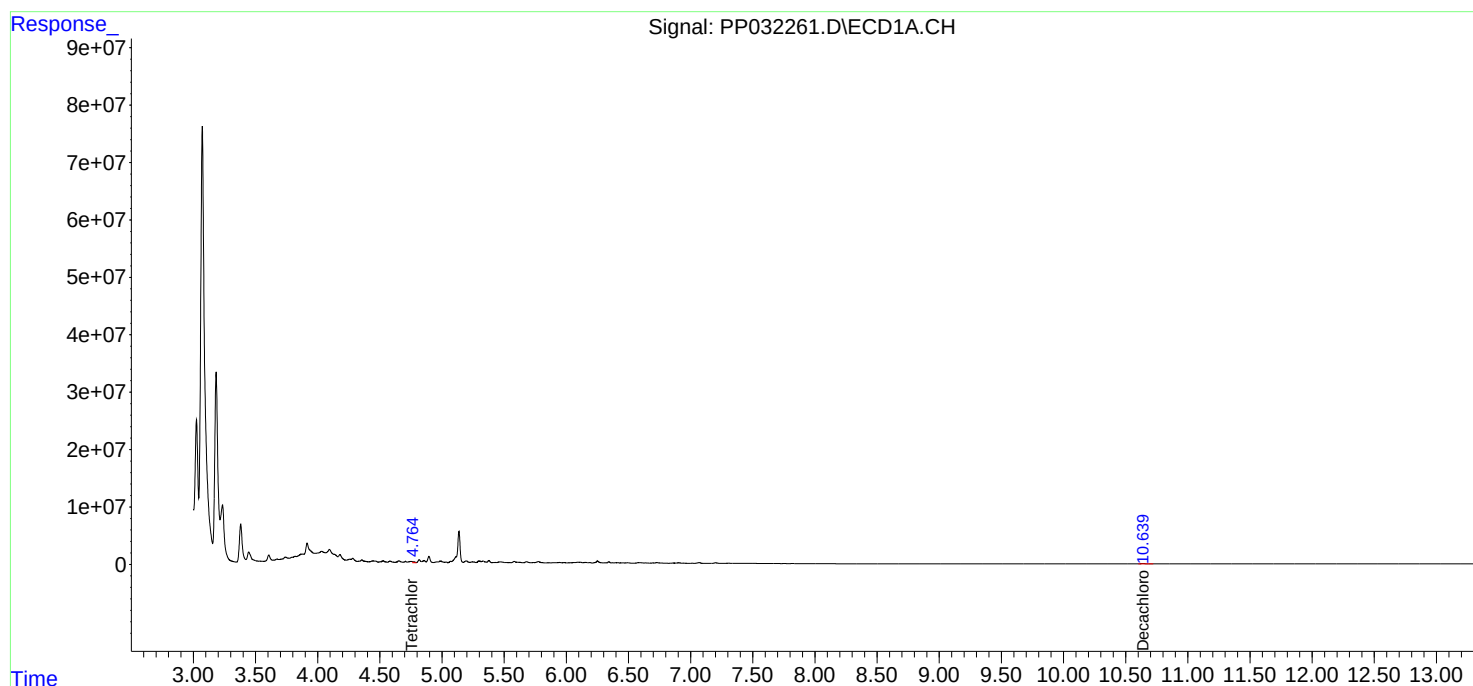

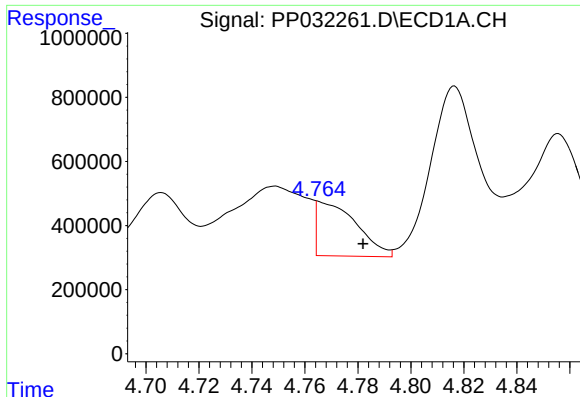


#1 Tetrachloro-m-xylene

R.T.: 4.764 min
Delta R.T.: -0.018 min
Response: 1721621
Conc: 33.42 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CGP-2


Manual Integrations
APPROVED

Ankita
12/22/2020 12:17:05 PM

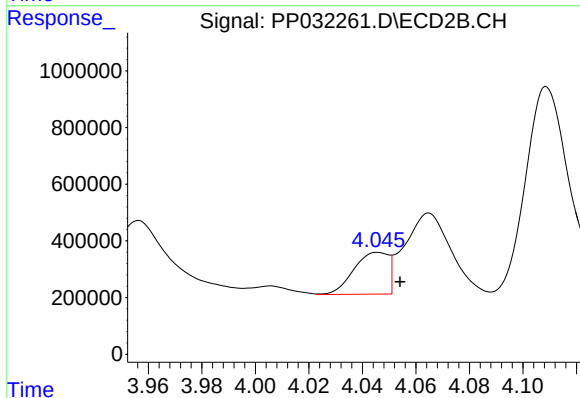


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.009 min
Response: 1351580
Conc: 28.58 ng/ml m

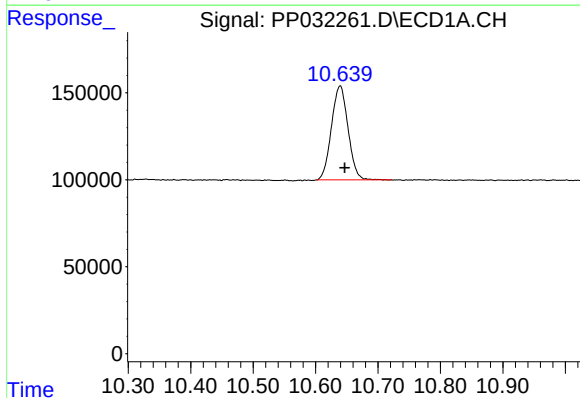

#2 Decachlorobiphenyl

R.T.: 10.640 min
Delta R.T.: -0.007 min
Response: 995917
Conc: 31.76 ng/ml

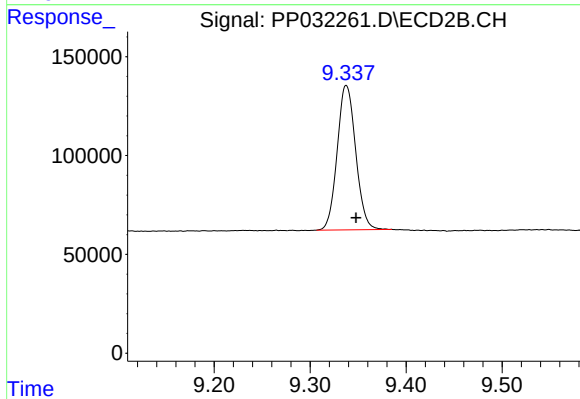

#2 Decachlorobiphenyl

R.T.: 9.338 min
Delta R.T.: -0.010 min
Response: 978729
Conc: 29.18 ng/ml