

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
 Data File : PP032262.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2020 14:00
 Operator : DD\AJ
 Sample : L5159-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CGP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 05:17:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.776	4.048	1300416	1076641	25.244	22.764
2)	SA Decachlor...	10.638	9.339	903733	896112	28.818	26.721

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
Data File : PP032262.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2020 14:00
Operator : DD\AJ
Sample : L5159-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CGP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 05:17:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

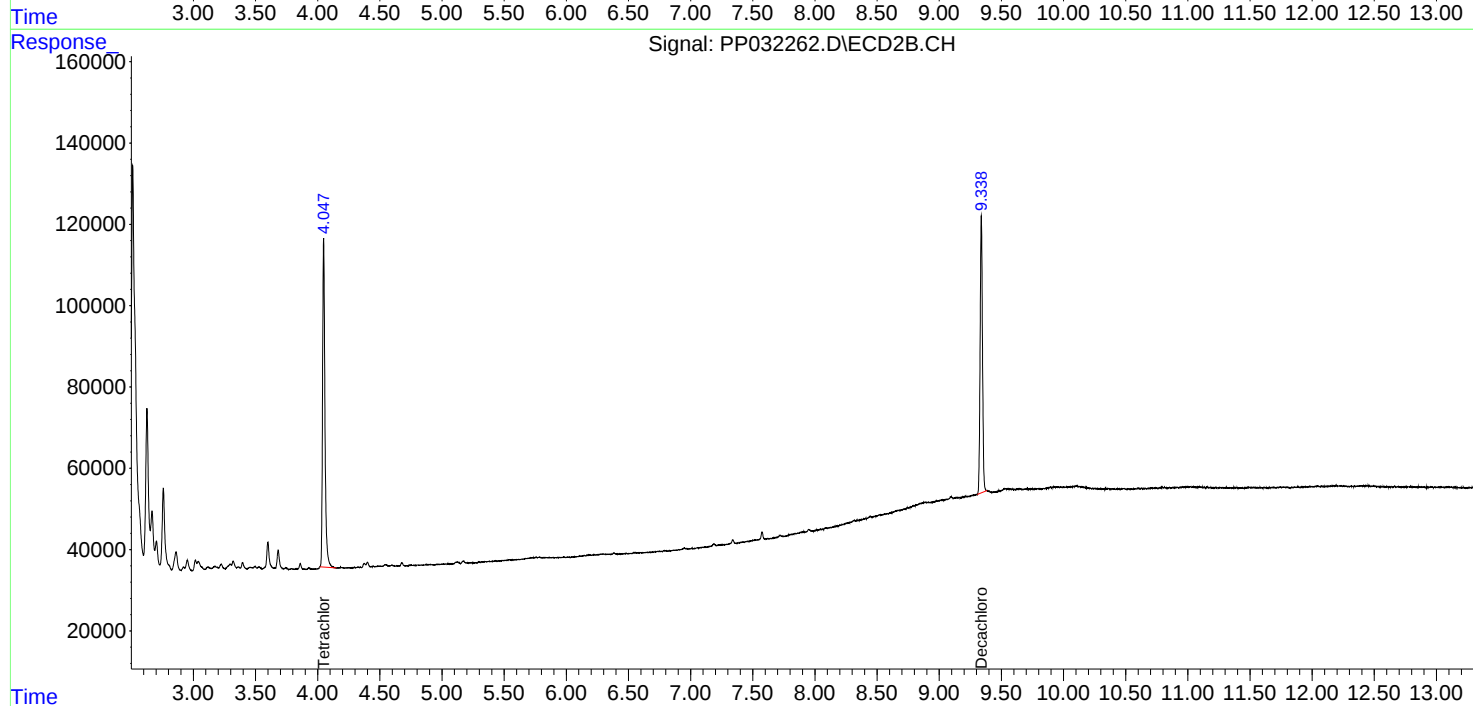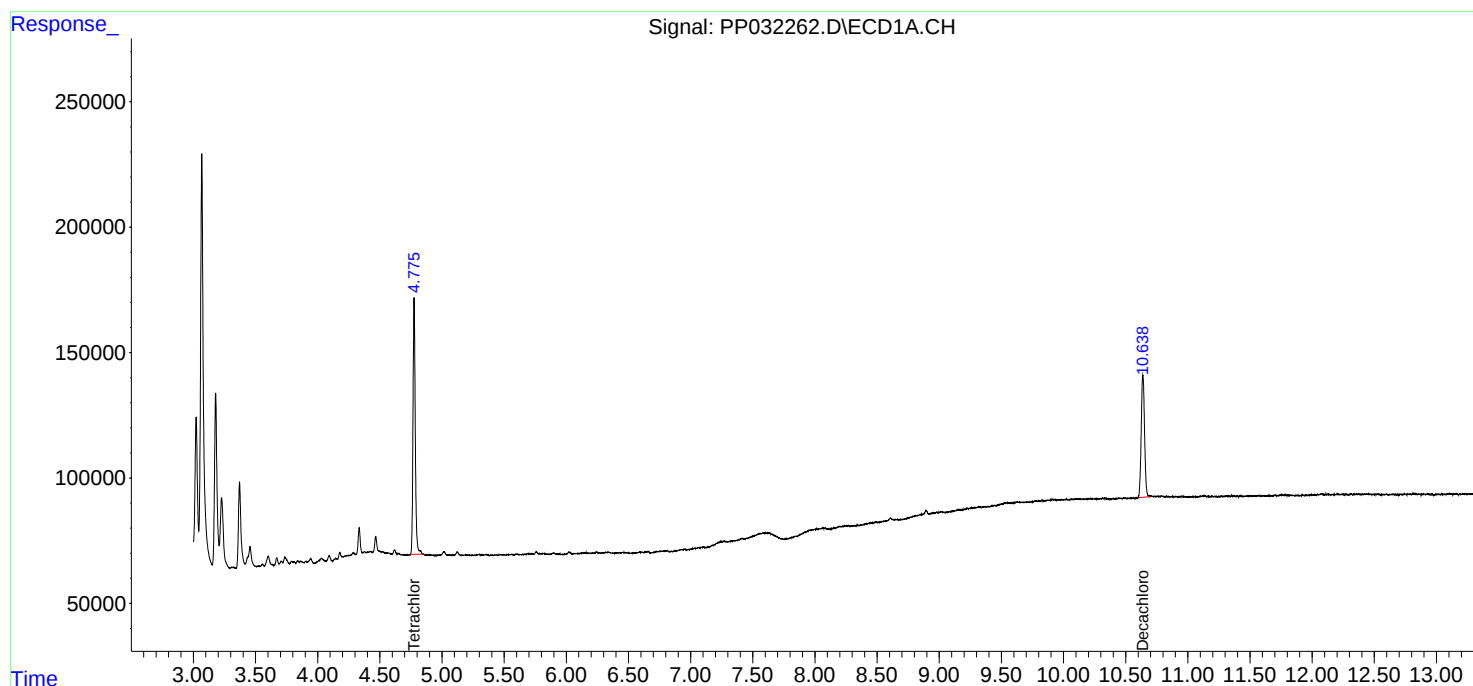


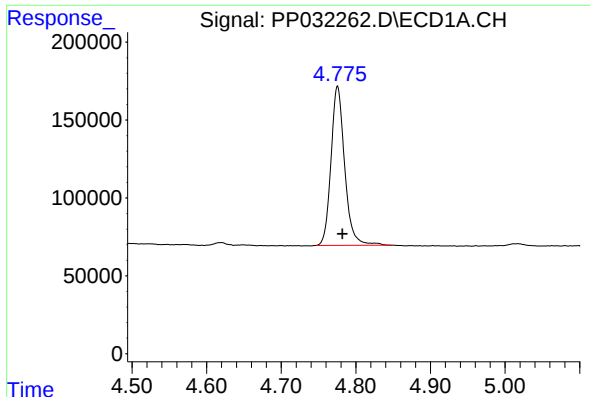

#1 Tetrachloro-m-xylene


R.T.: 4.776 min
Delta R.T.: -0.006 min
Response: 1300416
Conc: 25.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
CGP-3

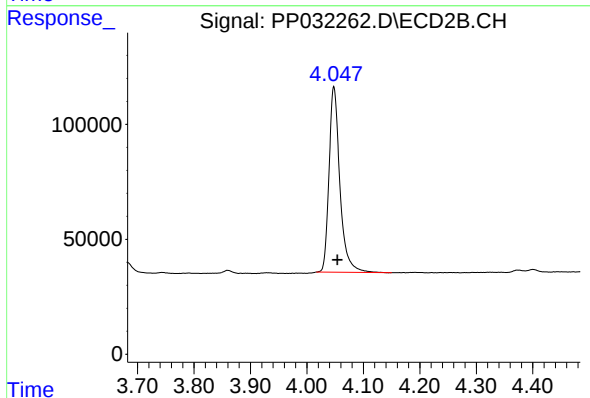


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.006 min
Response: 1076641
Conc: 22.76 ng/ml

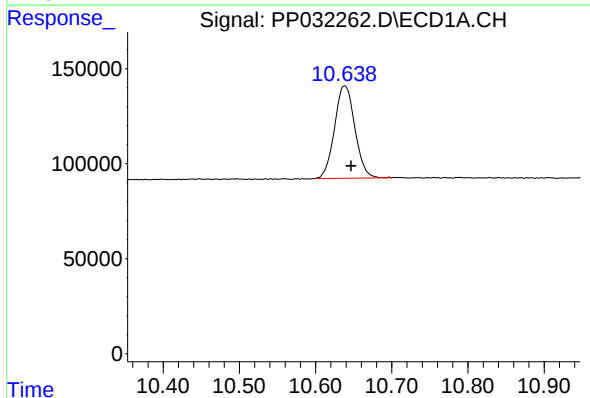

#2 Decachlorobiphenyl

R.T.: 10.638 min
Delta R.T.: -0.009 min
Response: 903733
Conc: 28.82 ng/ml

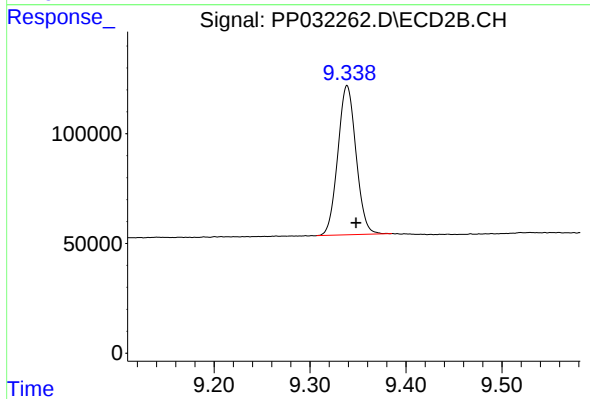

#2 Decachlorobiphenyl

R.T.: 9.339 min
Delta R.T.: -0.009 min
Response: 896112
Conc: 26.72 ng/ml