

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
 Data File : PP032264.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2020 14:34
 Operator : DD\AJ
 Sample : L5159-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CGP-5

Manual Integrations
 APPROVED

Ankita
 12/22/2020 12:17:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 05:18:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.757f	4.044	6102136	2072063	118.458m	43.810m#
2) SA Decachlor...	10.640	9.338	965715	926119	30.795	27.615

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
Data File : PP032264.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2020 14:34
Operator : DD\AJ
Sample : L5159-09
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CGP-5


Manual Integrations
APPROVED

Ankita
12/22/2020 12:17:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 05:18:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

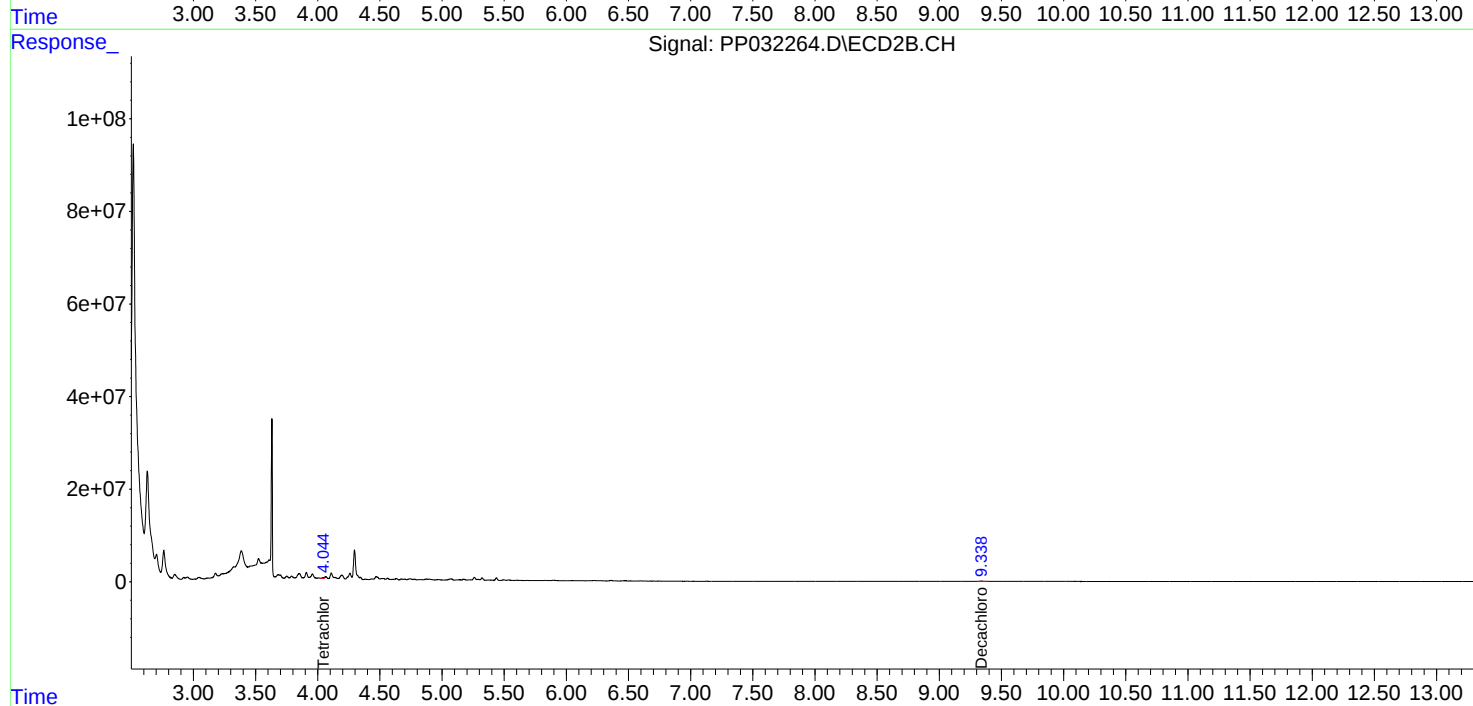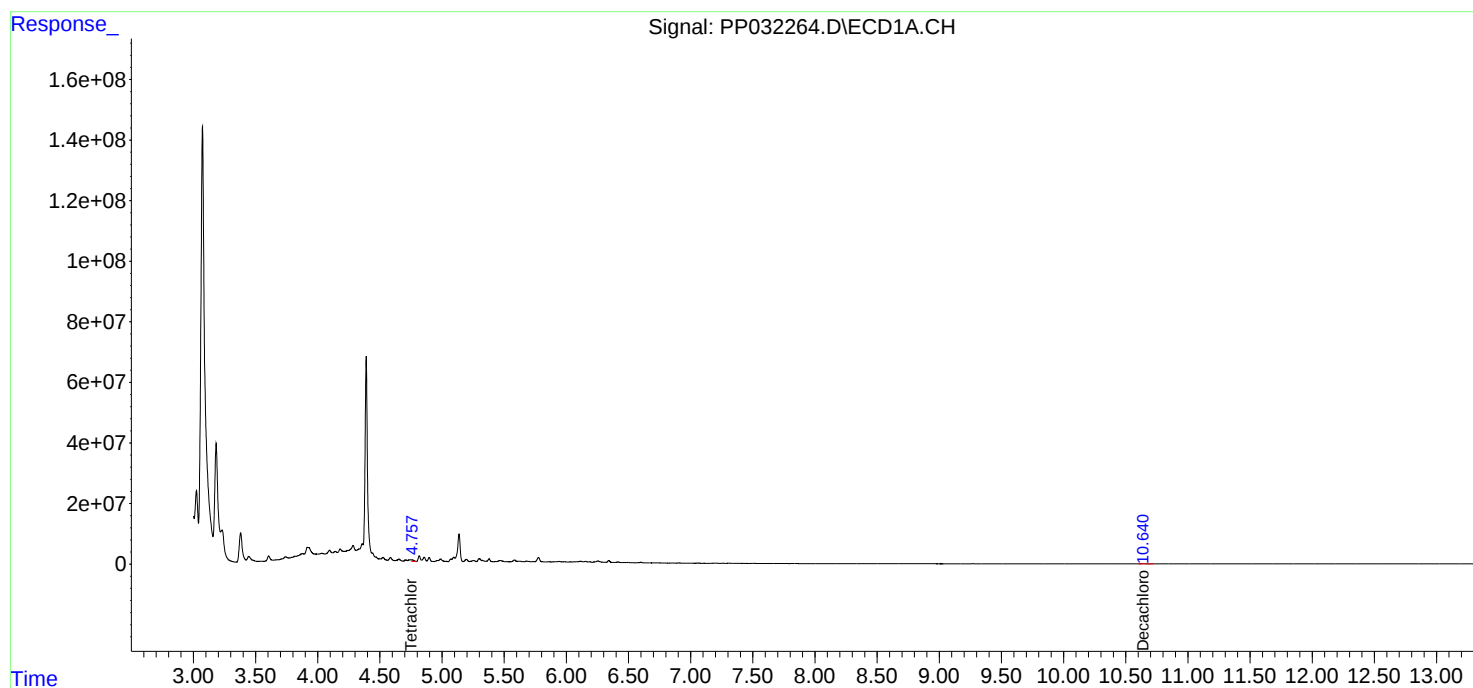

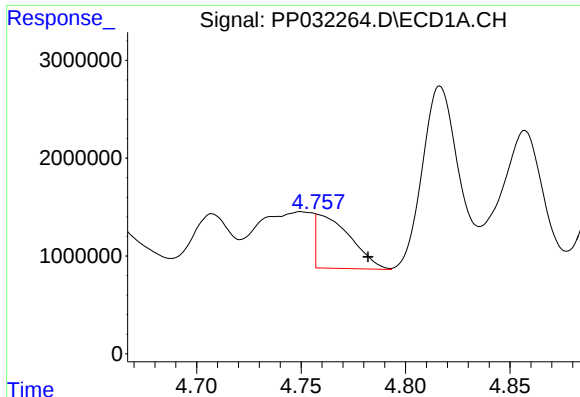


#1 Tetrachloro-m-xylene

R.T.: 4.757 min
Delta R.T.: -0.025 min
Response: 6102136
Conc: 118.46 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CGP-5


Manual Integrations
APPROVED

Ankita
12/22/2020 12:17:09 PM

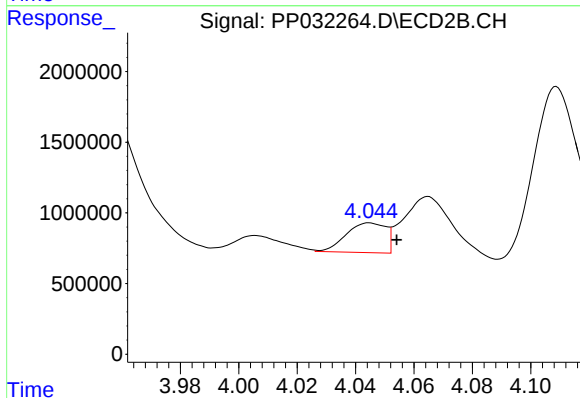


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.010 min
Response: 2072063
Conc: 43.81 ng/ml m

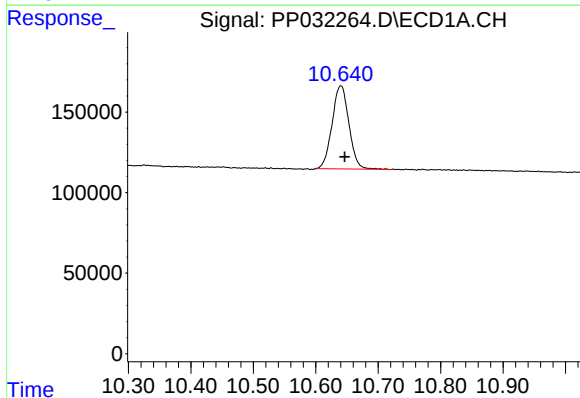

#2 Decachlorobiphenyl

R.T.: 10.640 min
Delta R.T.: -0.006 min
Response: 965715
Conc: 30.79 ng/ml

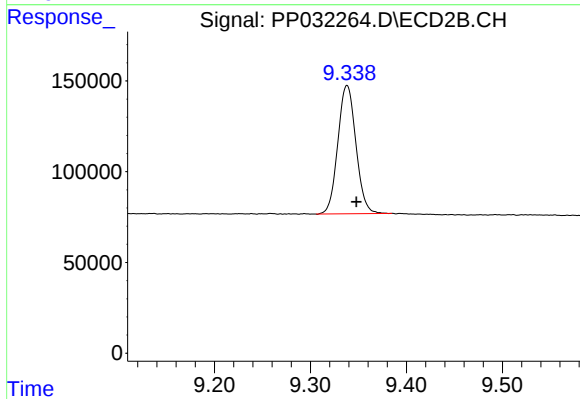

#2 Decachlorobiphenyl

R.T.: 9.338 min
Delta R.T.: -0.010 min
Response: 926119
Conc: 27.62 ng/ml