

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
 Data File : PP032271.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2020 16:30
 Operator : DD\AJ
 Sample : L5159-19
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CGP-10

Manual Integrations
 APPROVED

Ankita
 12/22/2020 12:17:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 05:22:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.776	4.050	803460	821401	15.597m	17.367
2) SA Decachlor...	10.640	9.338	862929	838035	27.517	24.989

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122120\
Data File : PP032271.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2020 16:30
Operator : DD\AJ
Sample : L5159-19
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
CGP-10


Manual Integrations
APPROVED

Ankita
12/22/2020 12:17:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 05:22:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

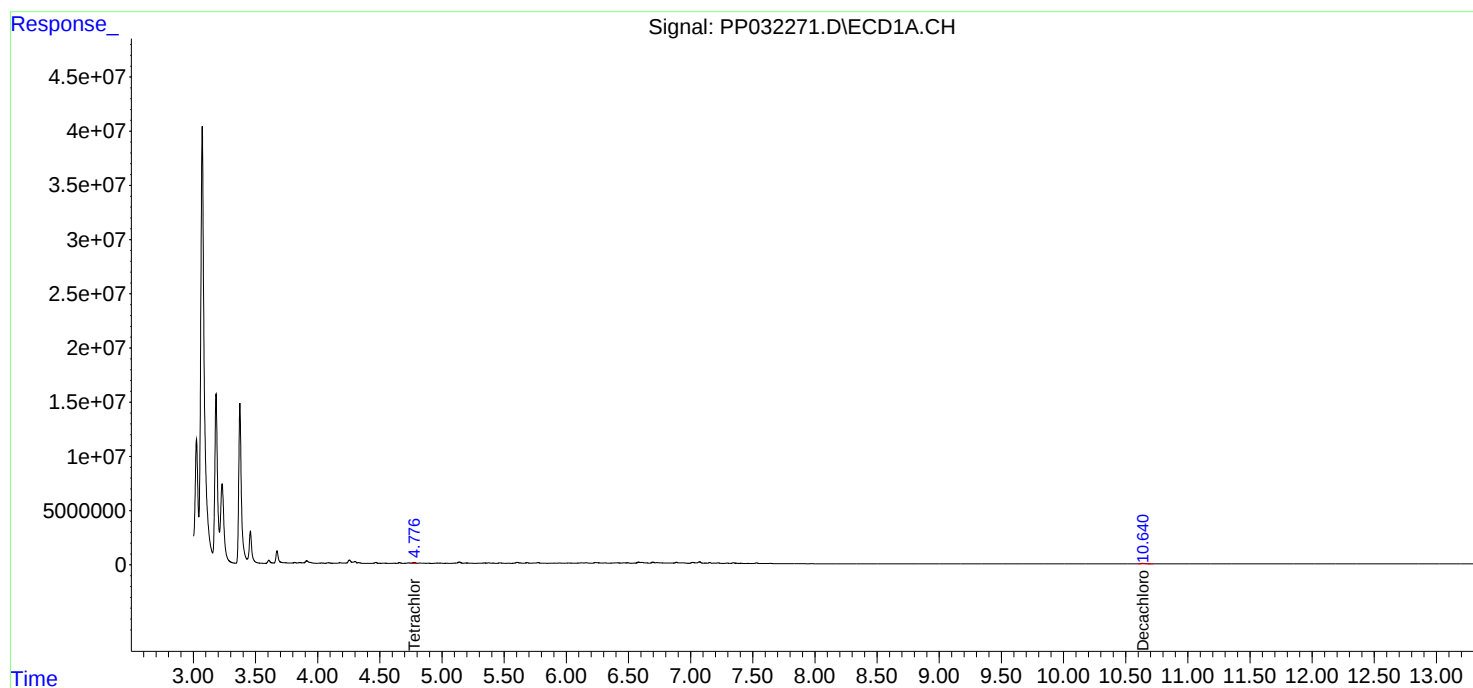

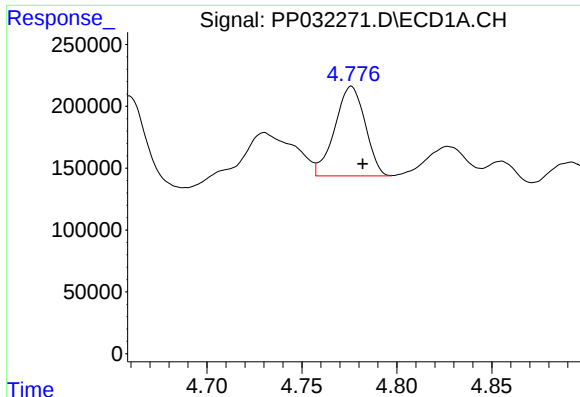


#1 Tetrachloro-m-xylene

R.T.: 4.776 min
Delta R.T.: -0.006 min
Response: 803460
Conc: 15.60 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CGP-10


Manual Integrations
APPROVED

Ankita
12/22/2020 12:17:17 PM

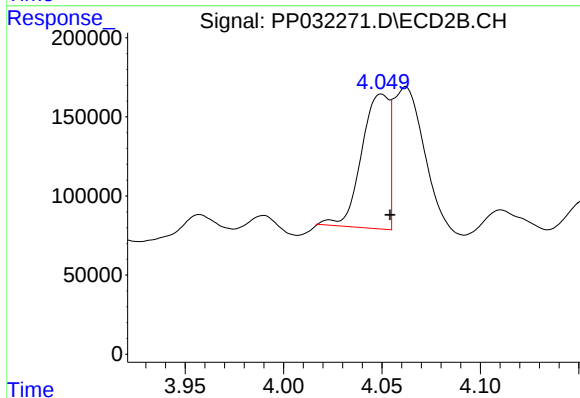


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.004 min
Response: 821401
Conc: 17.37 ng/ml

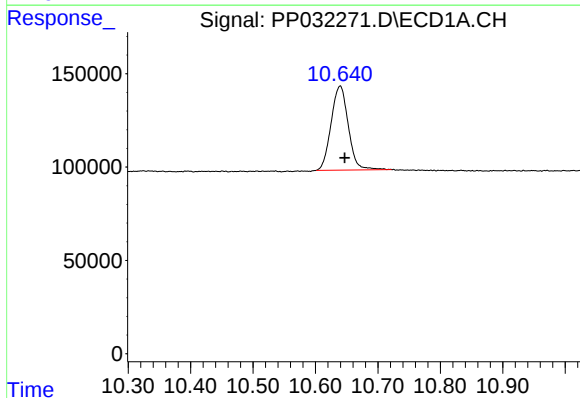

#2 Decachlorobiphenyl

R.T.: 10.640 min
Delta R.T.: -0.007 min
Response: 862929
Conc: 27.52 ng/ml

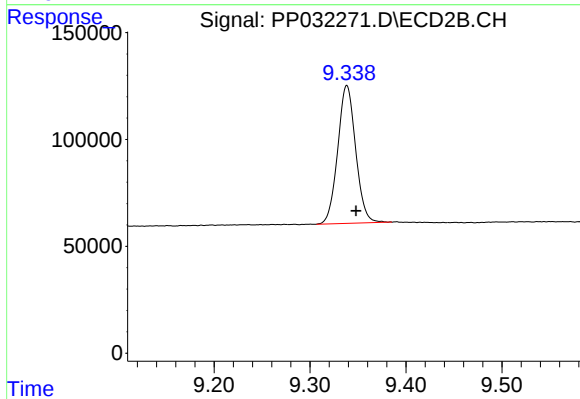

#2 Decachlorobiphenyl

R.T.: 9.338 min
Delta R.T.: -0.009 min
Response: 838035
Conc: 24.99 ng/ml