

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122121\
 Data File : PP042118.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2021 21:24
 Operator : AJ\MA
 Sample : M5144-02 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEC-2021-68-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 01:36:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 06:21:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.926	4.065	30798	51273	2.387	2.090
2)	SA Decachlor...	10.923	9.421	43482	52556	3.300m	2.614m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122121\
Data File : PP042118.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2021 21:24
Operator : AJ\MA
Sample : M5144-02 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SEC-2021-68-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 01:36:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 06:21:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

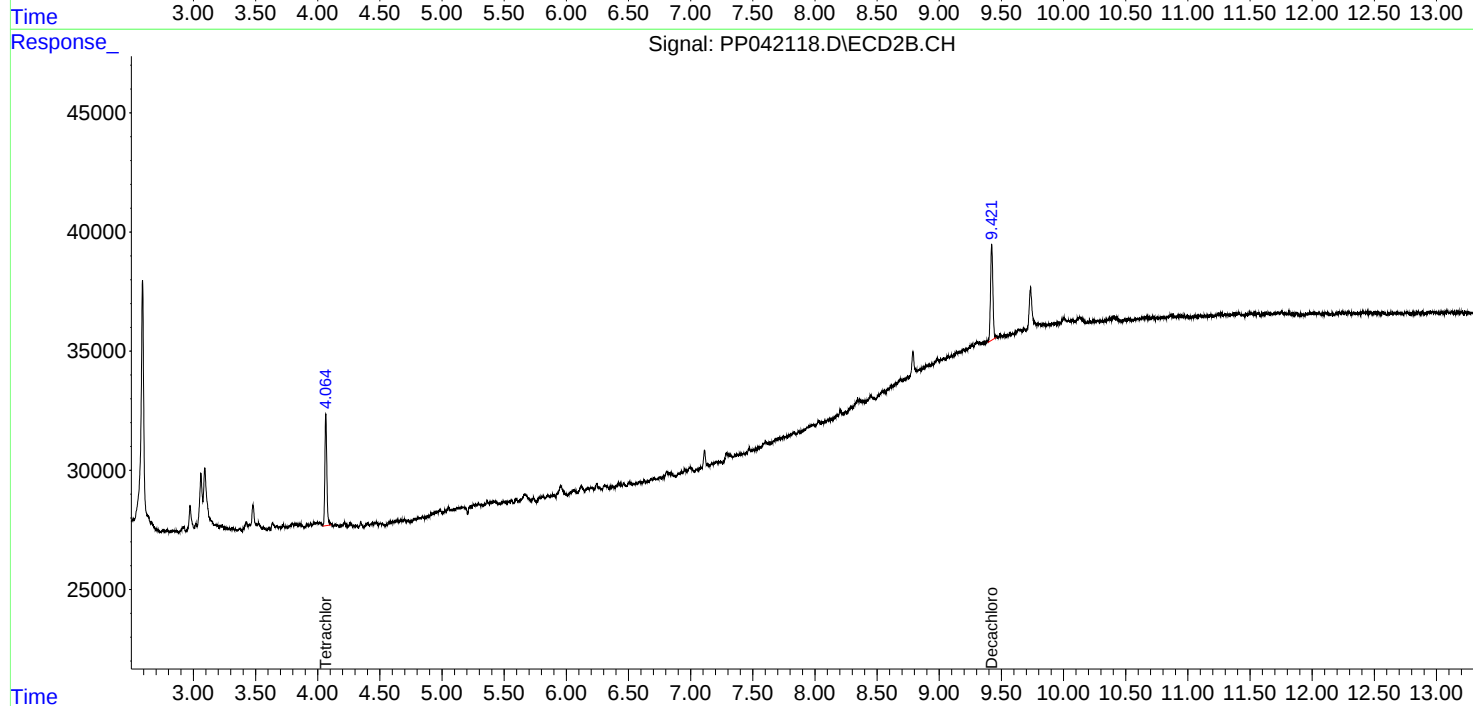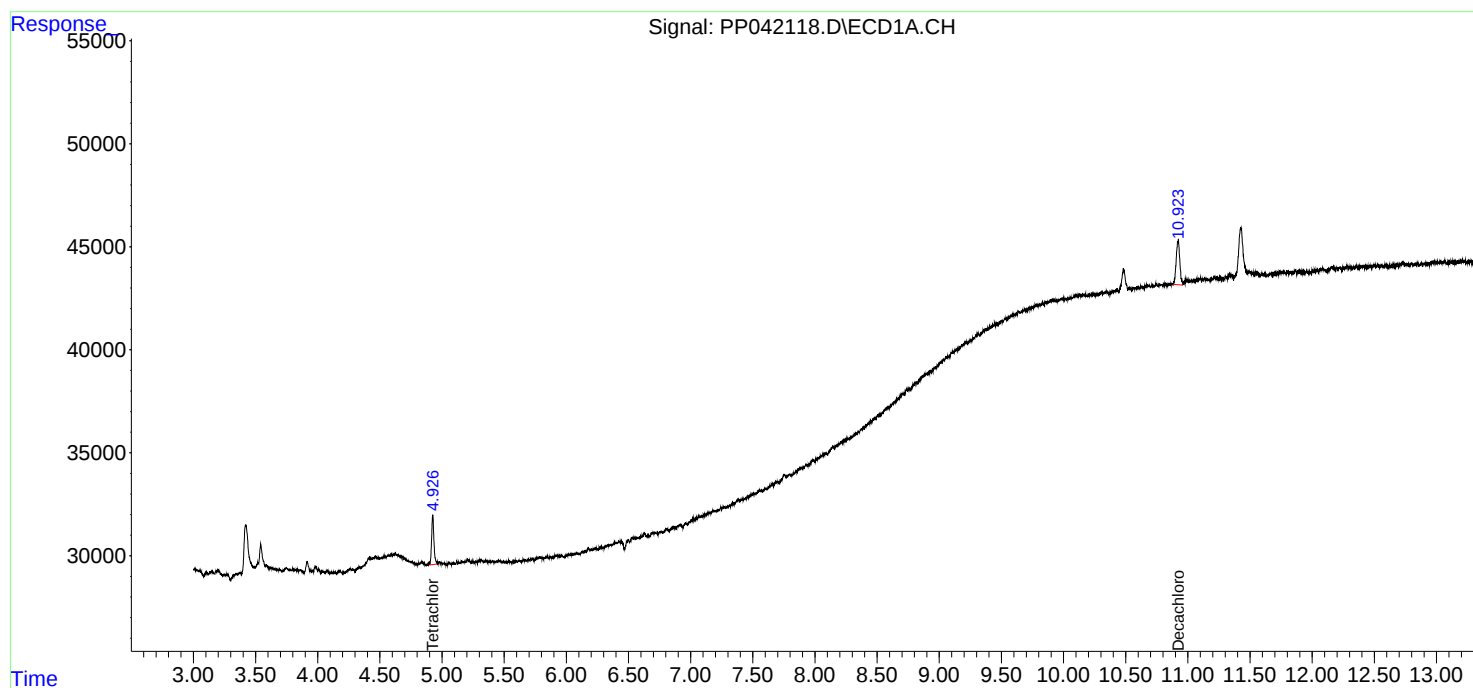


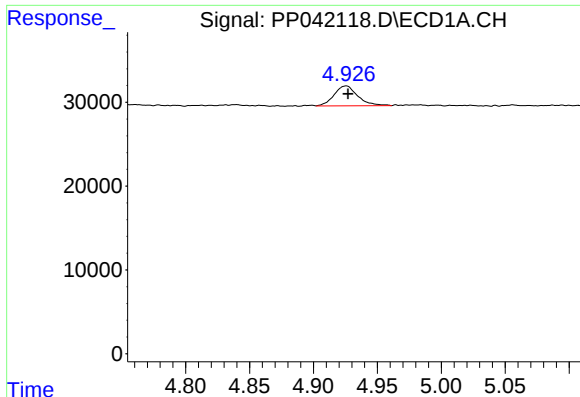

#1 Tetrachloro-m-xylene


R.T.: 4.926 min
Delta R.T.: -0.001 min
Response: 30798
Conc: 2.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2021-68-A

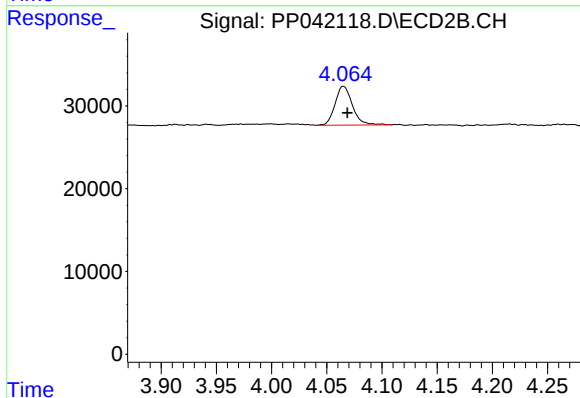


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: -0.004 min
Response: 51273
Conc: 2.09 ng/ml

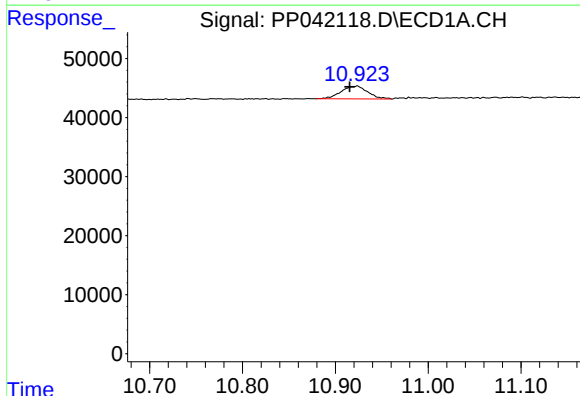

#2 Decachlorobiphenyl

R.T.: 10.923 min
Delta R.T.: 0.008 min
Response: 43482
Conc: 3.30 ng/ml m

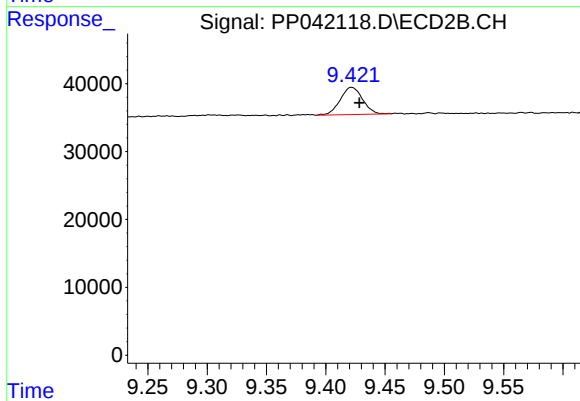

#2 Decachlorobiphenyl

R.T.: 9.421 min
Delta R.T.: -0.007 min
Response: 52556
Conc: 2.61 ng/ml m