

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122121\
 Data File : PP042119.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2021 21:41
 Operator : AJ\MA
 Sample : M5144-03 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEC-2021-68-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 01:37:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 06:21:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	4.065	26105	47336	2.023m	1.930m
2) SA Decachlor...	10.924	9.423	30991	45124	2.352	2.244m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122121\
Data File : PP042119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2021 21:41
Operator : AJ\MA
Sample : M5144-03 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SEC-2021-68-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 01:37:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 06:21:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

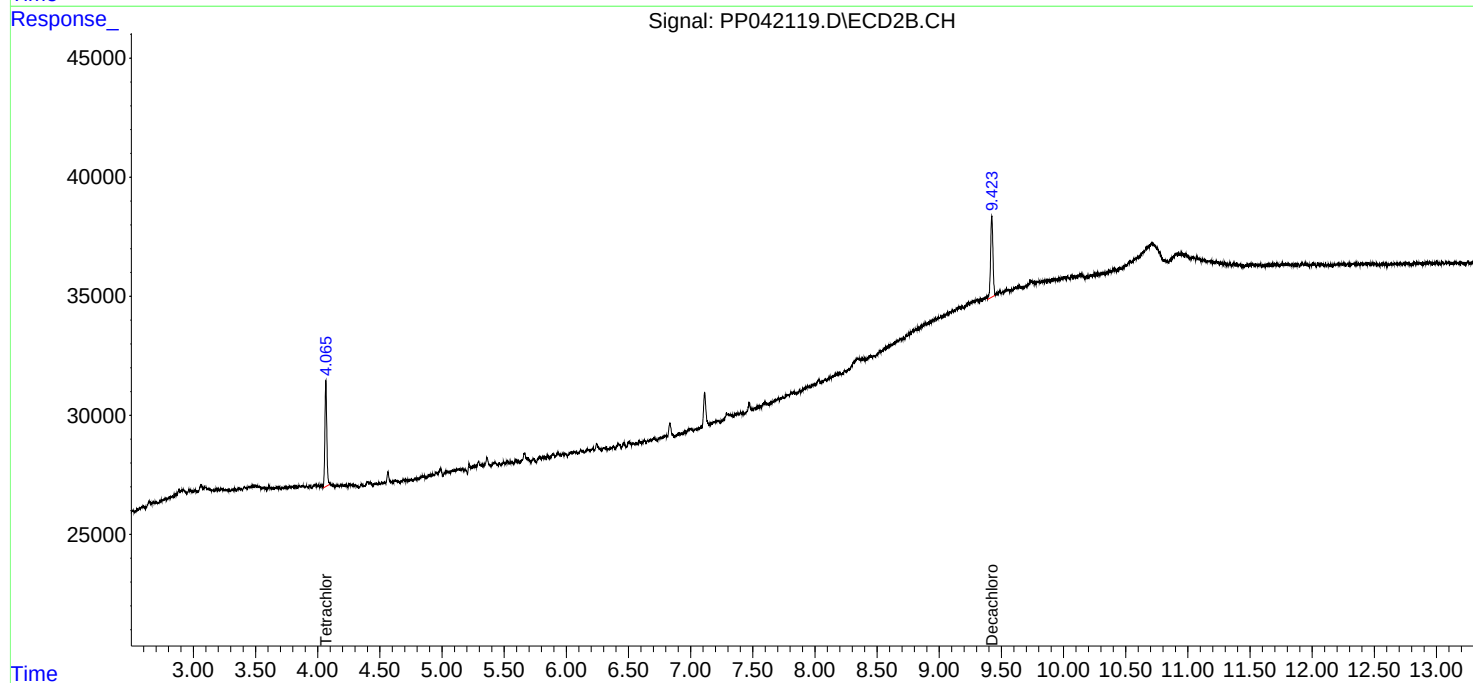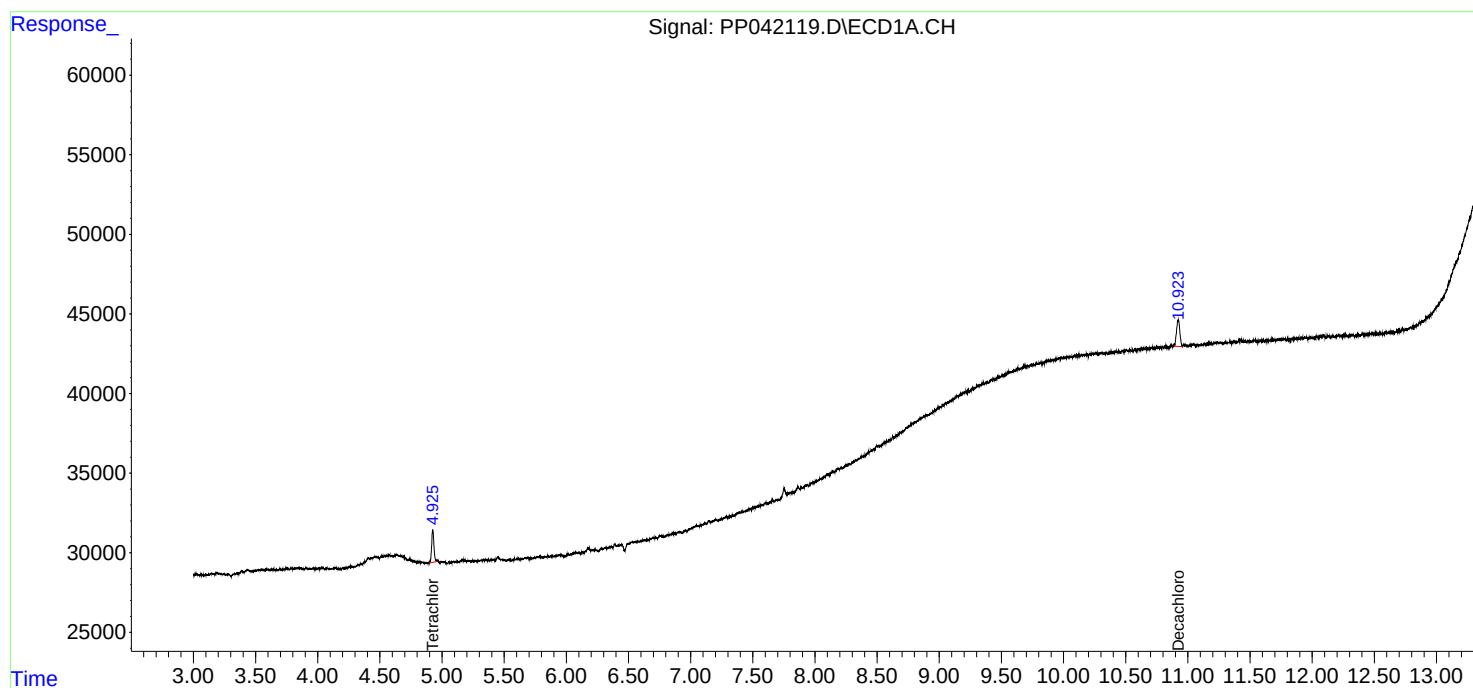


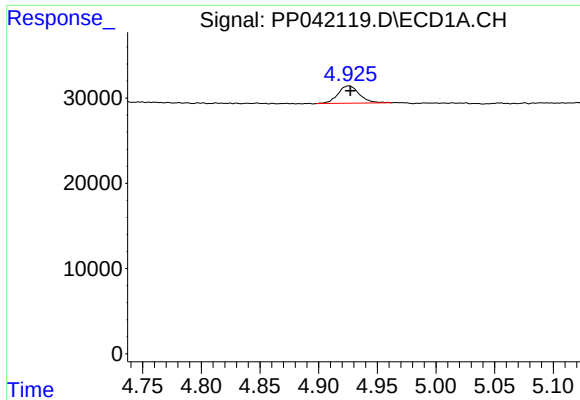

#1 Tetrachloro-m-xylene


R.T.: 4.925 min
Delta R.T.: -0.002 min
Response: 26105
Conc: 2.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2021-68-B

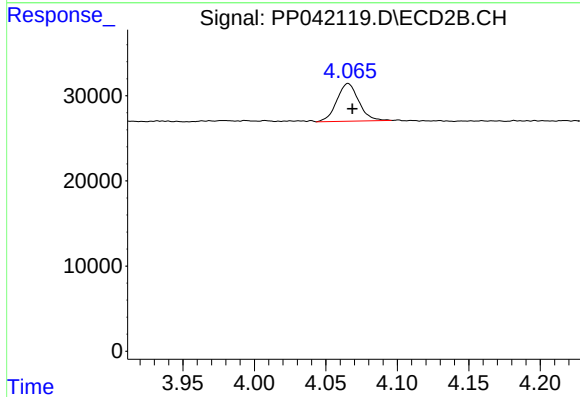


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: -0.003 min
Response: 47336
Conc: 1.93 ng/ml m

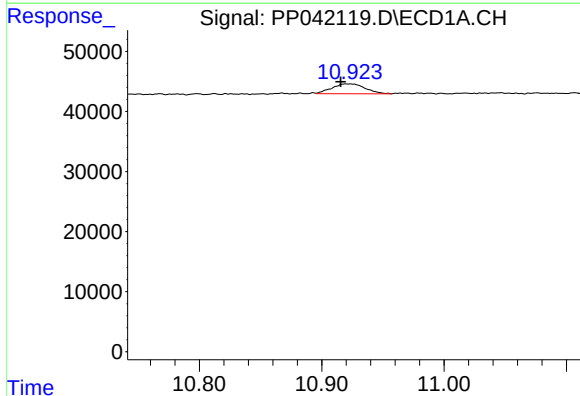

#2 Decachlorobiphenyl

R.T.: 10.924 min
Delta R.T.: 0.008 min
Response: 30991
Conc: 2.35 ng/ml

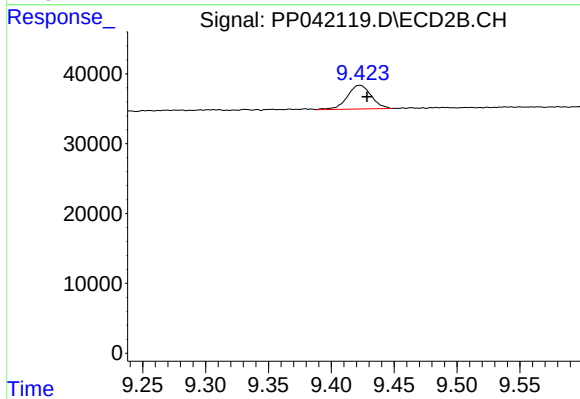

#2 Decachlorobiphenyl

R.T.: 9.423 min
Delta R.T.: -0.006 min
Response: 45124
Conc: 2.24 ng/ml m