

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122121\
 Data File : PP042123.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2021 22:47
 Operator : AJ\MA
 Sample : M5144-07 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEC-2021-70-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 01:38:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 06:21:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	4.065	35247	58178	2.732m	2.371m
2) SA Decachlor...	10.922	9.424	38763	42981	2.941m	2.138m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122121\
Data File : PP042123.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2021 22:47
Operator : AJ\MA
Sample : M5144-07 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SEC-2021-70-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 01:38:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 06:21:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

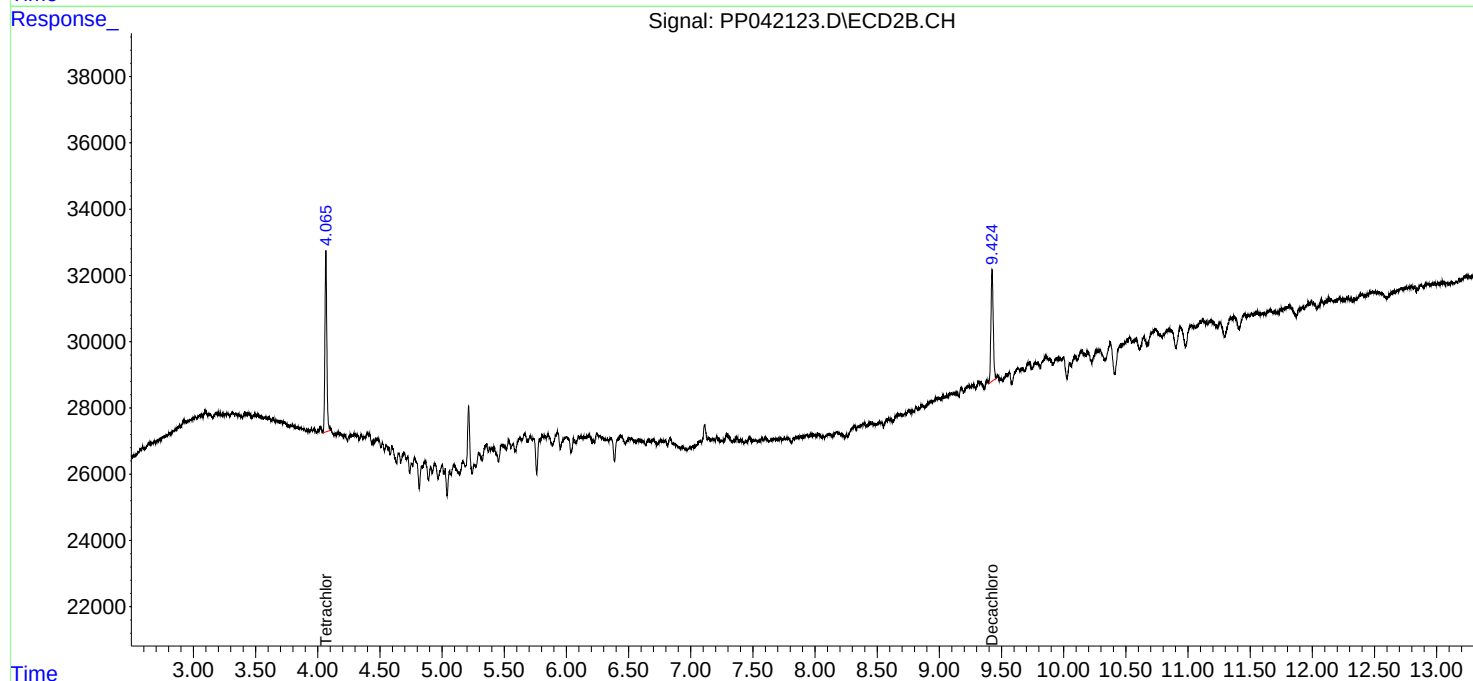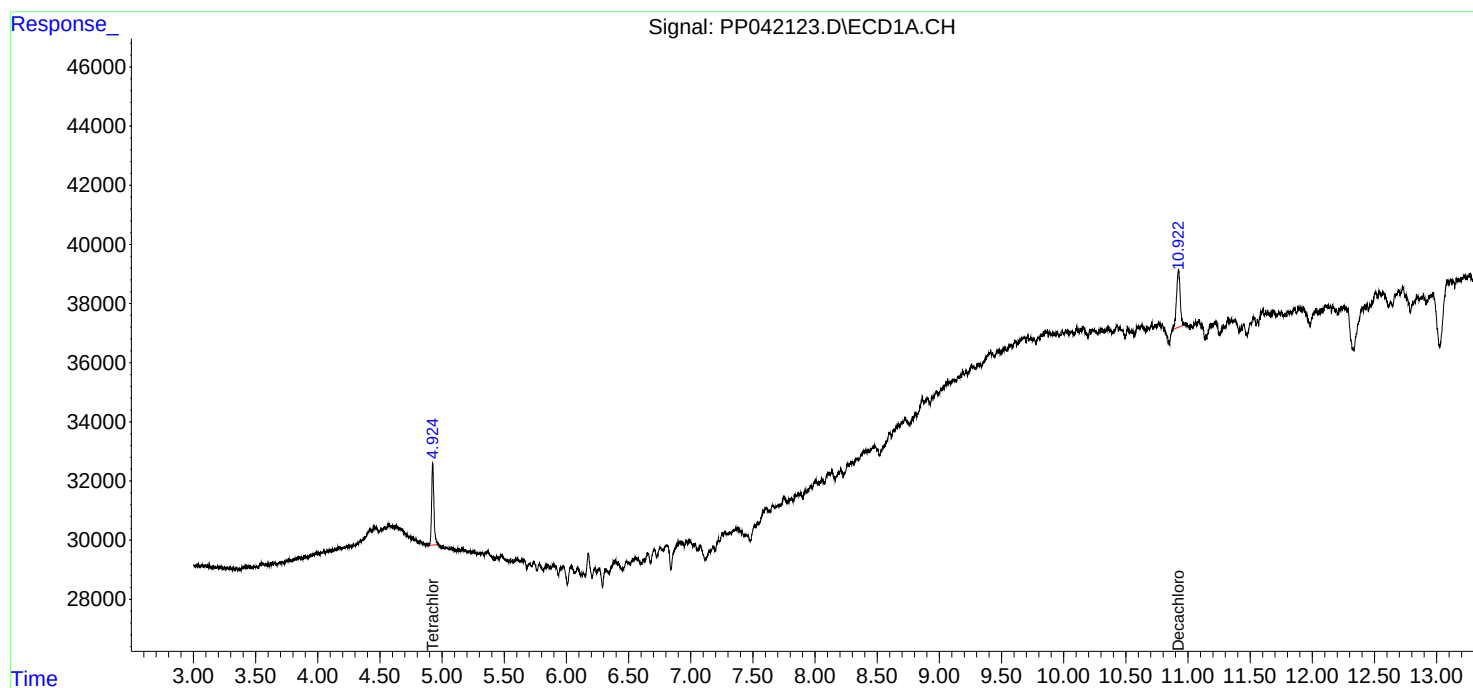


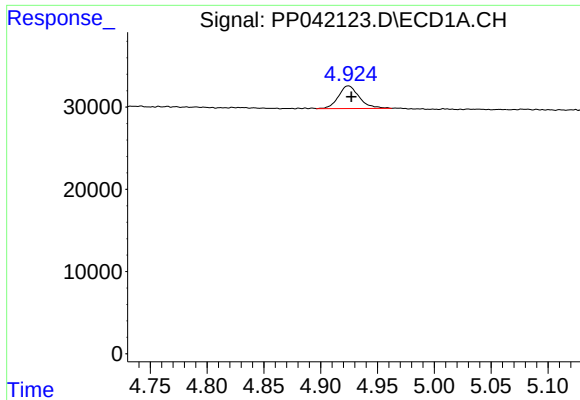

#1 Tetrachloro-m-xylene


R.T.: 4.924 min
Delta R.T.: -0.003 min
Response: 35247
Conc: 2.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2021-70-B

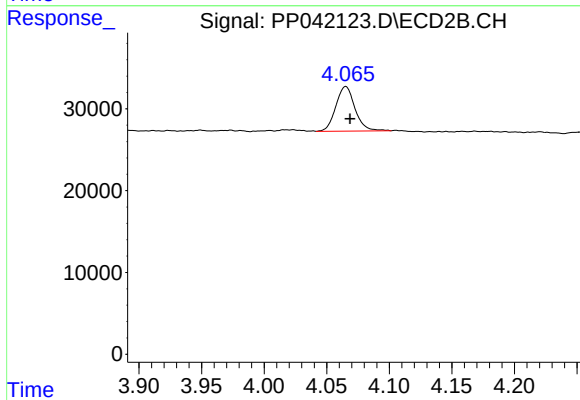


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: -0.004 min
Response: 58178
Conc: 2.37 ng/ml m

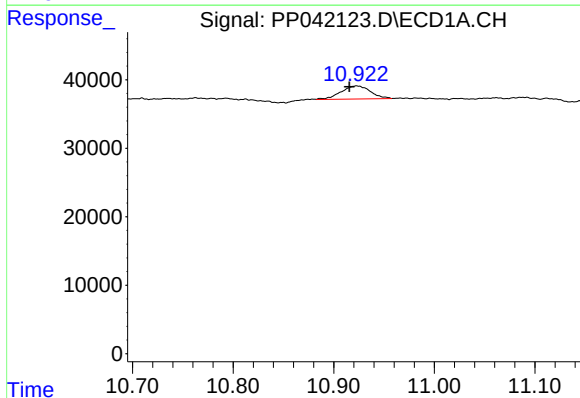

#2 Decachlorobiphenyl

R.T.: 10.922 min
Delta R.T.: 0.007 min
Response: 38763
Conc: 2.94 ng/ml m

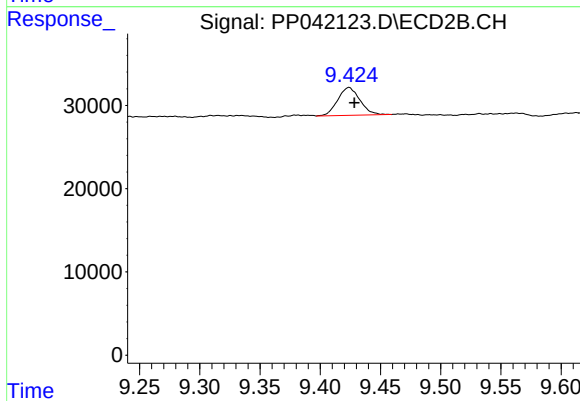

#2 Decachlorobiphenyl

R.T.: 9.424 min
Delta R.T.: -0.005 min
Response: 42981
Conc: 2.14 ng/ml m