

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122220\
 Data File : PP032315.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Dec 2020 13:50
 Operator : DD\AJ
 Sample : L5158-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 32841

Manual Integrations
 APPROVED

Ankita
 12/23/2020 2:17:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 17:19:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.774	4.046	1133008	1070354	21.995m	22.631
2) SA Decachlor...	10.635	9.334	981412	997259	31.296m	29.737

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122220\
Data File : PP032315.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Dec 2020 13:50
Operator : DD\AJ
Sample : L5158-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
32841


Manual Integrations
APPROVED

Ankita
12/23/2020 2:17:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 17:19:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

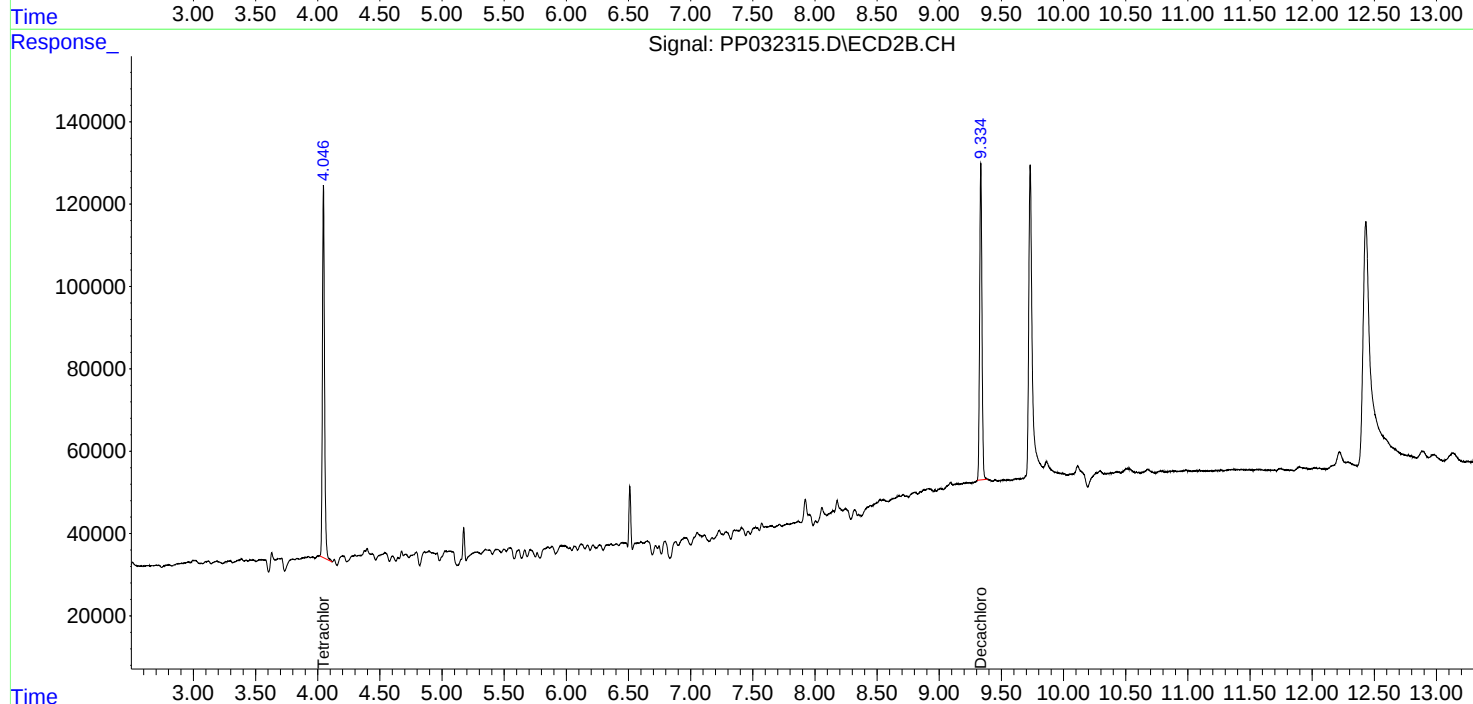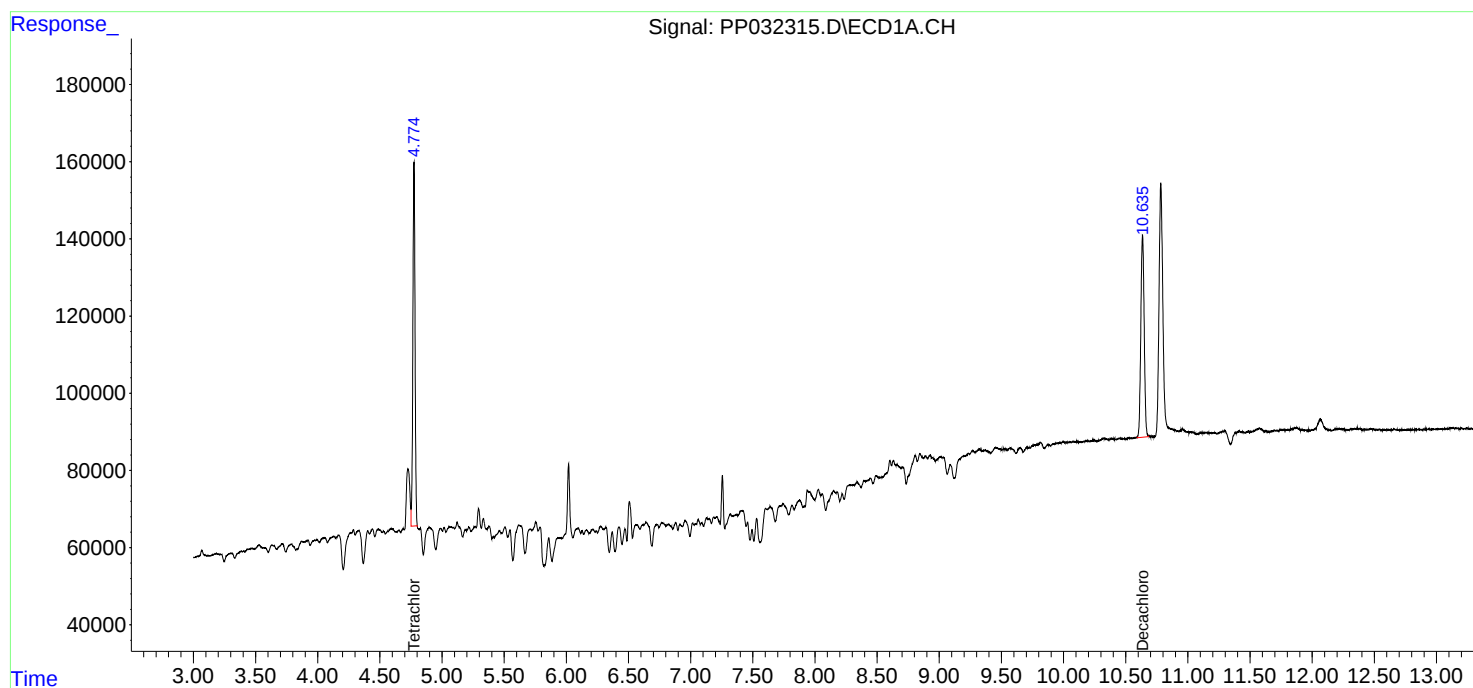

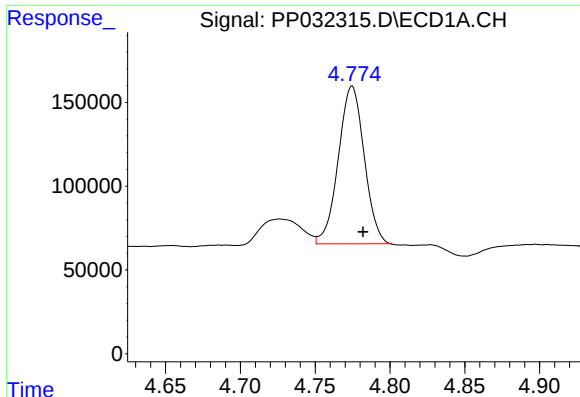


#1 Tetrachloro-m-xylene

R.T.: 4.774 min
Delta R.T.: -0.008 min
Response: 1133008
Conc: 21.99 ng/ml m

Instrument :
ECD_P
ClientSampleId :
32841


Manual Integrations
APPROVED

Ankita
12/23/2020 2:17:50 PM

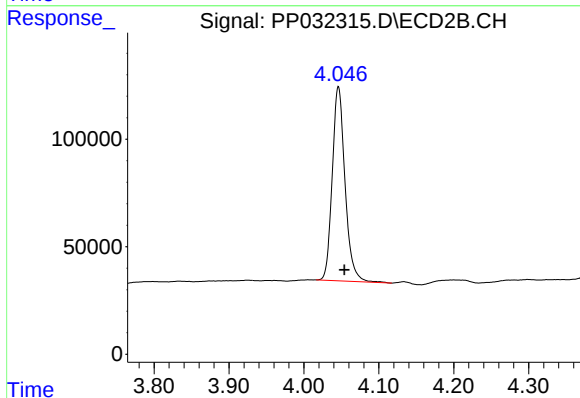


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.008 min
Response: 1070354
Conc: 22.63 ng/ml

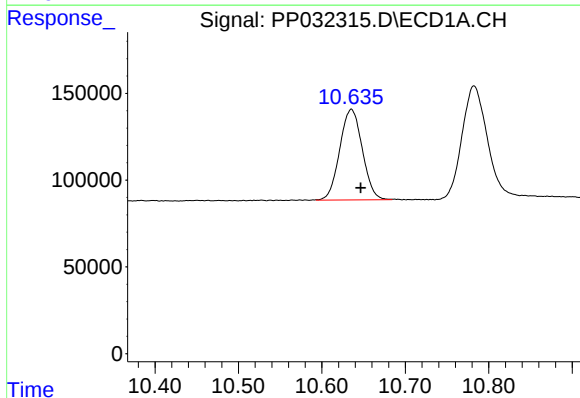

#2 Decachlorobiphenyl

R.T.: 10.635 min
Delta R.T.: -0.012 min
Response: 981412
Conc: 31.30 ng/ml m

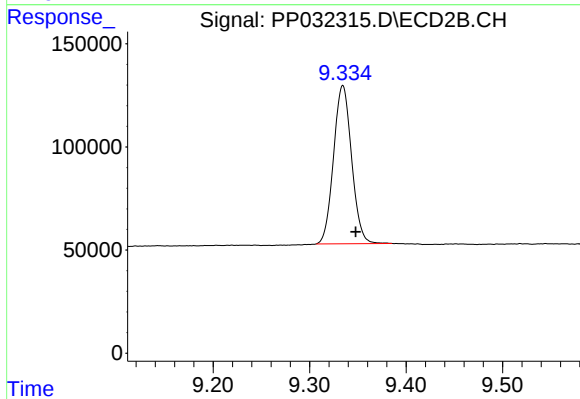

#2 Decachlorobiphenyl

R.T.: 9.334 min
Delta R.T.: -0.014 min
Response: 997259
Conc: 29.74 ng/ml