

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122220\
 Data File : PP032318.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Dec 2020 14:40
 Operator : DD\AJ
 Sample : L5159-09RE
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CGP-5RE

Manual Integrations
 APPROVED

Ankita
 12/23/2020 2:17:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 17:20:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.770	4.064	4542401	4895268	88.179m	103.502
2) SA Decachlor...	10.635	9.335	911006	907958	29.050m	27.074

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122220\
Data File : PP032318.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Dec 2020 14:40
Operator : DD\AJ
Sample : L5159-09RE
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CGP-5RE


Manual Integrations
APPROVED

Ankita
12/23/2020 2:17:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 17:20:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

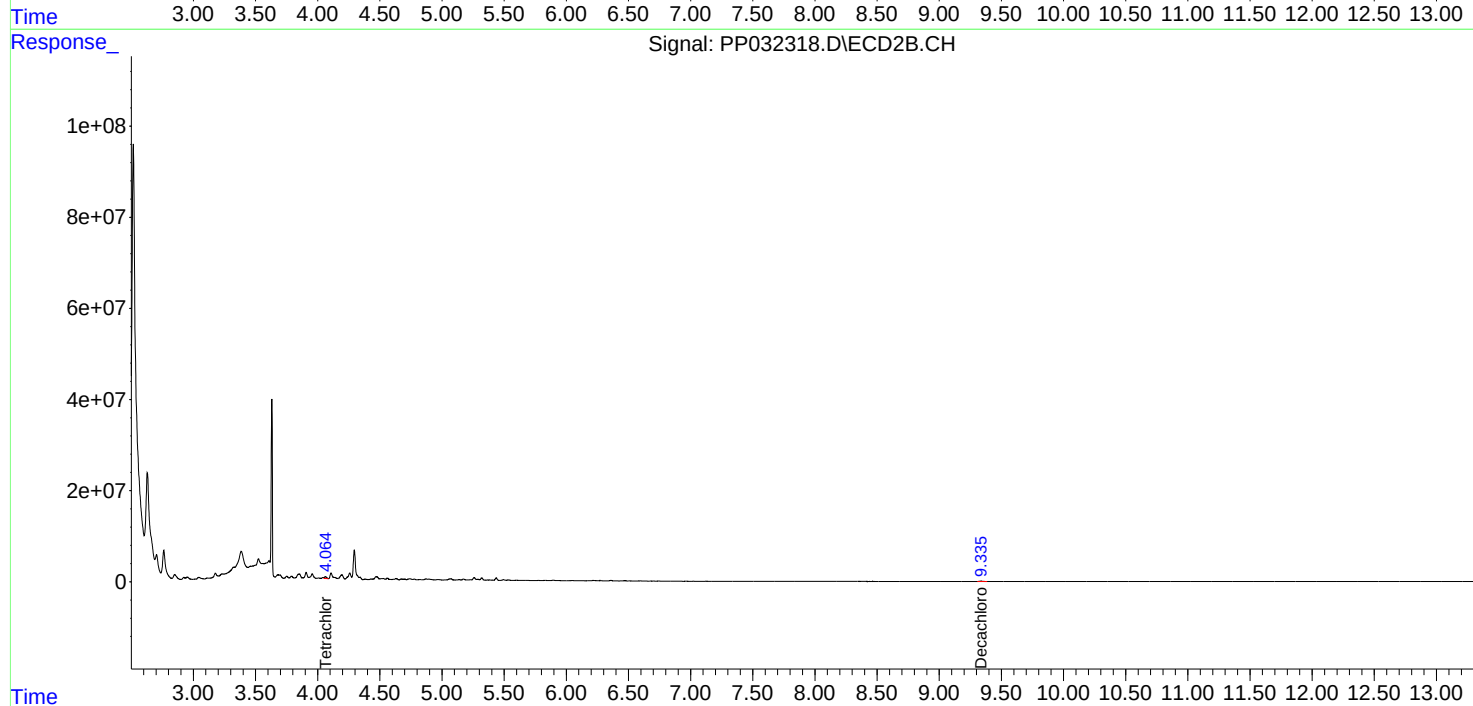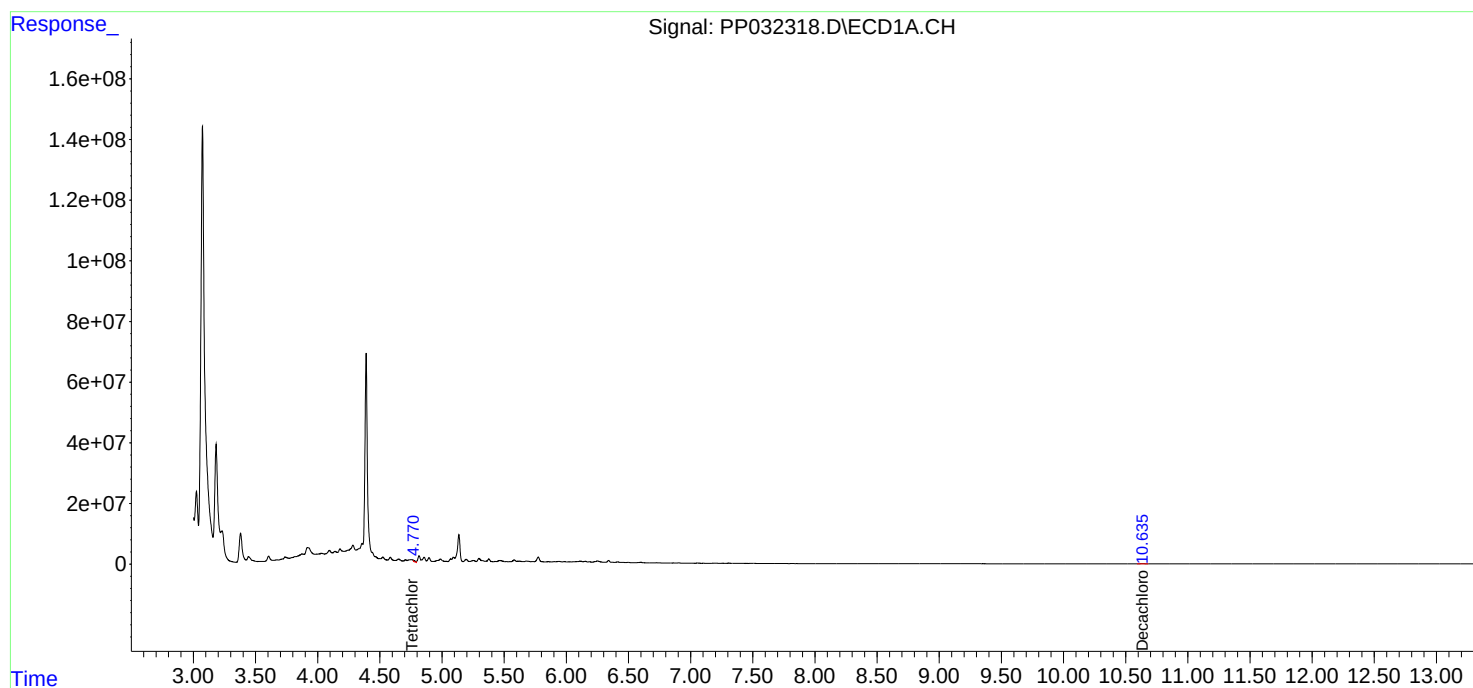

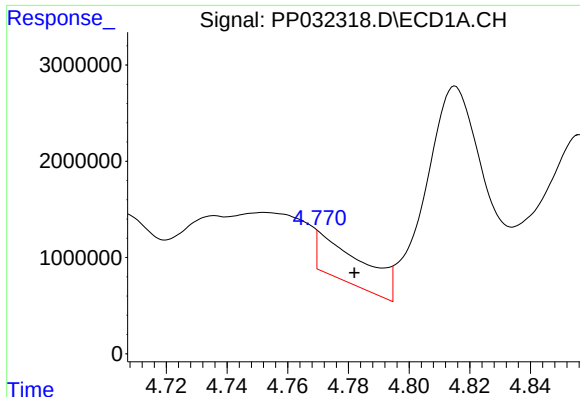


#1 Tetrachloro-m-xylene

R.T.: 4.770 min
Delta R.T.: -0.012 min
Response: 4542401
Conc: 88.18 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CGP-5RE


Manual Integrations
APPROVED

Ankita
12/23/2020 2:17:54 PM

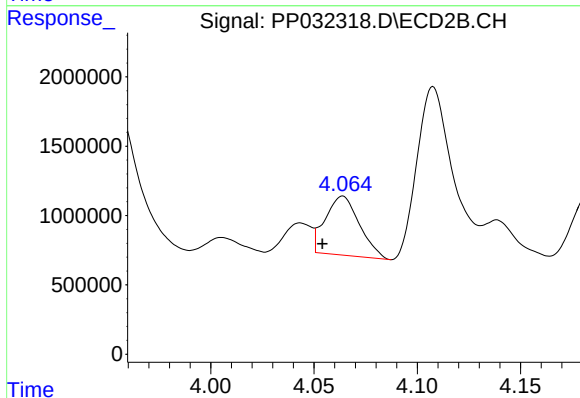


#1 Tetrachloro-m-xylene

R.T.: 4.064 min
Delta R.T.: 0.010 min
Response: 4895268
Conc: 103.50 ng/ml

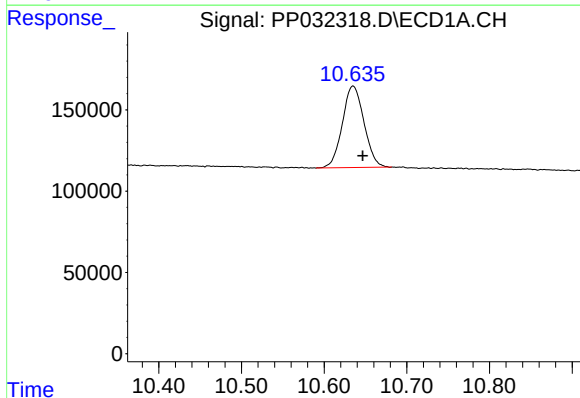

#2 Decachlorobiphenyl

R.T.: 10.635 min
Delta R.T.: -0.012 min
Response: 911006
Conc: 29.05 ng/ml m

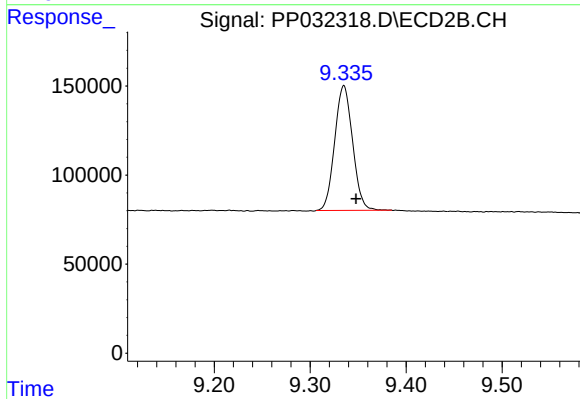

#2 Decachlorobiphenyl

R.T.: 9.335 min
Delta R.T.: -0.013 min
Response: 907958
Conc: 27.07 ng/ml