

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122220\
 Data File : PP032319.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Dec 2020 14:57
 Operator : DD\AJ
 Sample : L5159-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CGP-7

Manual Integrations
 APPROVED

Ankita
 12/23/2020 2:17:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 17:21:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.777	4.063	686323	2084915	13.323m	44.082 #
2) SA Decachlor...	10.636	9.336	870377	852598	27.755m	25.423

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122220\
Data File : PP032319.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Dec 2020 14:57
Operator : DD\AJ
Sample : L5159-13
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CGP-7


Manual Integrations
APPROVED

Ankita
12/23/2020 2:17:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 17:21:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

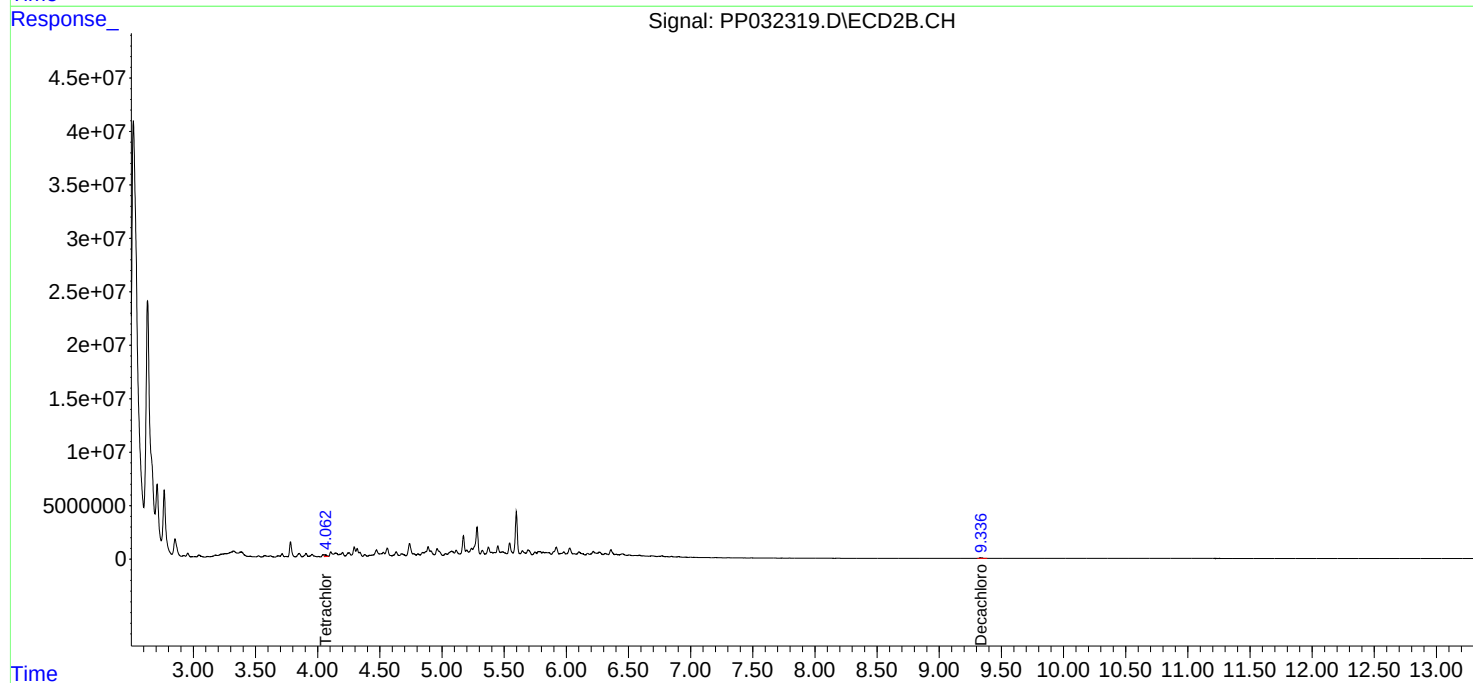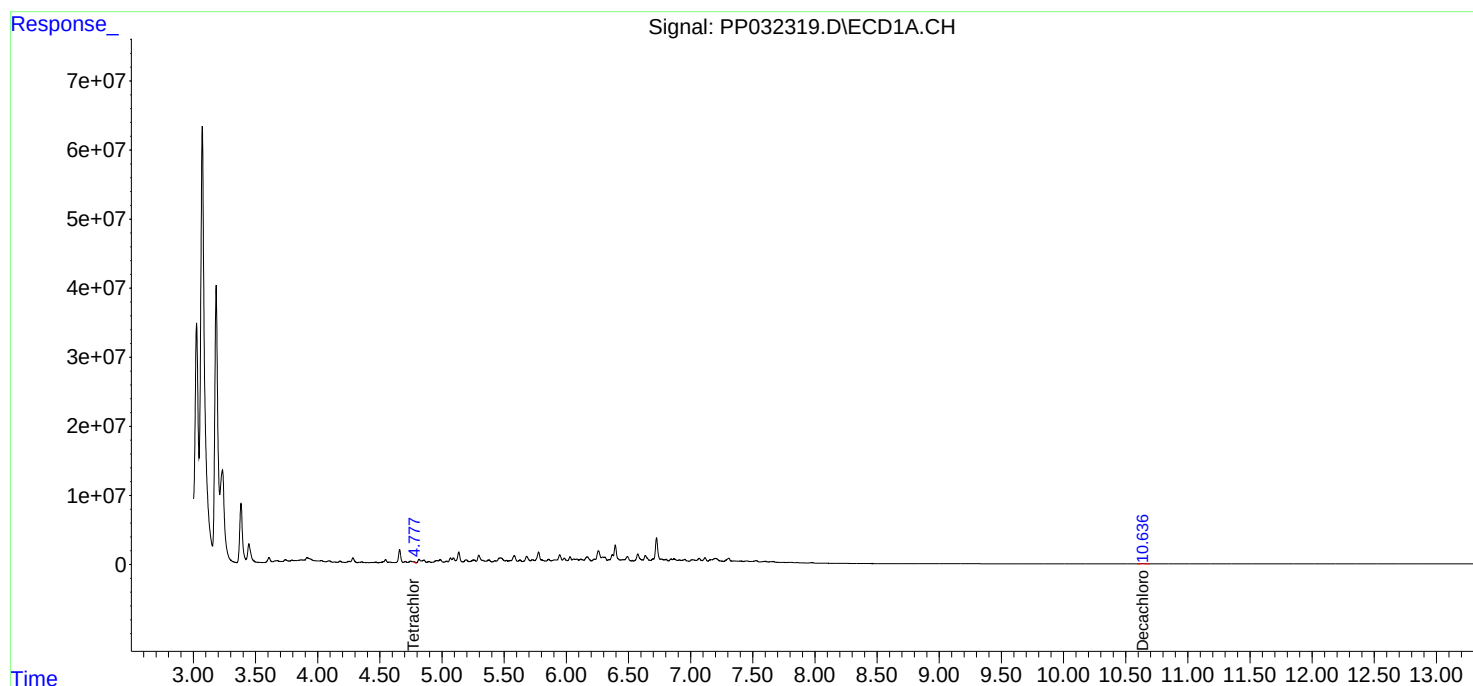

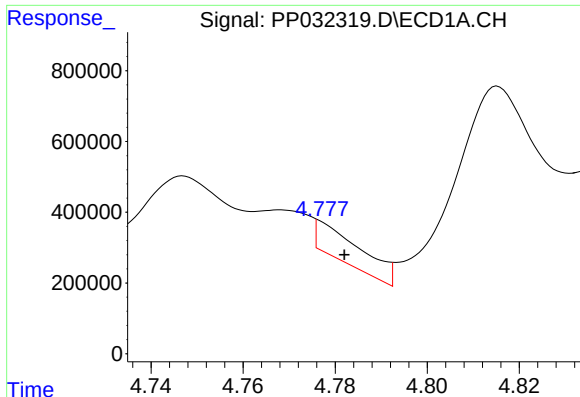


#1 Tetrachloro-m-xylene

R.T.: 4.777 min
Delta R.T.: -0.005 min
Response: 686323
Conc: 13.32 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CGP-7


Manual Integrations
APPROVED

Ankita
12/23/2020 2:17:56 PM

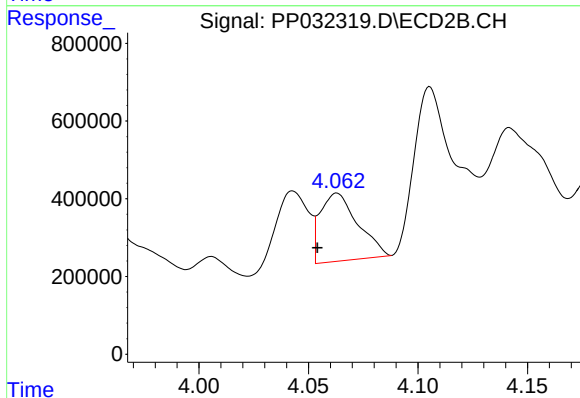


#1 Tetrachloro-m-xylene

R.T.: 4.063 min
Delta R.T.: 0.009 min
Response: 2084915
Conc: 44.08 ng/ml

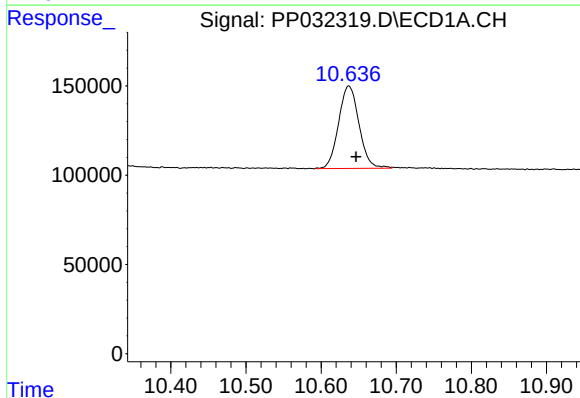

#2 Decachlorobiphenyl

R.T.: 10.636 min
Delta R.T.: -0.010 min
Response: 870377
Conc: 27.75 ng/ml m

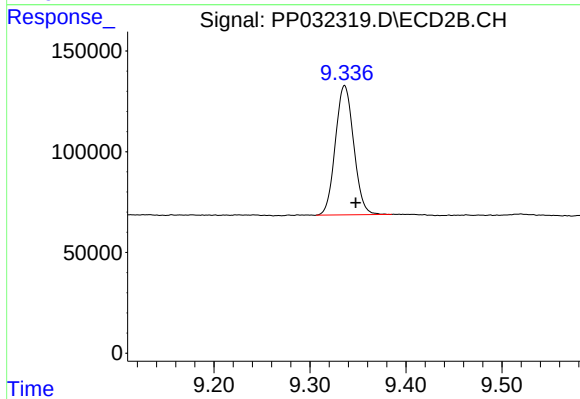

#2 Decachlorobiphenyl

R.T.: 9.336 min
Delta R.T.: -0.012 min
Response: 852598
Conc: 25.42 ng/ml