

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122220\
 Data File : PP032353.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Dec 2020 00:26
 Operator : DD\AJ
 Sample : L5178-01
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VERONA-236129

Manual Integrations
 APPROVED

Ankita
 12/23/2020 2:57:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 09:29:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.794	4.071f	961607	856976	18.667m	18.119
2) SA Decachlor...	10.641	9.337	680322	739821	21.694	22.060

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122220\
Data File : PP032353.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Dec 2020 00:26
Operator : DD\AJ
Sample : L5178-01
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VERONA-236129


Manual Integrations
APPROVED

Ankita
12/23/2020 2:57:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 09:29:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

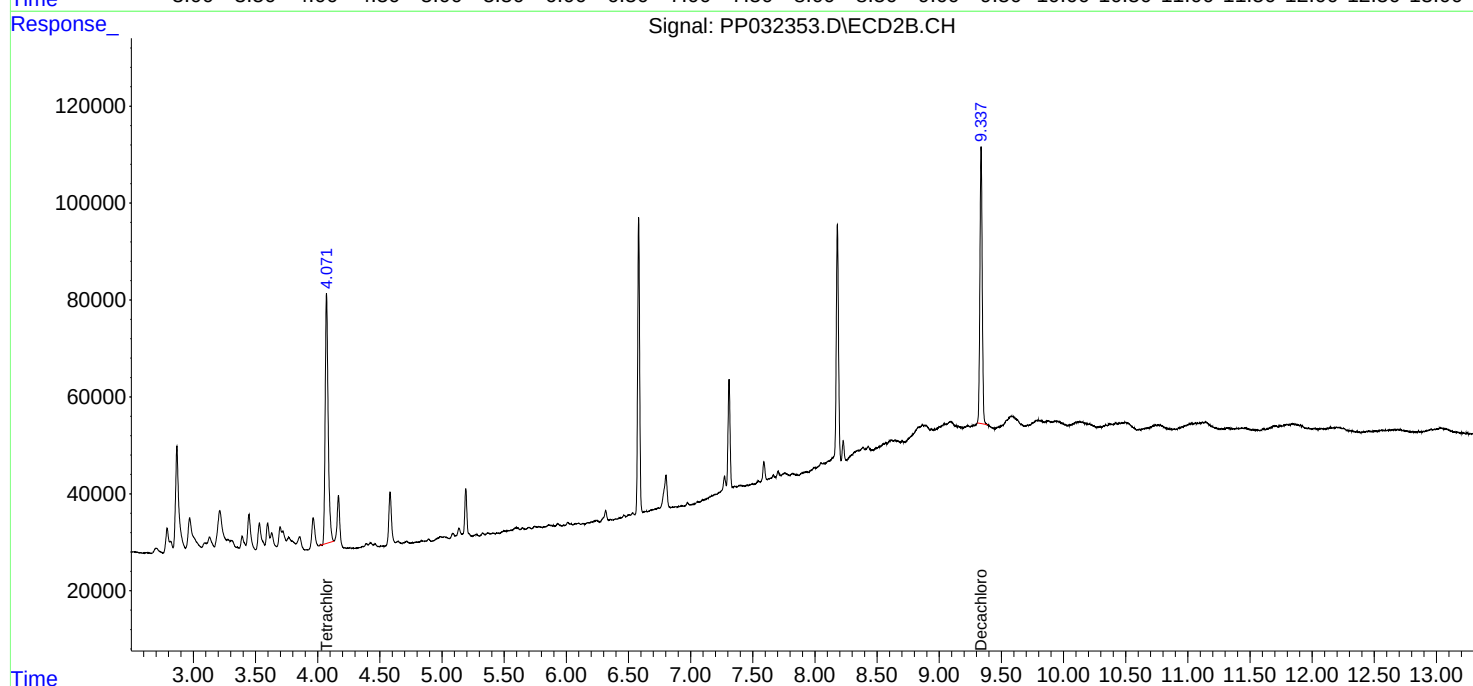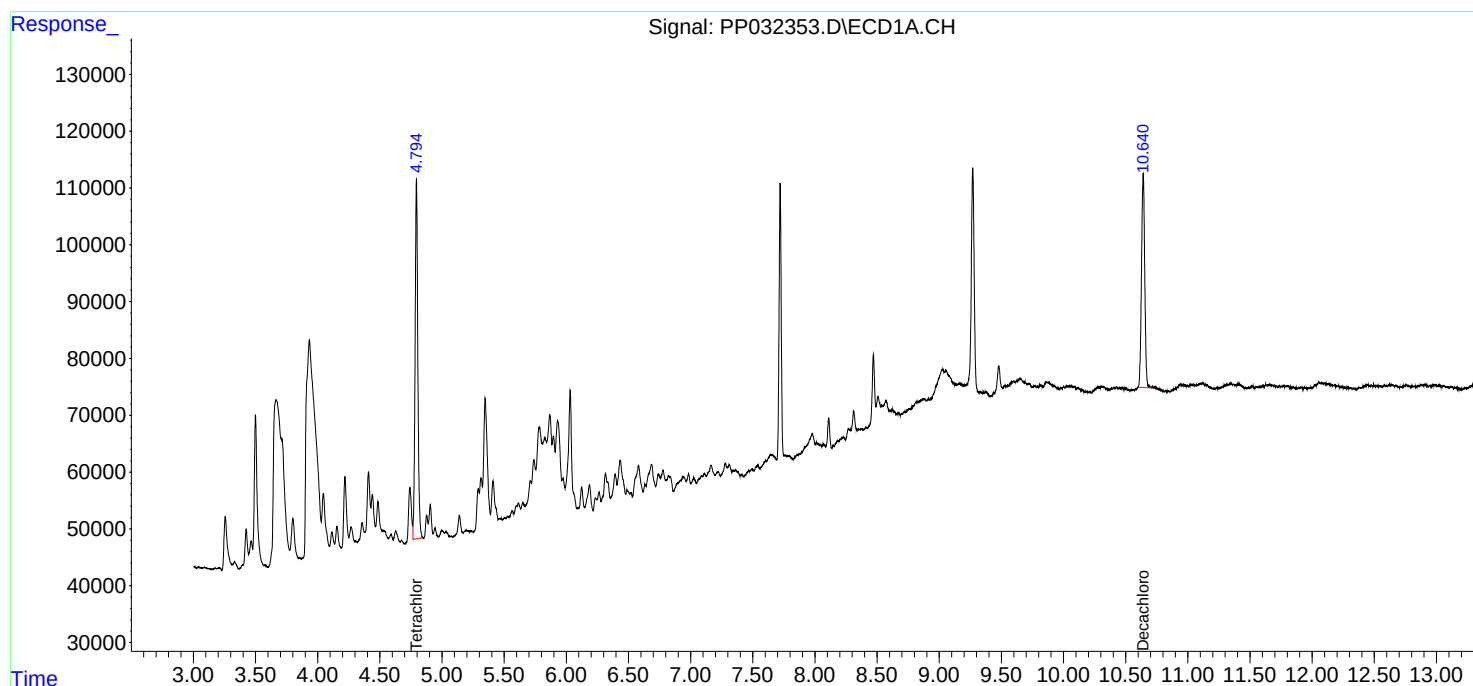

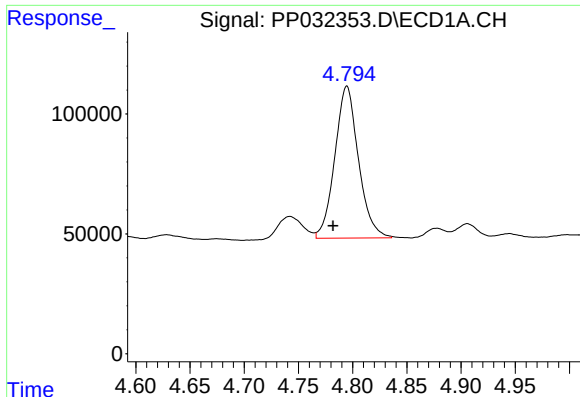


#1 Tetrachloro-m-xylene

R.T.: 4.794 min
Delta R.T.: 0.012 min
Response: 961607
Conc: 18.67 ng/ml m

Instrument :
ECD_P
ClientSampleId :
VERONA-236129


Manual Integrations
APPROVED

Ankita
12/23/2020 2:57:20 PM

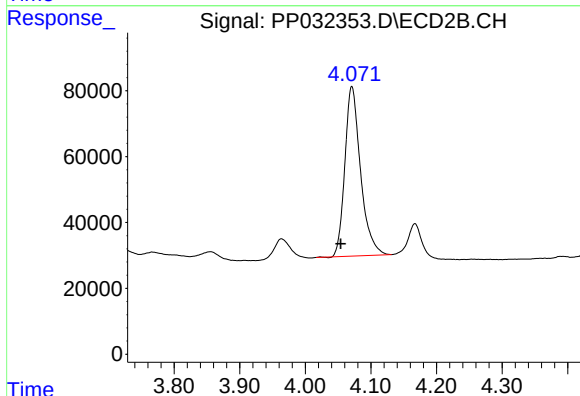


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.017 min
Response: 856976
Conc: 18.12 ng/ml

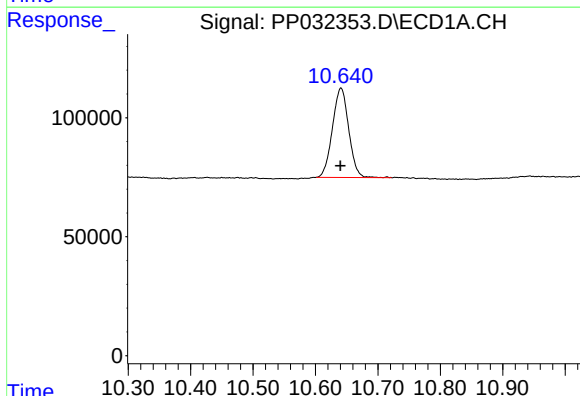

#2 Decachlorobiphenyl

R.T.: 10.641 min
Delta R.T.: 0.000 min
Response: 680322
Conc: 21.69 ng/ml

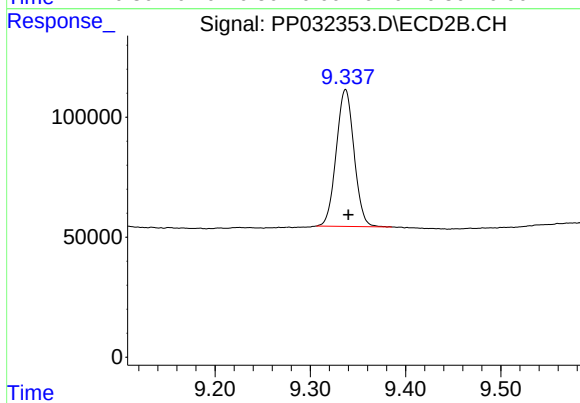

#2 Decachlorobiphenyl

R.T.: 9.337 min
Delta R.T.: -0.003 min
Response: 739821
Conc: 22.06 ng/ml