

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122222\
 Data File : PP053967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2022 19:13
 Operator : YP\AJ
 Sample : N6088-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EB-2022-12-15

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/23/2022
 Supervised By :Ankita Jodhani 12/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 20:55:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 14 05:38:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.597	32640520	20297930	15.545	12.997m
2) SA Decachlor...	10.103	8.623	30216052	23611161	17.797	16.904

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122222\
Data File : PP053967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2022 19:13
Operator : YP\AJ
Sample : N6088-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
EB-2022-12-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/23/2022
Supervised By :Ankita Jodhani 12/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 20:55:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 14 05:38:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

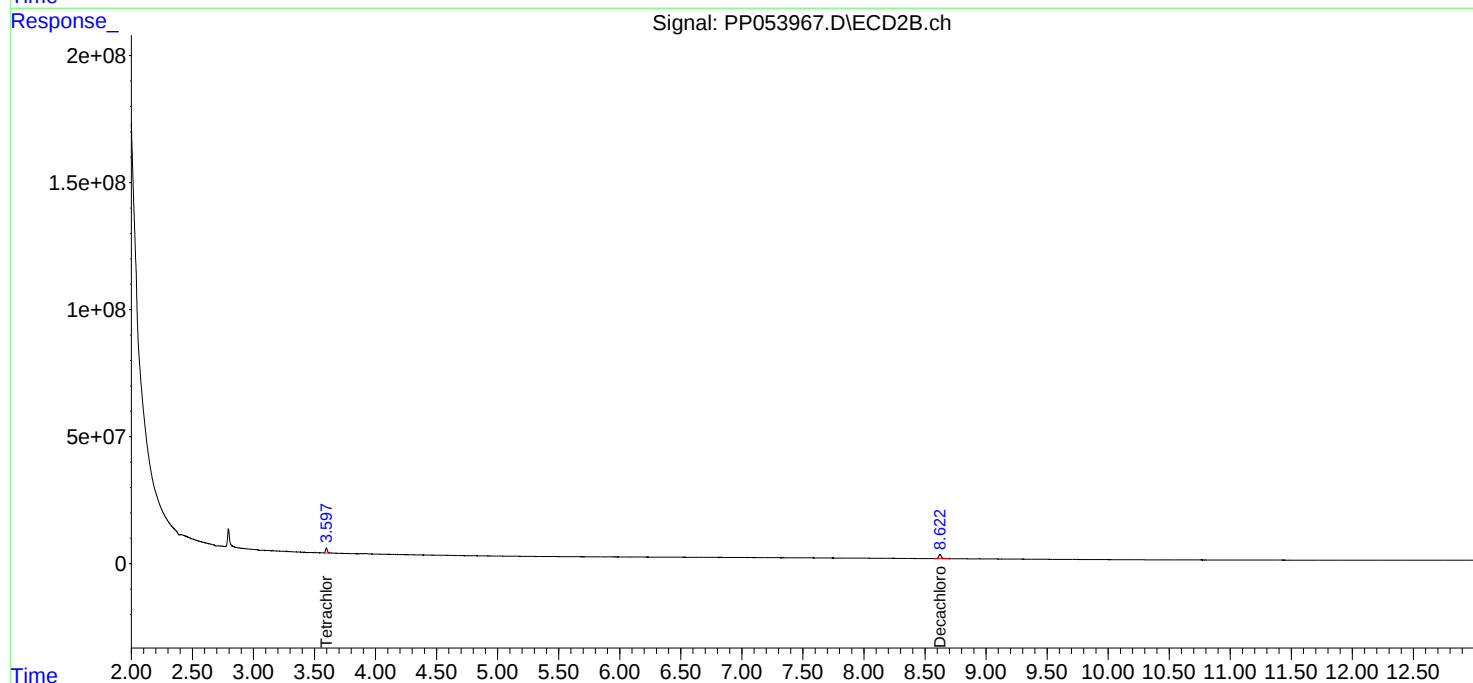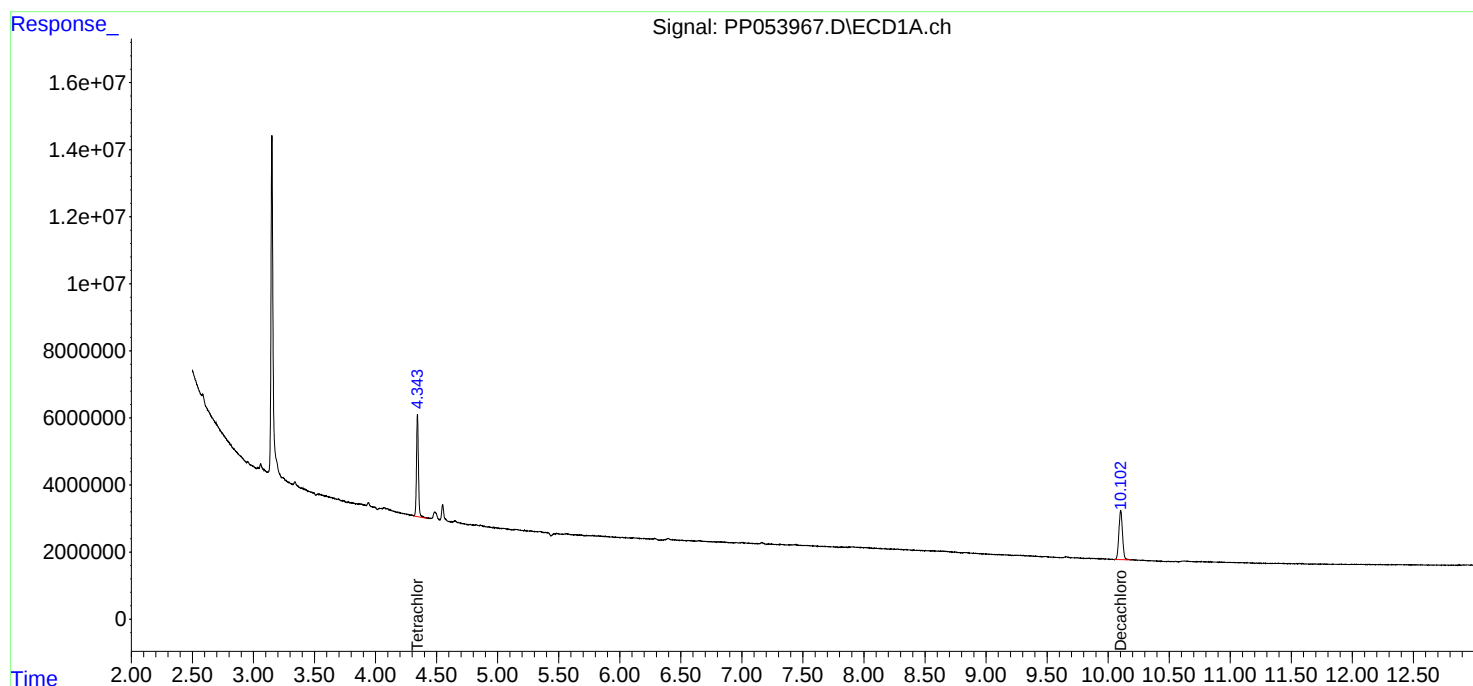

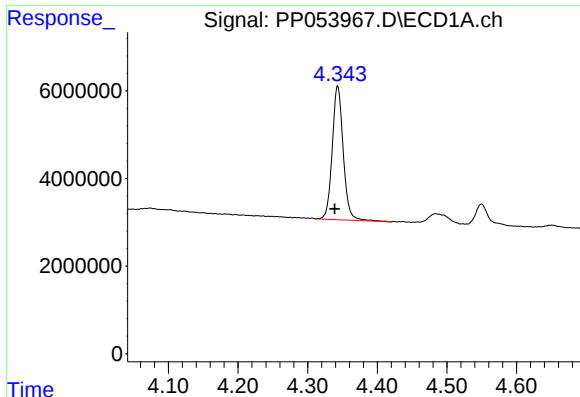


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: 0.004 min
Response: 32640520
Conc: 15.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
EB-2022-12-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/23/2022
Supervised By :Ankita Jodhani 12/23/2022

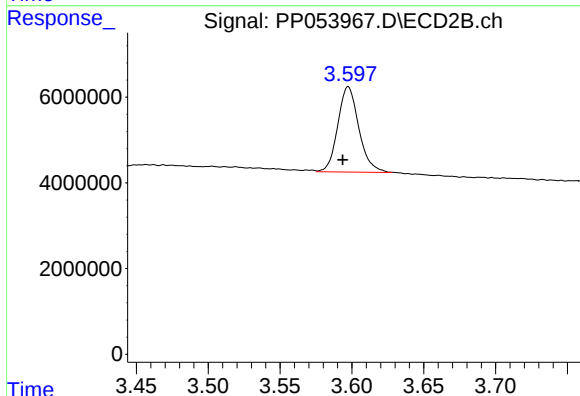


#1 Tetrachloro-m-xylene

R.T.: 3.597 min
Delta R.T.: 0.004 min
Response: 20297930
Conc: 13.00 ng/ml m

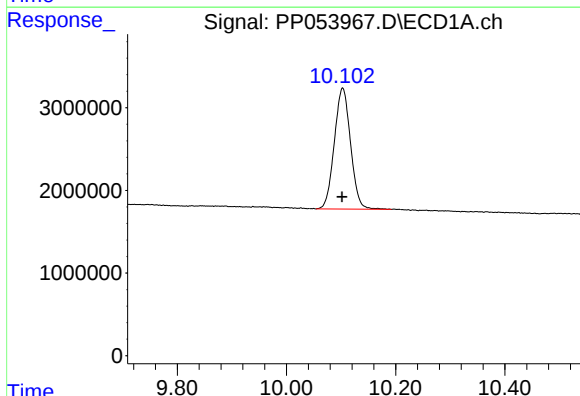

#2 Decachlorobiphenyl

R.T.: 10.103 min
Delta R.T.: 0.000 min
Response: 30216052
Conc: 17.80 ng/ml

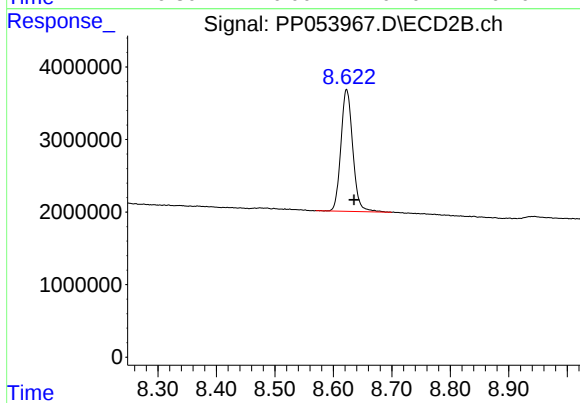

#2 Decachlorobiphenyl

R.T.: 8.623 min
Delta R.T.: -0.013 min
Response: 23611161
Conc: 16.90 ng/ml