

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122322\
 Data File : PP054026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 21:14
 Operator : YP\AJ
 Sample : N6197-02 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2022-59B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/27/2022
 Supervised By :Ankita Jodhani 12/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 06:32:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 14 05:38:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.589	4053204	2710981	1.930	1.736
2) SA Decachlor...	10.110	8.628	3624156	2843182	2.135m	2.036

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122322\
Data File : PP054026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 21:14
Operator : YP\AJ
Sample : N6197-02 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LAW-2022-59B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2022
Supervised By :Ankita Jodhani 12/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 06:32:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 14 05:38:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

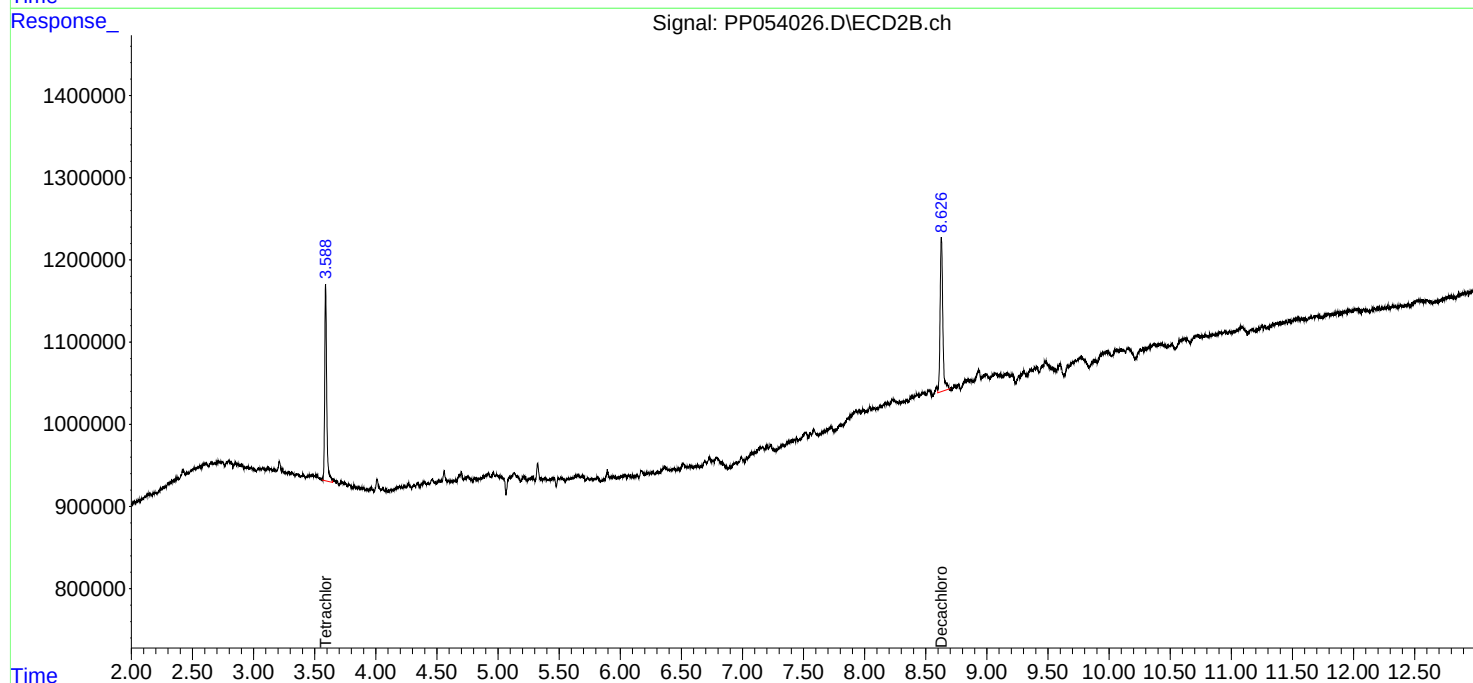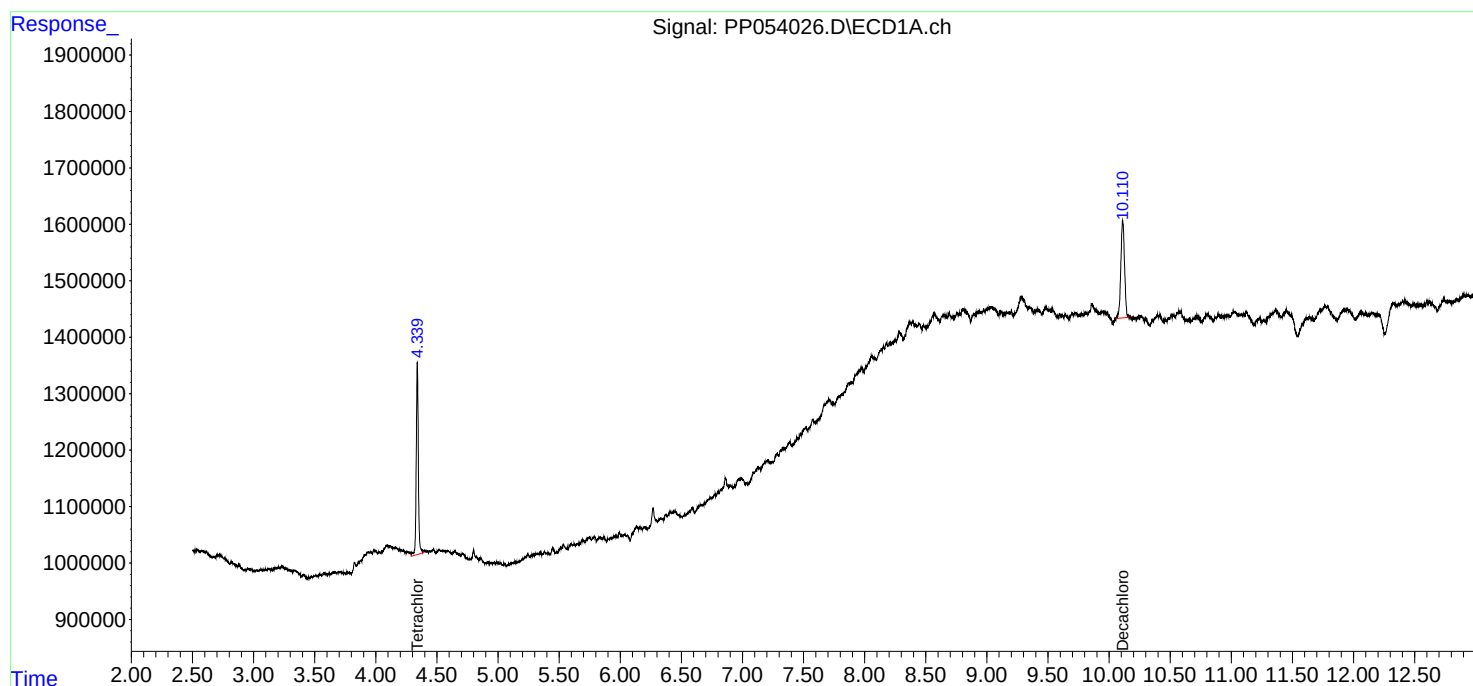

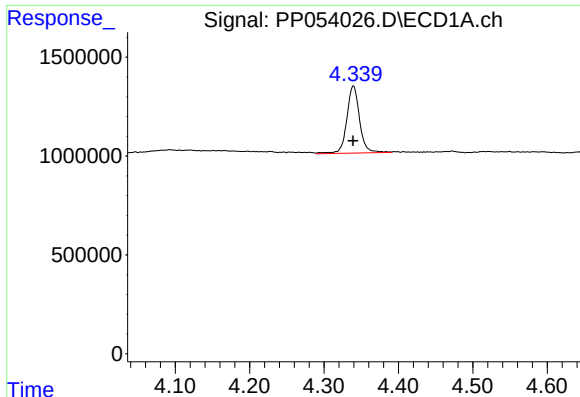


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 4053204
Conc: 1.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-59B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2022
Supervised By :Ankita Jodhani 12/27/2022

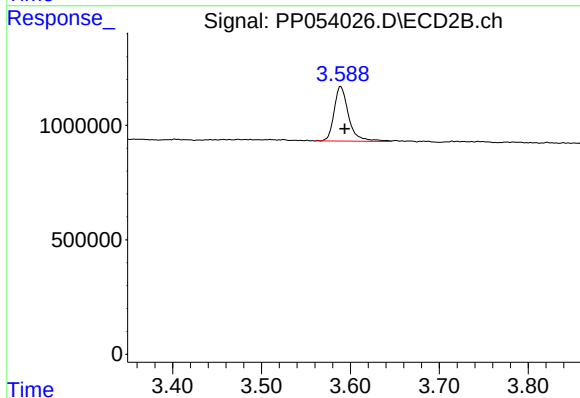


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.005 min
Response: 2710981
Conc: 1.74 ng/ml

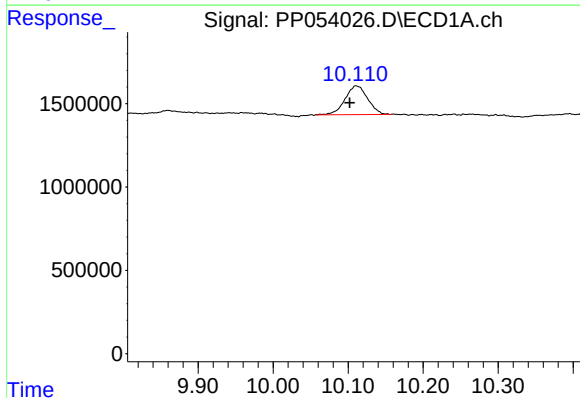

#2 Decachlorobiphenyl

R.T.: 10.110 min
Delta R.T.: 0.008 min
Response: 3624156
Conc: 2.13 ng/ml m

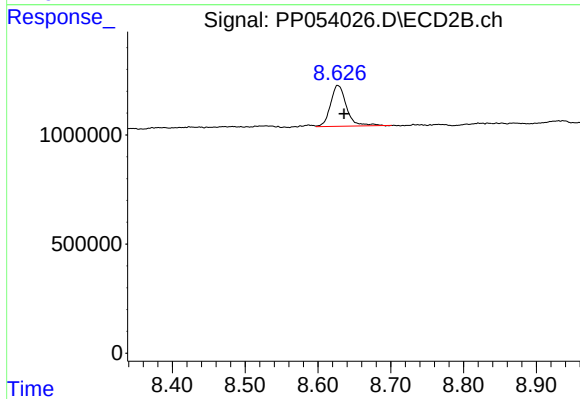

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: -0.008 min
Response: 2843182
Conc: 2.04 ng/ml