

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122322\
 Data File : PP054027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 21:31
 Operator : YP\AJ
 Sample : N6197-03 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2022-60A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 06:33:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 14 05:38:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.340	3.589	4128759	2301322	1.966	1.474 #
2) SA Decachlor...	10.115	8.633	3364796	2529071	1.982	1.811
Target Compounds						
26) L6 AR-1254-1	6.372	5.487	138.9E6	126.8E6	1792.298	1935.619
27) L6 AR-1254-2	6.592	5.635	209.2E6	110.9E6	1798.101	1901.795
28) L6 AR-1254-3	6.959	6.041	207.4E6	166.7E6	1771.099	1894.654
29) L6 AR-1254-4	7.247	6.271	150.0E6	94926942	1891.812	2071.961
30) L6 AR-1254-5	7.668	6.691	178.9E6	154.4E6	1833.968	1981.682



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122322\
Data File : PP054027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 21:31
Operator : YP\AJ
Sample : N6197-03 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 06:33:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 14 05:38:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

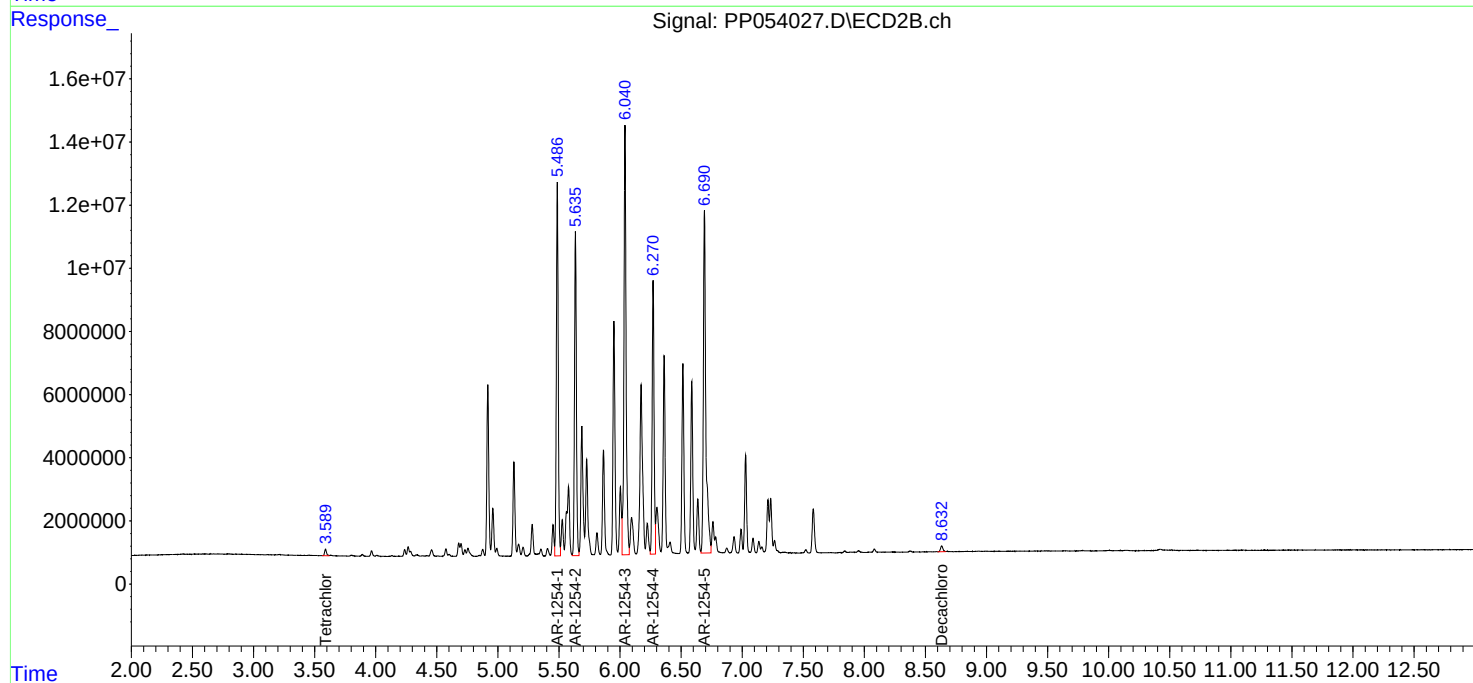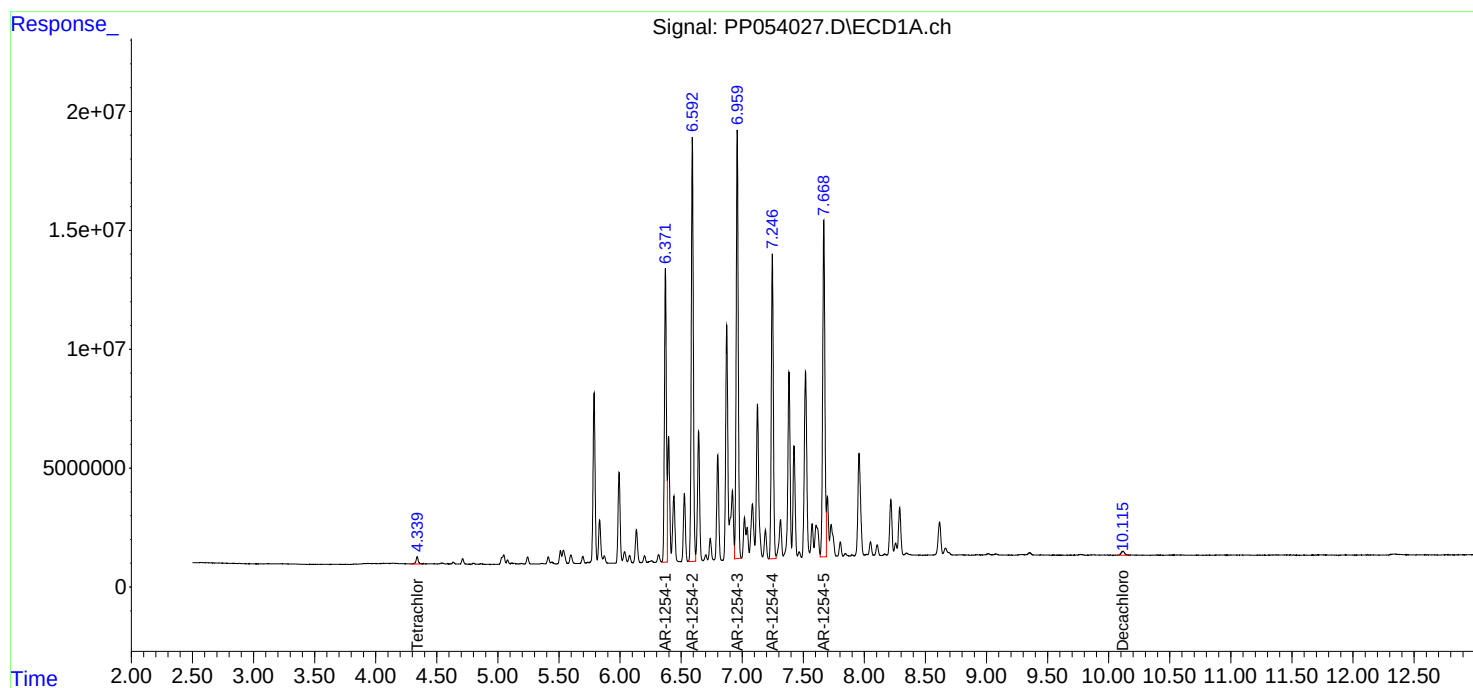


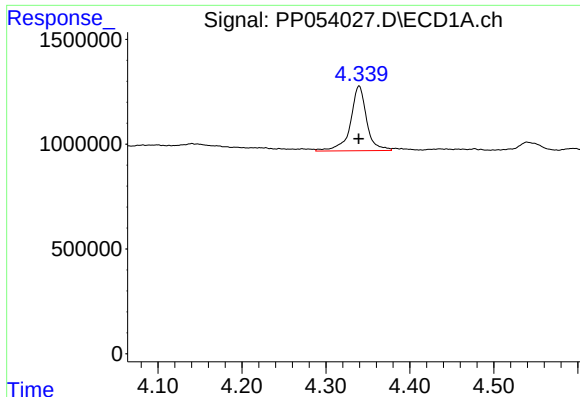

#1 Tetrachloro-m-xylene


R.T.: 4.340 min
Delta R.T.: 0.000 min
Response: 4128759
Conc: 1.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

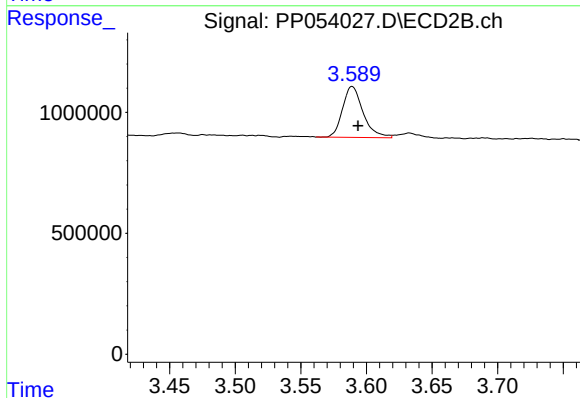


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 2301322
Conc: 1.47 ng/ml

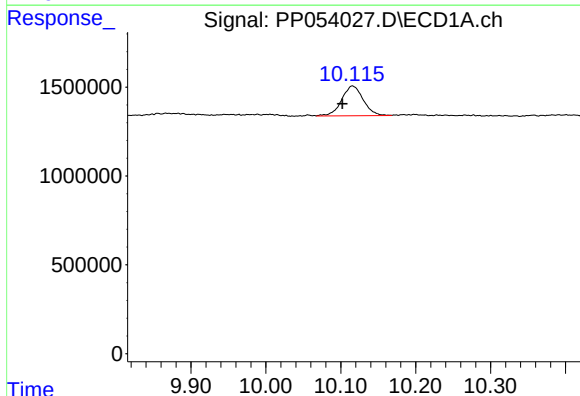


#2 Decachlorobiphenyl

R.T.: 10.115 min
Delta R.T.: 0.013 min
Response: 3364796
Conc: 1.98 ng/ml

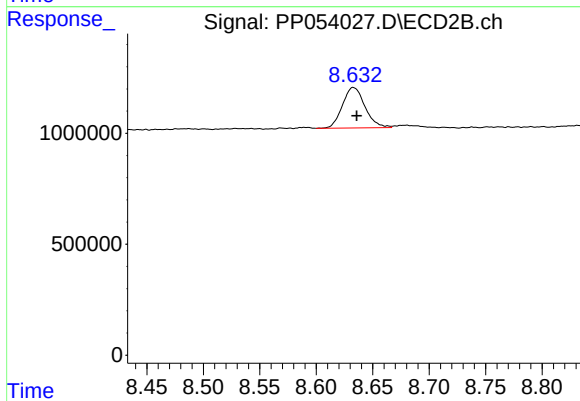

#2 Decachlorobiphenyl


R.T.: 8.633 min
Delta R.T.: -0.003 min
Response: 2529071
Conc: 1.81 ng/ml

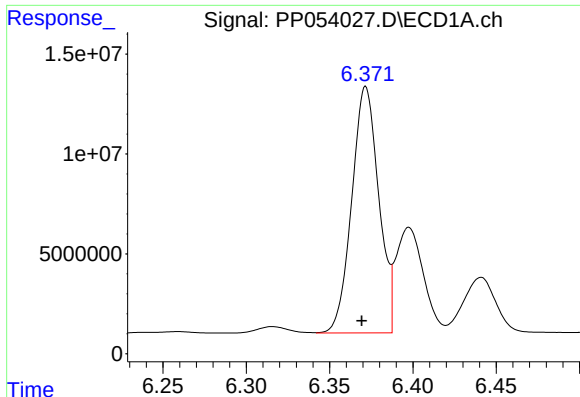

#26 AR-1254-1


R.T.: 6.372 min
Delta R.T.: 0.002 min
Response: 138889598
Conc: 1792.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

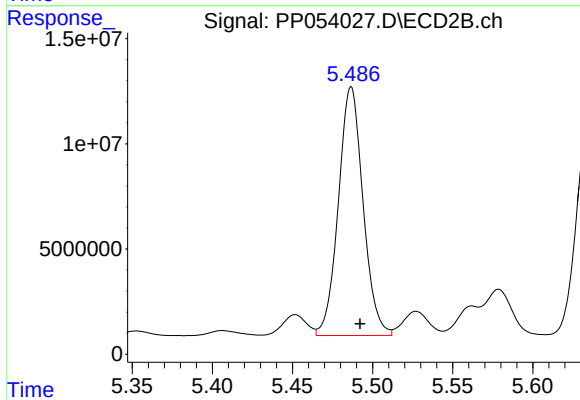


#26 AR-1254-1

R.T.: 5.487 min
Delta R.T.: -0.005 min
Response: 126750800
Conc: 1935.62 ng/ml

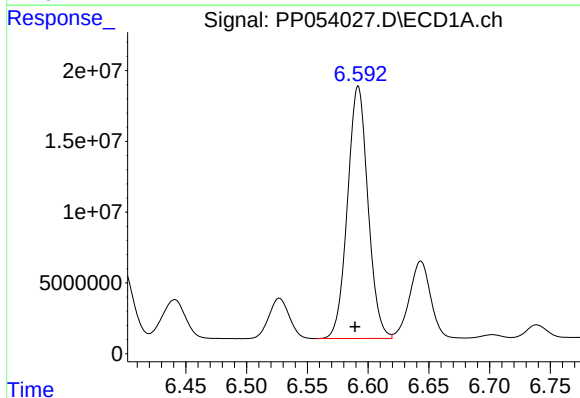


#27 AR-1254-2

R.T.: 6.592 min
Delta R.T.: 0.003 min
Response: 209203198
Conc: 1798.10 ng/ml

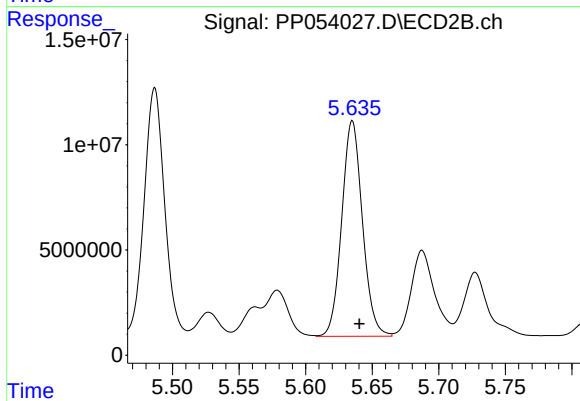

#27 AR-1254-2


R.T.: 5.635 min
Delta R.T.: -0.005 min
Response: 110911996
Conc: 1901.79 ng/ml

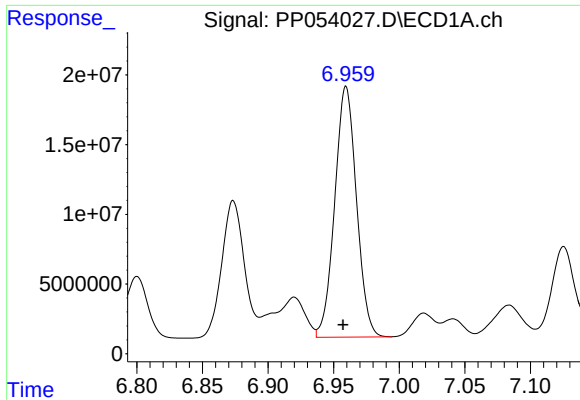

#28 AR-1254-3


R.T.: 6.959 min
Delta R.T.: 0.002 min
Response: 207444289
Conc: 1771.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

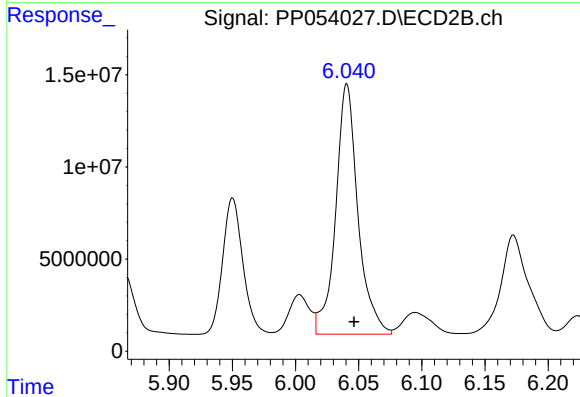


#28 AR-1254-3

R.T.: 6.041 min
Delta R.T.: -0.006 min
Response: 166676481
Conc: 1894.65 ng/ml

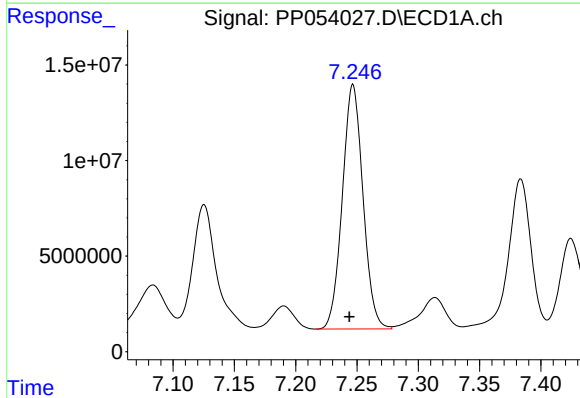


#29 AR-1254-4

R.T.: 7.247 min
Delta R.T.: 0.003 min
Response: 149979369
Conc: 1891.81 ng/ml

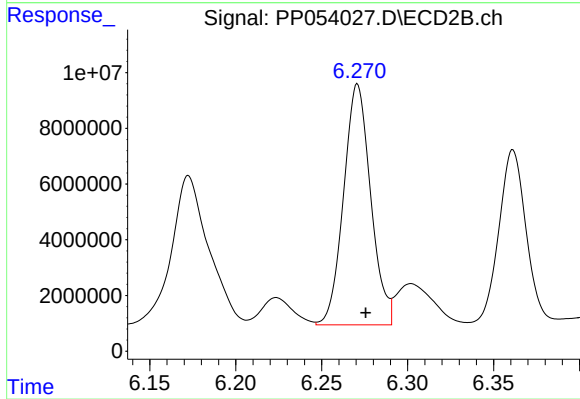

#29 AR-1254-4


R.T.: 6.271 min
Delta R.T.: -0.005 min
Response: 94926942
Conc: 2071.96 ng/ml

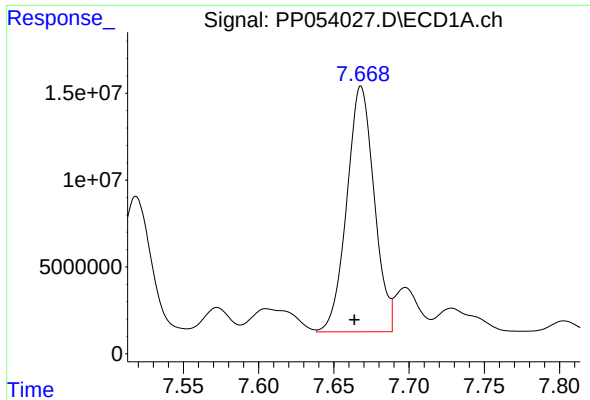

#30 AR-1254-5

R.T.: 7.668 min
Delta R.T.: 0.004 min
Response: 178857596
Conc: 1833.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

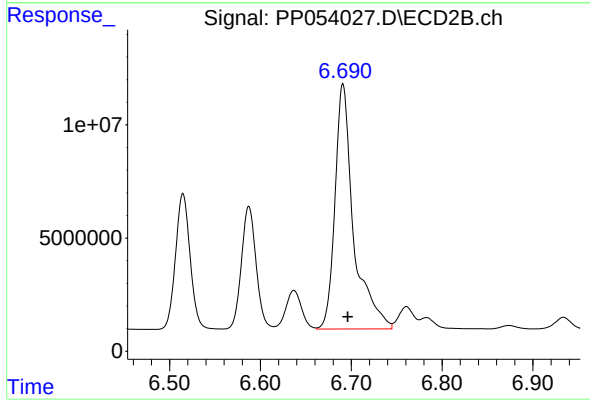

#30 AR-1254-5

R.T.: 6.691 min
Delta R.T.: -0.005 min
Response: 154439972
Conc: 1981.68 ng/ml