

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122322\
 Data File : PP054038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2022 01:13
 Operator : YP\AJ
 Sample : N6197-09 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2022-63A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 06:44:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 14 05:38:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.589	4100548	2446469	1.953	1.567
2) SA Decachlor...	10.110	8.627	3566093	2661537	2.100	1.906
Target Compounds						
26) L6 AR-1254-1	6.370	5.486	66826600	60750744	862.363	927.728
27) L6 AR-1254-2	6.591	5.634	98871836	54100815	849.803	927.660
28) L6 AR-1254-3	6.958	6.040	97228015	79137134	830.105	899.572
29) L6 AR-1254-4	7.245	6.269	70804605	44770039	893.116	977.191
30) L6 AR-1254-5	7.666	6.689	98677776	72892962	1011.821	935.319



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122322\
Data File : PP054038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2022 01:13
Operator : YP\AJ
Sample : N6197-09 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2022-63A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 06:44:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 14 05:38:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

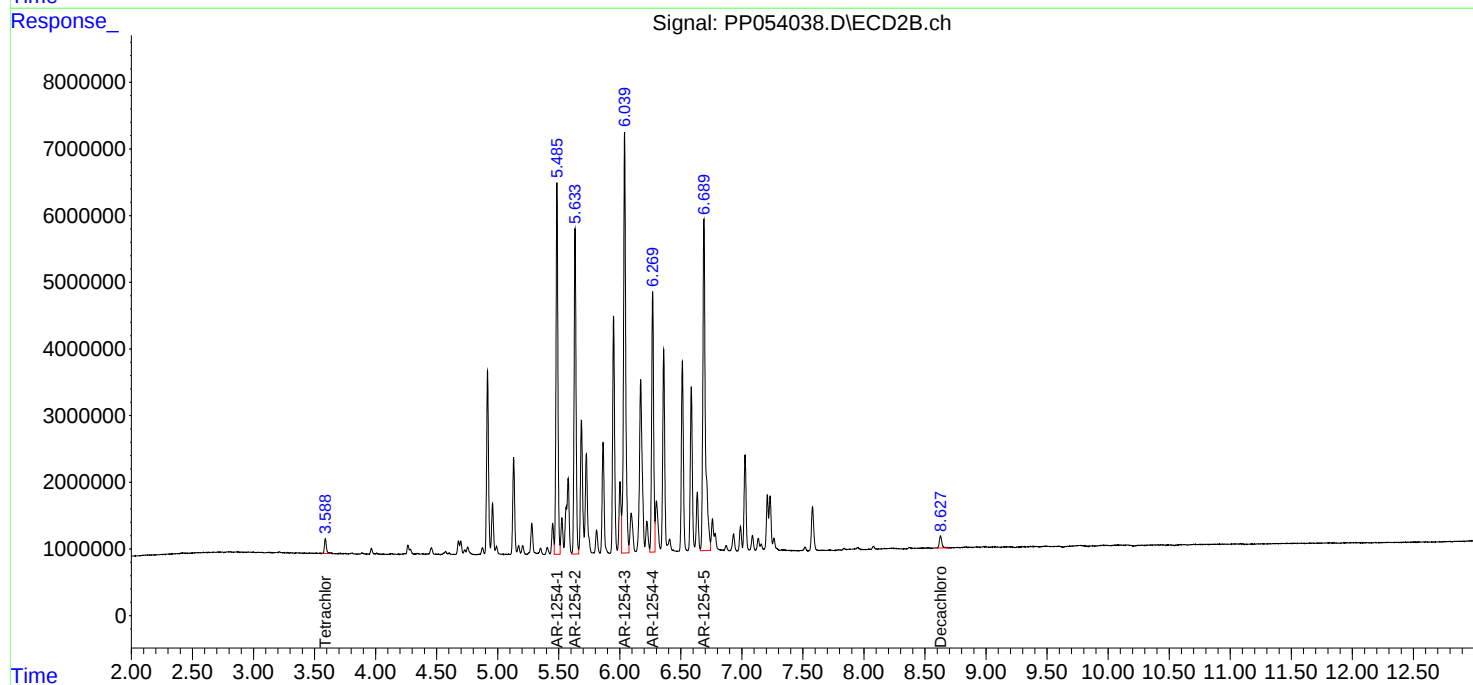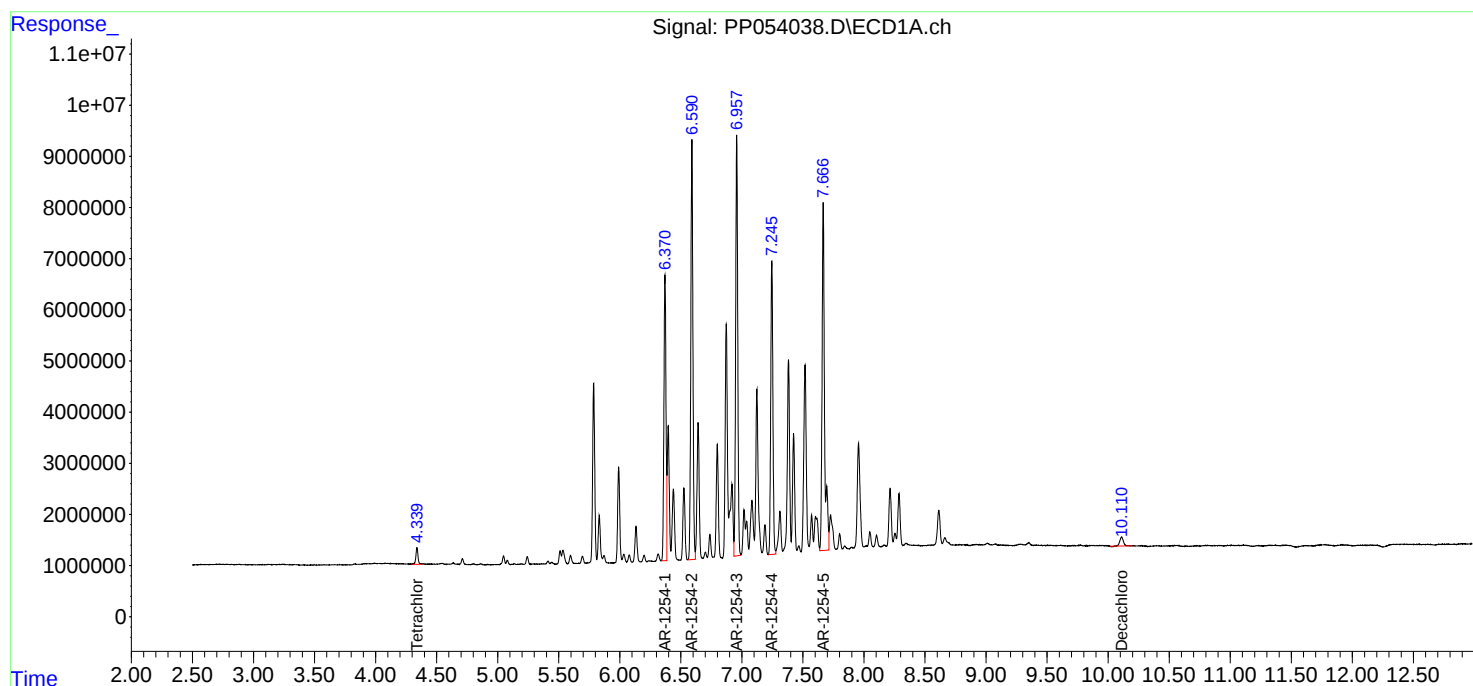


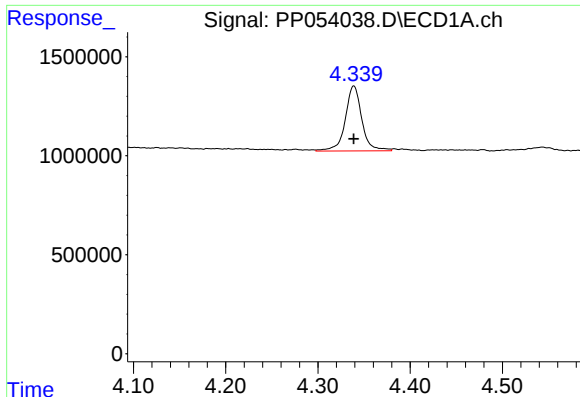

#1 Tetrachloro-m-xylene


R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 4100548
Conc: 1.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-63A

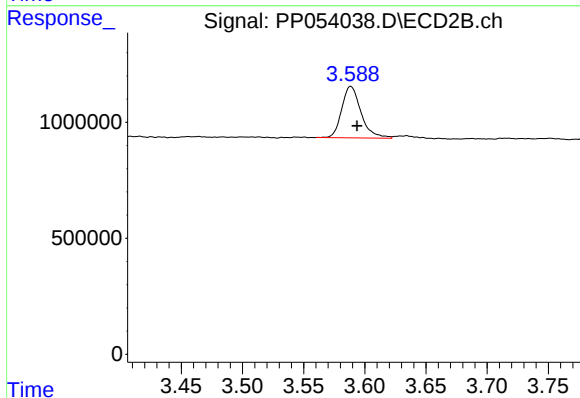


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.005 min
Response: 2446469
Conc: 1.57 ng/ml

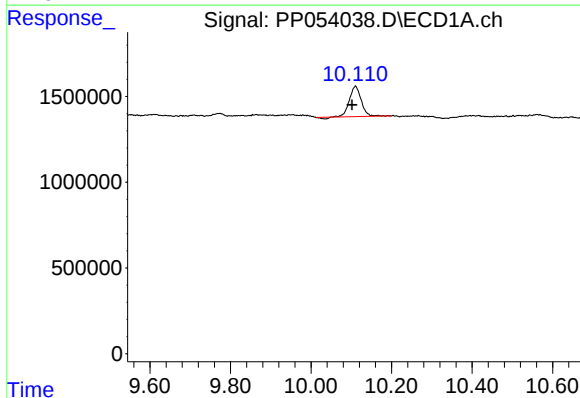


#2 Decachlorobiphenyl

R.T.: 10.110 min
Delta R.T.: 0.008 min
Response: 3566093
Conc: 2.10 ng/ml

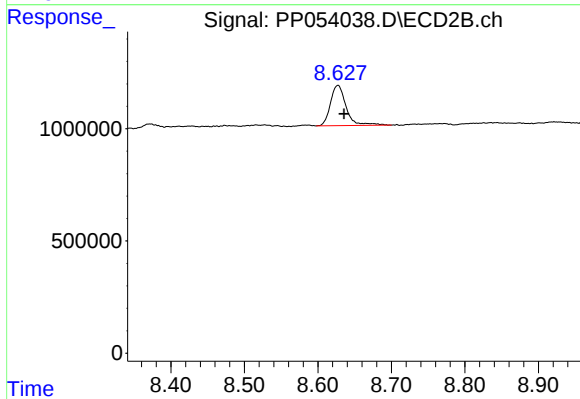

#2 Decachlorobiphenyl


R.T.: 8.627 min
Delta R.T.: -0.008 min
Response: 2661537
Conc: 1.91 ng/ml

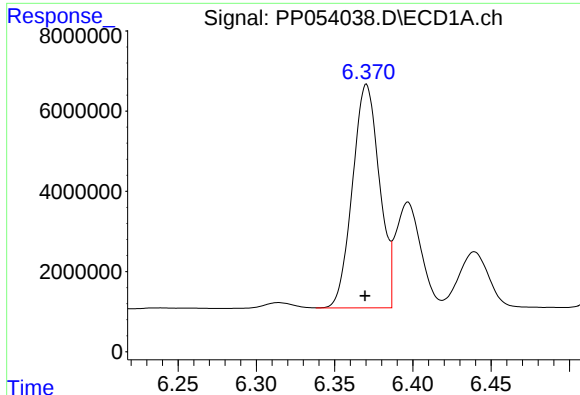

#26 AR-1254-1


R.T.: 6.370 min
Delta R.T.: 0.001 min
Response: 66826600
Conc: 862.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-63A

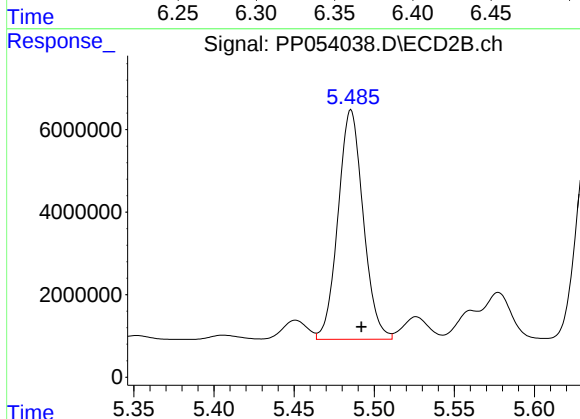


#26 AR-1254-1

R.T.: 5.486 min
Delta R.T.: -0.007 min
Response: 60750744
Conc: 927.73 ng/ml

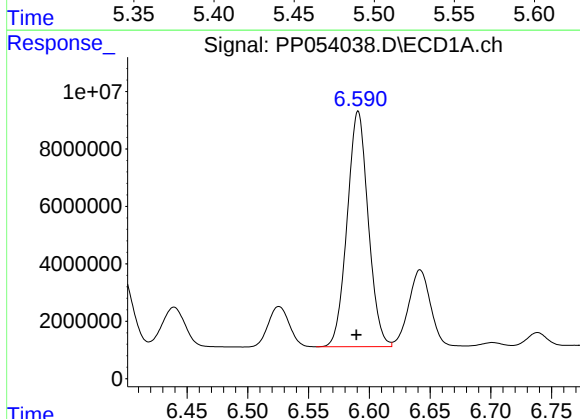


#27 AR-1254-2

R.T.: 6.591 min
Delta R.T.: 0.001 min
Response: 98871836
Conc: 849.80 ng/ml

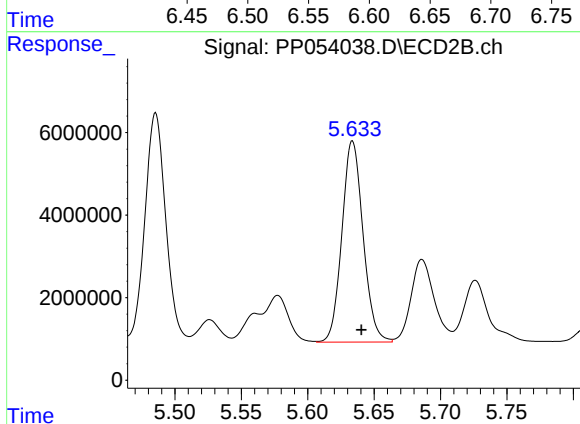

#27 AR-1254-2


R.T.: 5.634 min
Delta R.T.: -0.007 min
Response: 54100815
Conc: 927.66 ng/ml

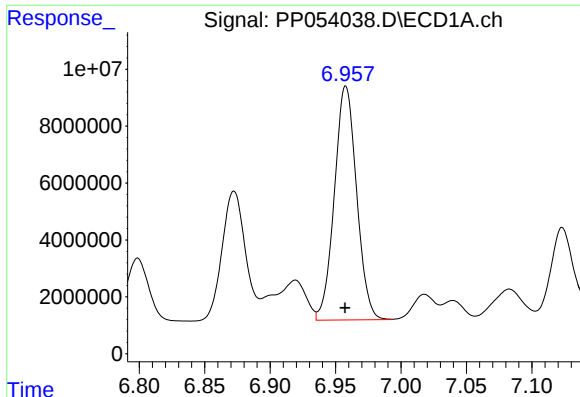

#28 AR-1254-3


R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 97228015
Conc: 830.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-63A

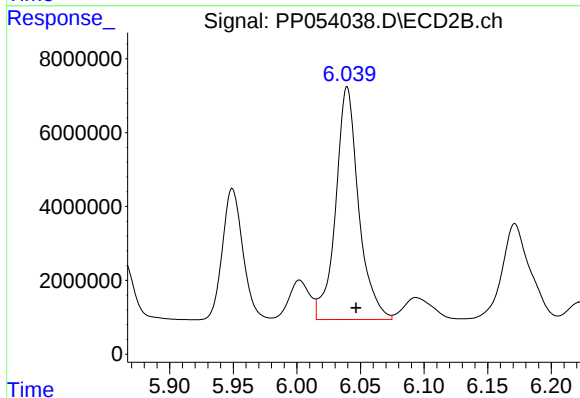


#28 AR-1254-3

R.T.: 6.040 min
Delta R.T.: -0.007 min
Response: 79137134
Conc: 899.57 ng/ml

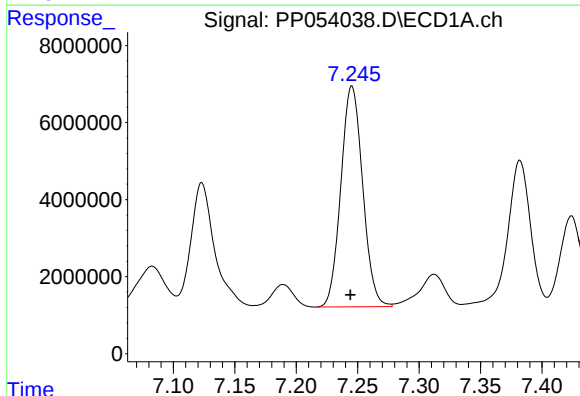


#29 AR-1254-4

R.T.: 7.245 min
Delta R.T.: 0.001 min
Response: 70804605
Conc: 893.12 ng/ml

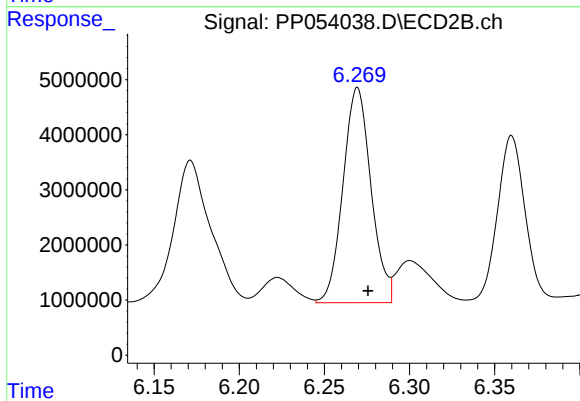

#29 AR-1254-4


R.T.: 6.269 min
Delta R.T.: -0.006 min
Response: 44770039
Conc: 977.19 ng/ml

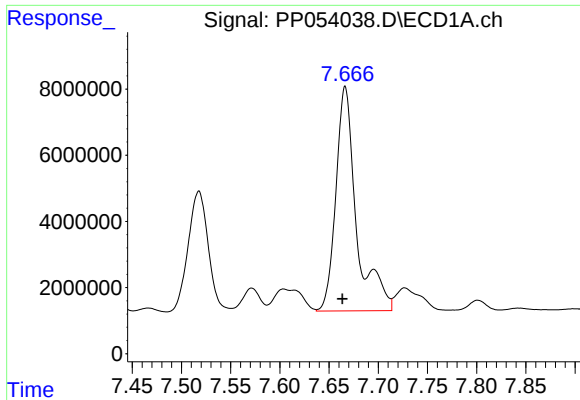

#30 AR-1254-5

R.T.: 7.666 min
Delta R.T.: 0.003 min
Response: 98677776
Conc: 1011.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-63A

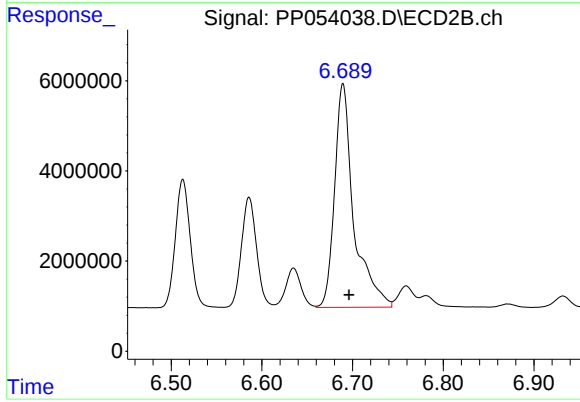

#30 AR-1254-5

R.T.: 6.689 min
Delta R.T.: -0.007 min
Response: 72892962
Conc: 935.32 ng/ml