

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122420\
 Data File : PP032409.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Dec 2020 15:07
 Operator : DD\AJ
 Sample : L5197-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EO-01-122320

Manual Integrations
 APPROVED

mohammad
 12/28/2020 1:00:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 16:20:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 24 07:15:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.772	4.044	986228	956438	21.233m	21.307
2) SA Decachlor...	10.627	9.327	796481	763805	27.188	23.679

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122420\
Data File : PP032409.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2020 15:07
Operator : DD\AJ
Sample : L5197-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
EO-01-122320


Manual Integrations
APPROVED

mohammad
12/28/2020 1:00:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 16:20:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 24 07:15:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

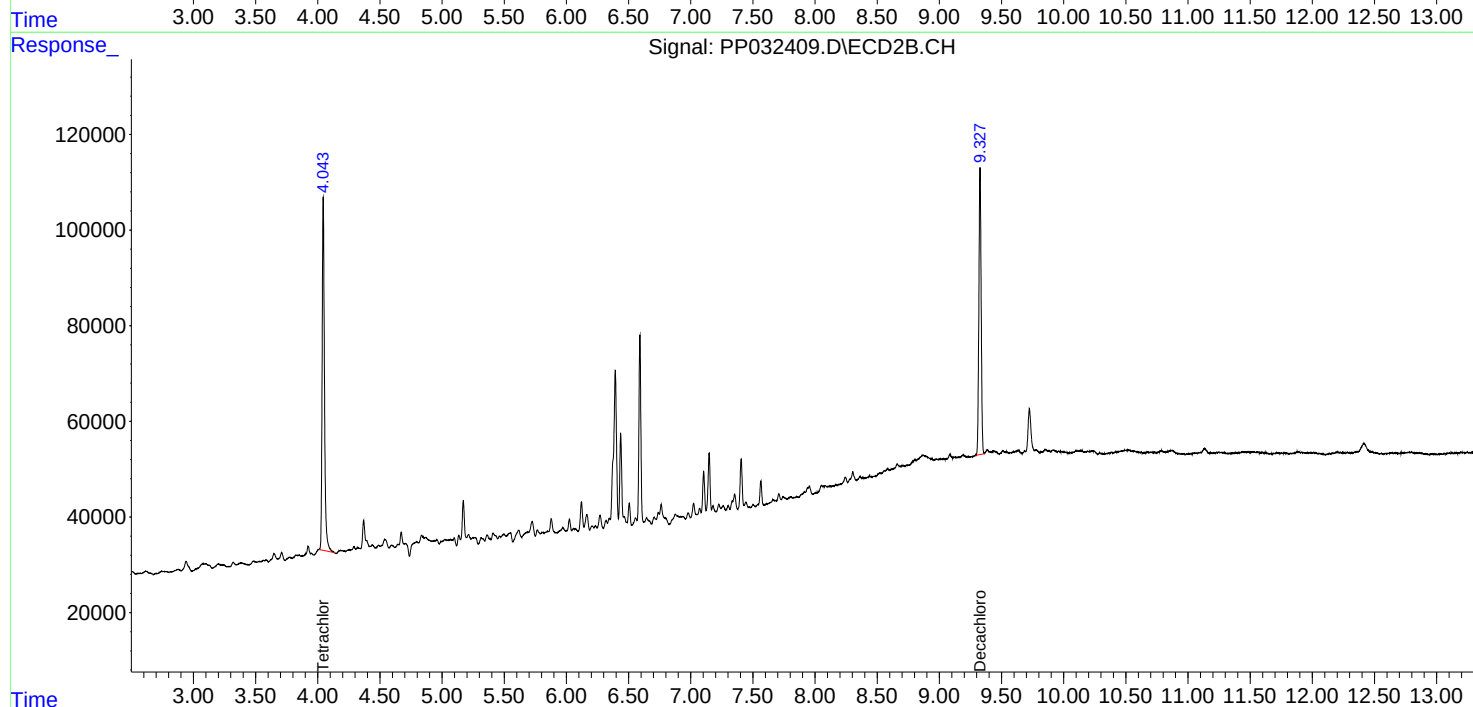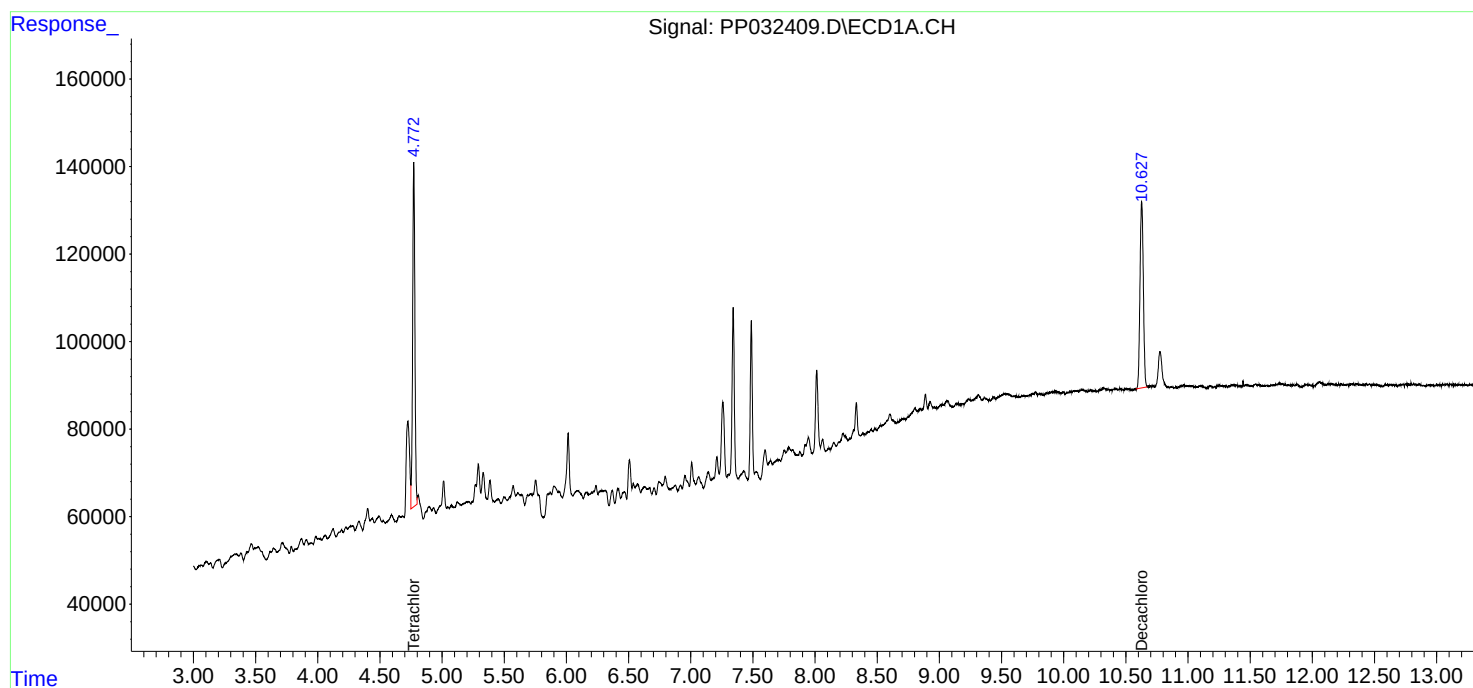

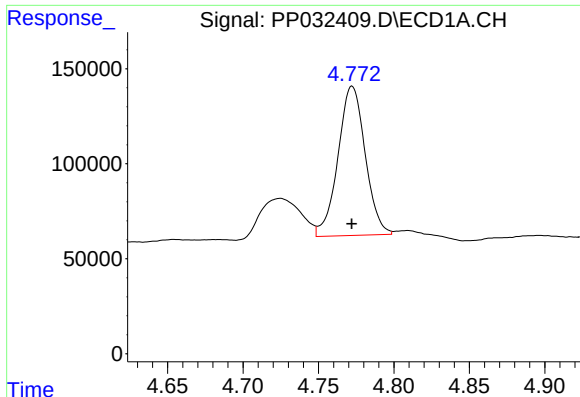


#1 Tetrachloro-m-xylene

R.T.: 4.772 min
Delta R.T.: 0.000 min
Response: 986228
Conc: 21.23 ng/ml m

Instrument :
ECD_P
ClientSampleId :
EO-01-122320


Manual Integrations
APPROVED

mohammad
12/28/2020 1:00:18 PM

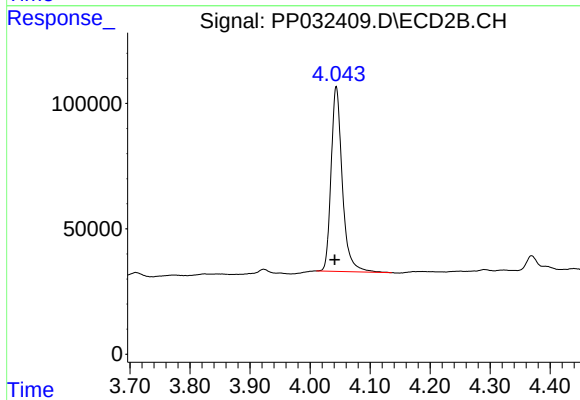


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.002 min
Response: 956438
Conc: 21.31 ng/ml

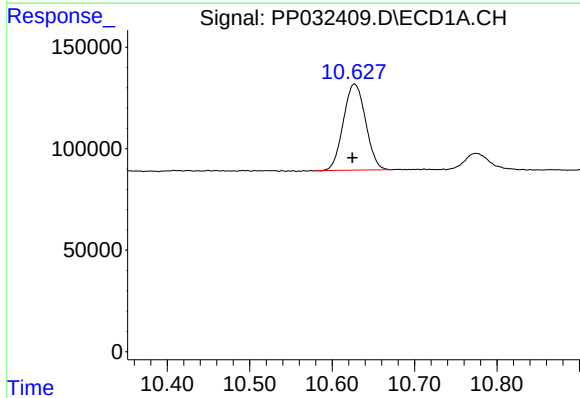

#2 Decachlorobiphenyl

R.T.: 10.627 min
Delta R.T.: 0.002 min
Response: 796481
Conc: 27.19 ng/ml

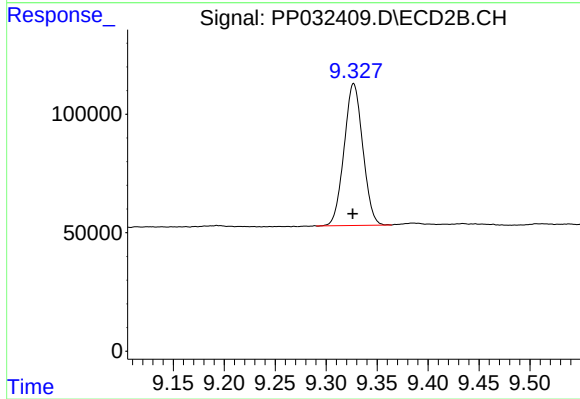

#2 Decachlorobiphenyl

R.T.: 9.327 min
Delta R.T.: 0.001 min
Response: 763805
Conc: 23.68 ng/ml