

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122421\
Data File : PP042193.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2021 14:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 04:18:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 24 23:47:53 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.923	4.061	279158	503871	21.261	22.061
2)	SA Decachlor...	10.917	9.414	302936	398837	24.871	24.663

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122421\
Data File : PP042193.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2021 14:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 04:18:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 24 23:47:53 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

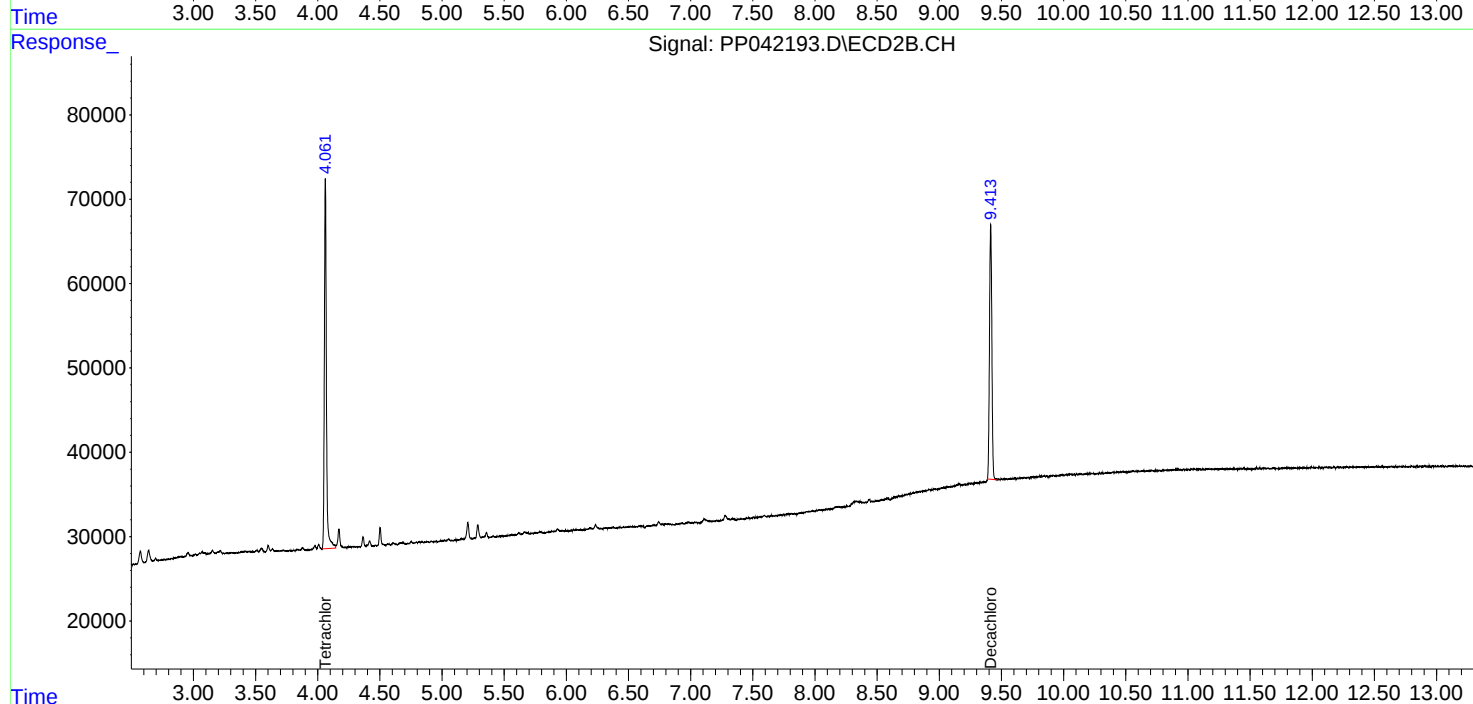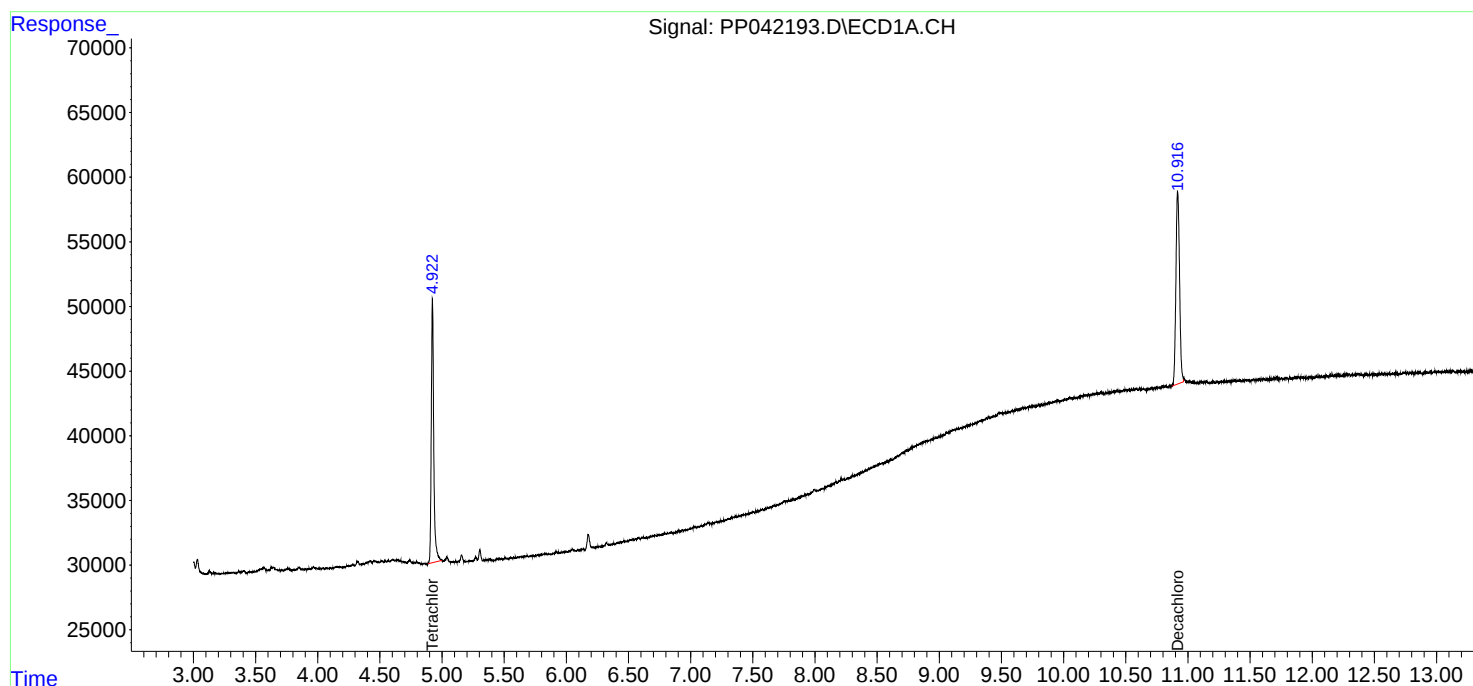


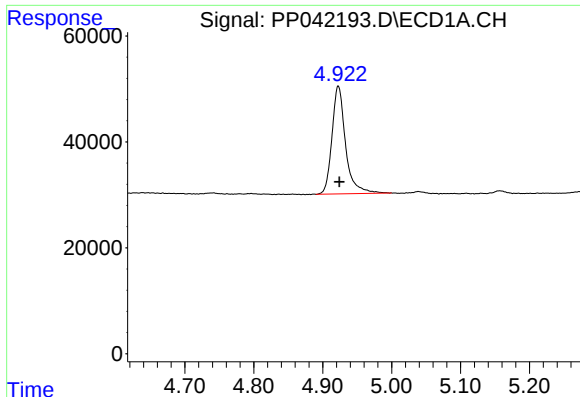

#1 Tetrachloro-m-xylene


R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 279158
Conc: 21.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

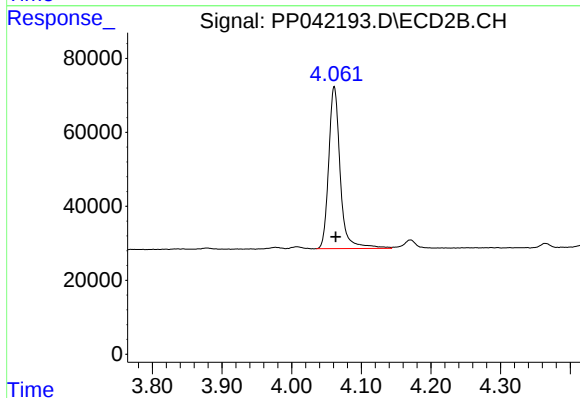


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: -0.002 min
Response: 503871
Conc: 22.06 ng/ml

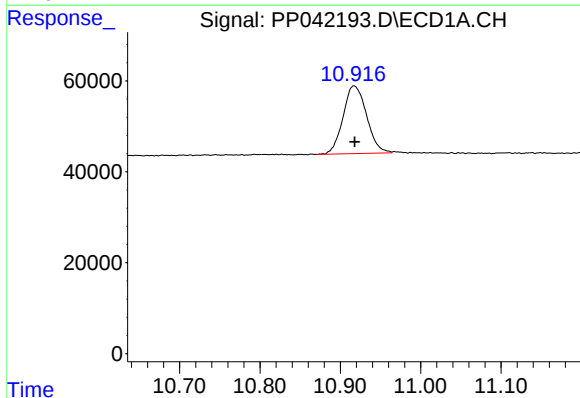

#2 Decachlorobiphenyl

R.T.: 10.917 min
Delta R.T.: -0.001 min
Response: 302936
Conc: 24.87 ng/ml

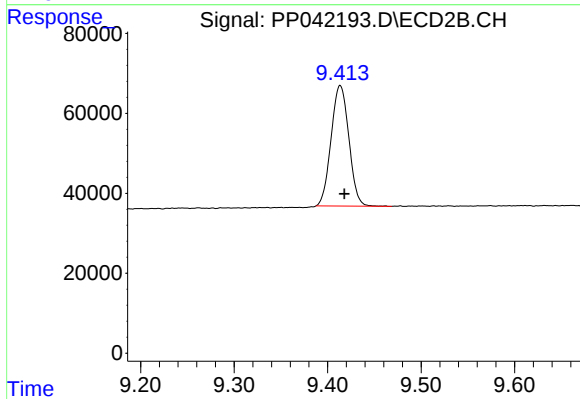

#2 Decachlorobiphenyl

R.T.: 9.414 min
Delta R.T.: -0.004 min
Response: 398837
Conc: 24.66 ng/ml