

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122421\
 Data File : PP042213.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Dec 2021 22:33
 Operator : AJ\MA
 Sample : M5144-14 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ECA342V-1-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/27/2021
 Supervised By :mohammad ahmed 12/28/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 04:27:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 24 23:47:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.921	4.061	20750	35431	1.580m	1.551m
2) SA Decachlor...	10.919	9.413	31003	34751	2.545m	2.149m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122421\
Data File : PP042213.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2021 22:33
Operator : AJ\MA
Sample : M5144-14 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ECA342V-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/27/2021
Supervised By :mohammad ahmed 12/28/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 04:27:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 24 23:47:53 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

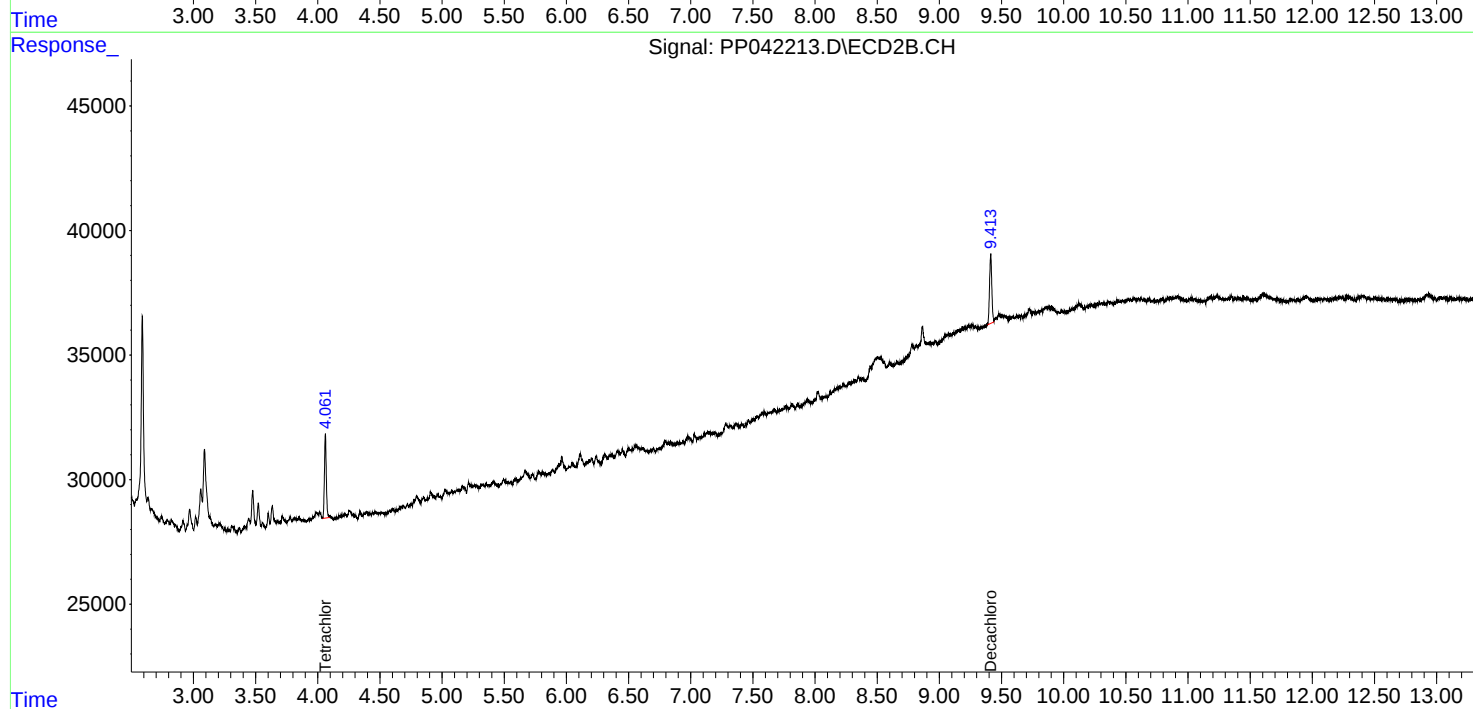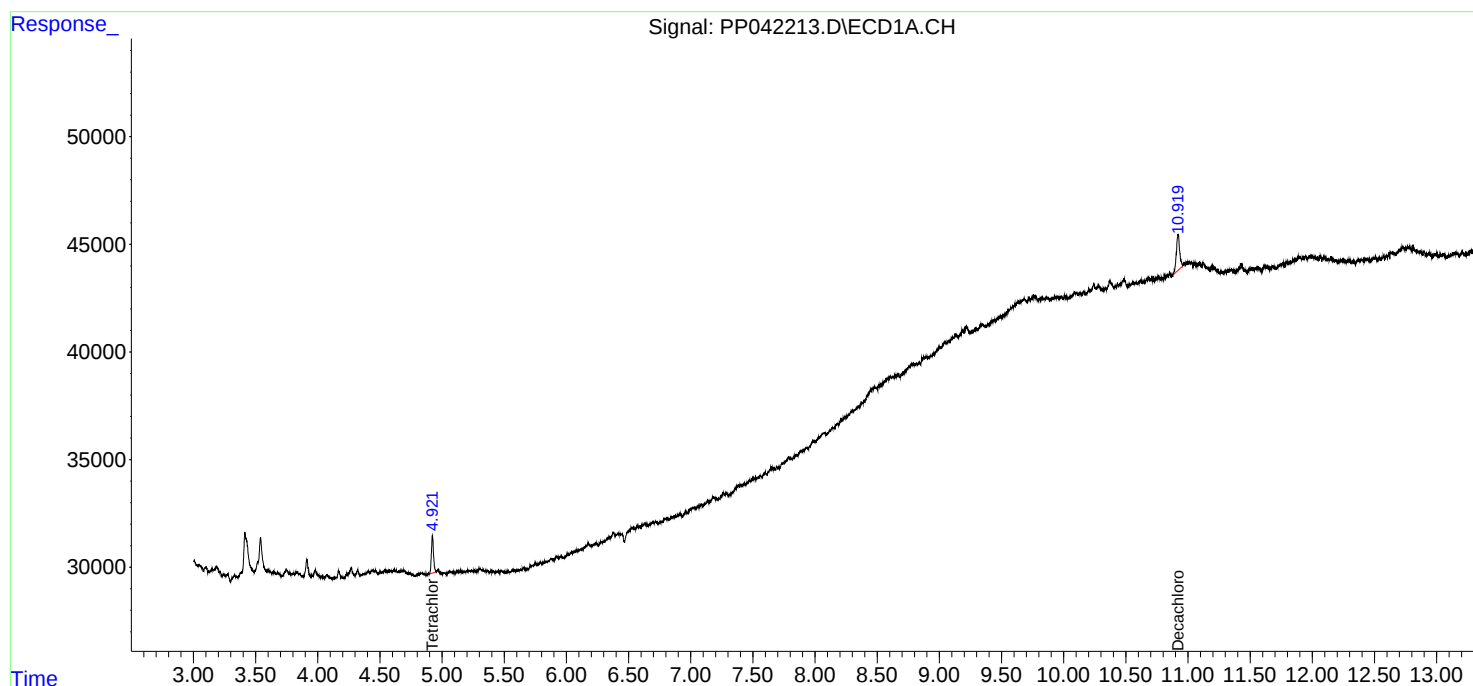

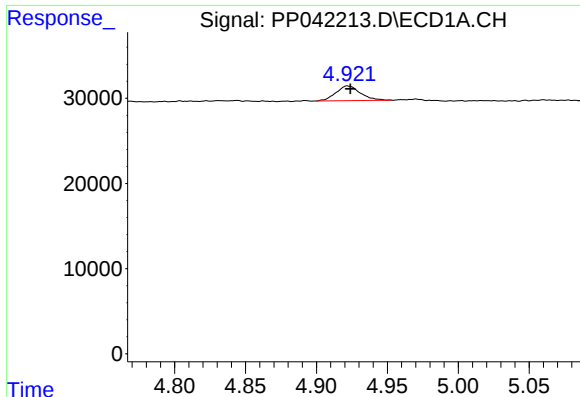


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: -0.003 min
Response: 20750
Conc: 1.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
ECA342V-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/27/2021
Supervised By :mohammad ahmed 12/28/2021

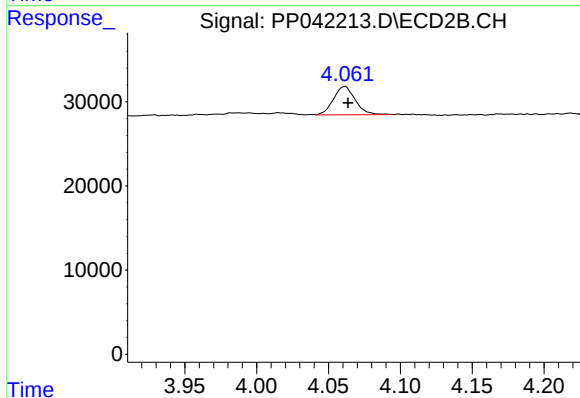


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: -0.002 min
Response: 35431
Conc: 1.55 ng/ml m

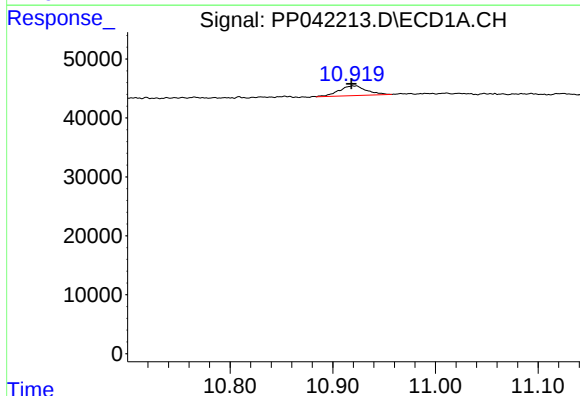

#2 Decachlorobiphenyl

R.T.: 10.919 min
Delta R.T.: 0.000 min
Response: 31003
Conc: 2.55 ng/ml m

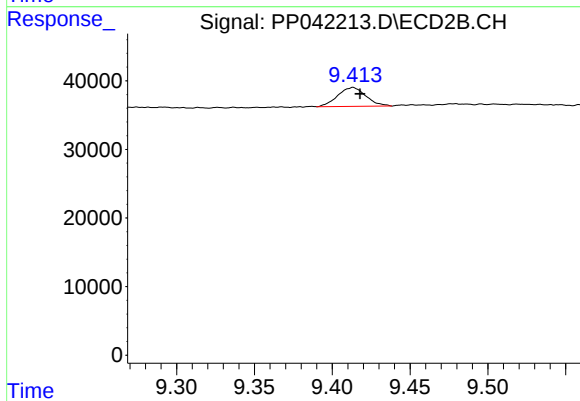

#2 Decachlorobiphenyl

R.T.: 9.413 min
Delta R.T.: -0.005 min
Response: 34751
Conc: 2.15 ng/ml m