

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122623\
 Data File : PP062632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2023 22:17
 Operator : YP\AJ
 Sample : 06018-03
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/27/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 01:00:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:29:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.396	3.683	51995130	67463742	23.916	22.607
2) SA Decachlor...	10.143	8.784	29437789	41966246	20.414	16.485
Target Compounds						
26) L6 AR-1254-1	6.427	5.607	2658332	5294542	32.213	33.351
27) L6 AR-1254-2	6.646	5.756	6012937	6049538	46.903	43.376
28) L6 AR-1254-3	7.013	6.166	5363079	10633805	41.538	48.118
29) L6 AR-1254-4	7.299	6.397	3949475	4062144	43.830	31.416 #
30) L6 AR-1254-5	7.719	6.820	4842346	8726438	49.428m	45.479

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122623\
Data File : PP062632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2023 22:17
Operator : YP\AJ
Sample : 06018-03
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 01:00:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:29:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

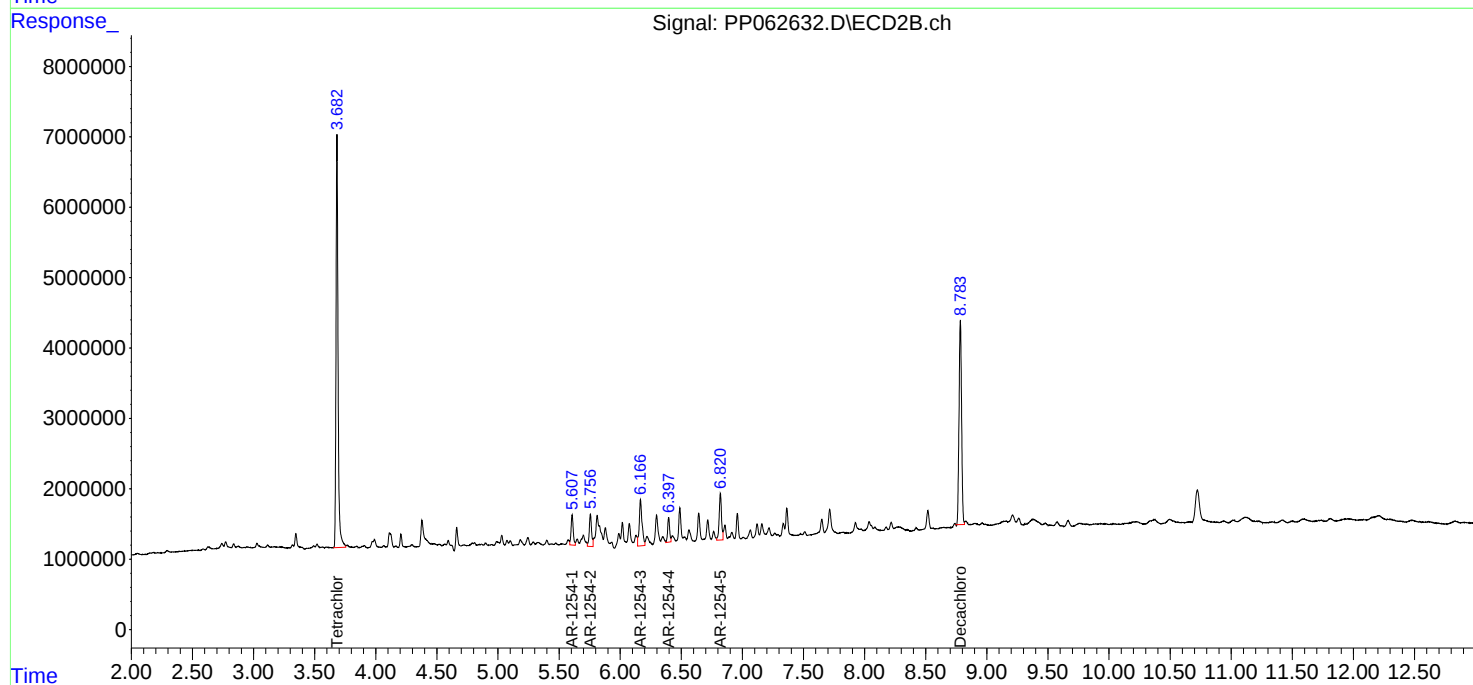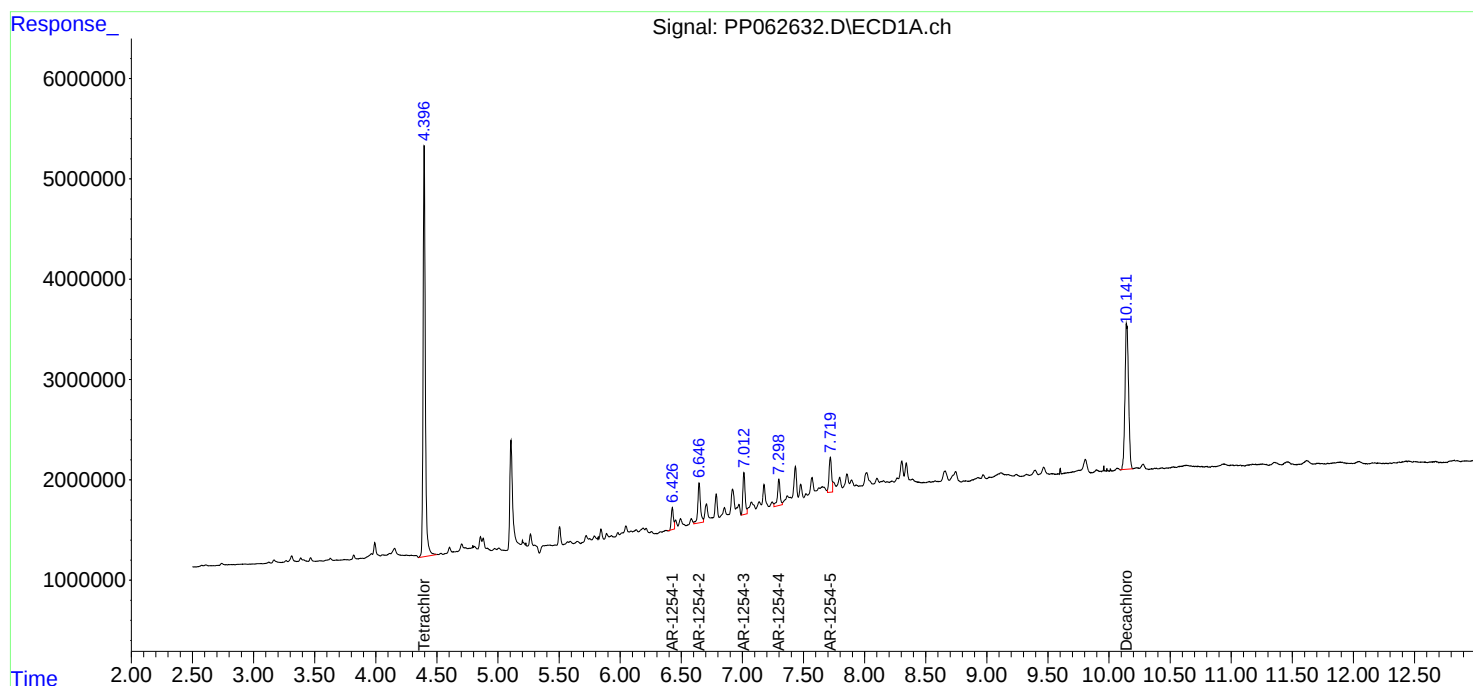

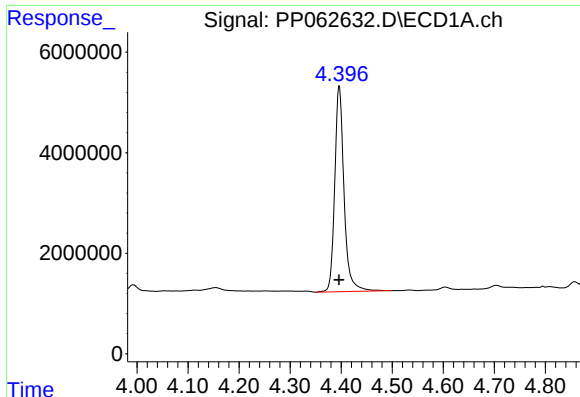


#1 Tetrachloro-m-xylene

R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 51995130
Conc: 23.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2023
Supervised By :Ankita Jodhani 12/28/2023

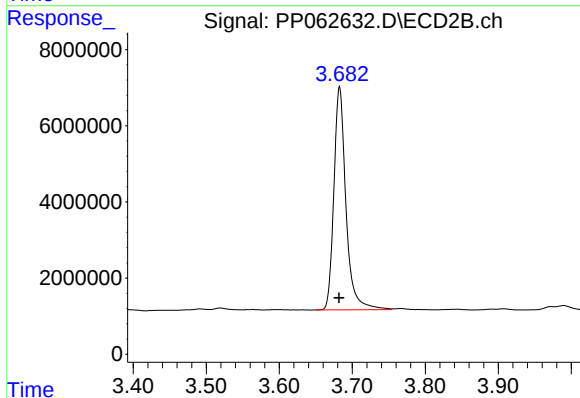


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: 0.000 min
Response: 67463742
Conc: 22.61 ng/ml

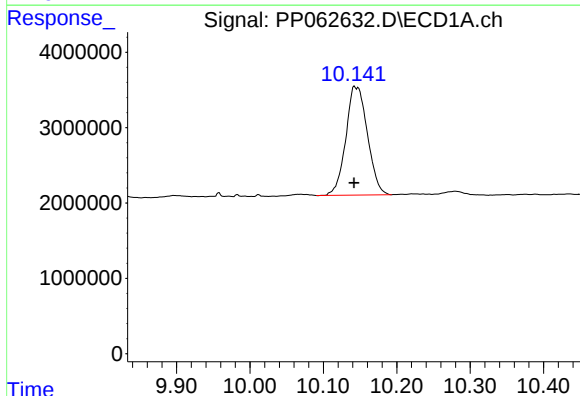


#2 Decachlorobiphenyl

R.T.: 10.143 min
Delta R.T.: 0.000 min
Response: 29437789
Conc: 20.41 ng/ml

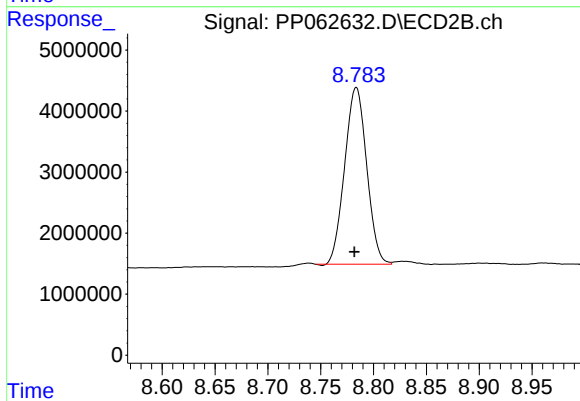

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: 0.002 min
Response: 41966246
Conc: 16.49 ng/ml

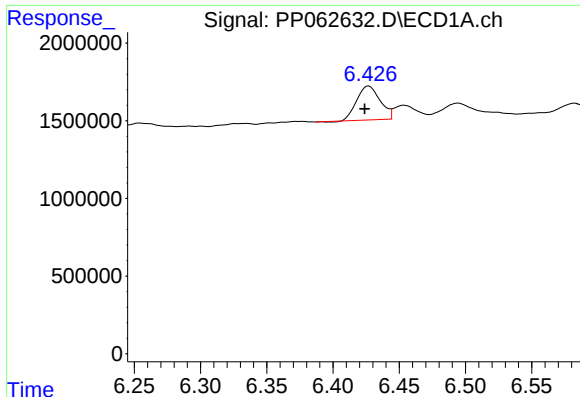


#26 AR-1254-1

R.T.: 6.427 min
Delta R.T.: 0.003 min
Response: 2658332
Conc: 32.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2023
Supervised By :Ankita Jodhani 12/28/2023

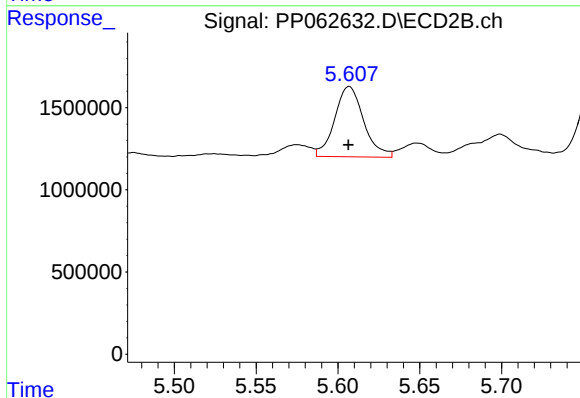


#26 AR-1254-1

R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 5294542
Conc: 33.35 ng/ml

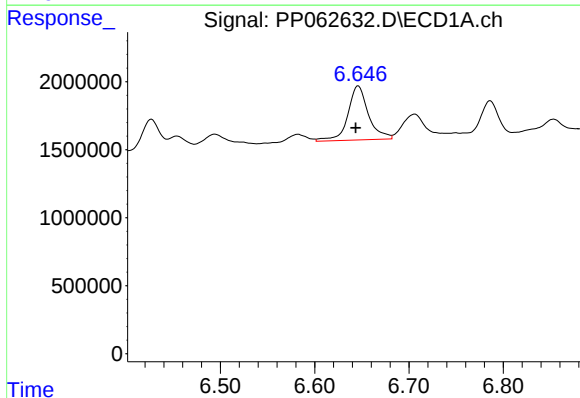


#27 AR-1254-2

R.T.: 6.646 min
Delta R.T.: 0.003 min
Response: 6012937
Conc: 46.90 ng/ml

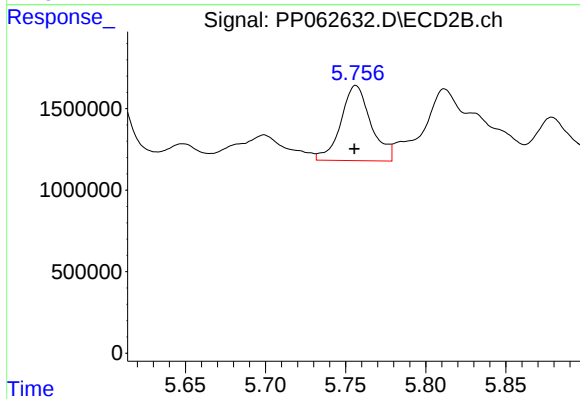

#27 AR-1254-2

R.T.: 5.756 min
Delta R.T.: 0.000 min
Response: 6049538
Conc: 43.38 ng/ml

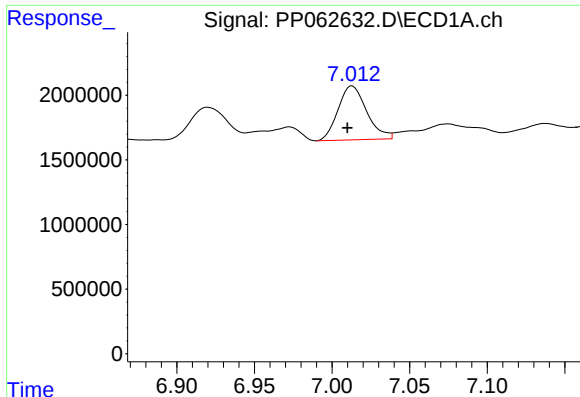


#28 AR-1254-3

R.T.: 7.013 min
Delta R.T.: 0.003 min
Response: 5363079
Conc: 41.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2023
Supervised By :Ankita Jodhani 12/28/2023

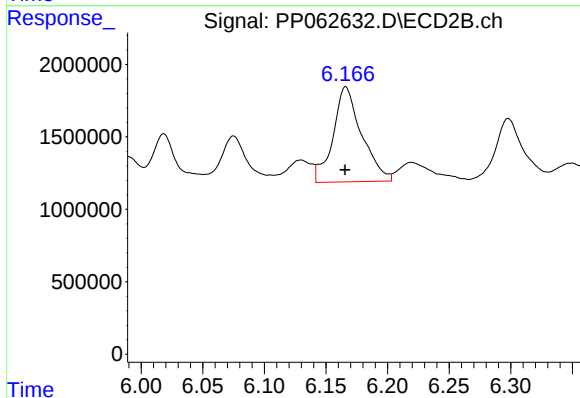


#28 AR-1254-3

R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 10633805
Conc: 48.12 ng/ml

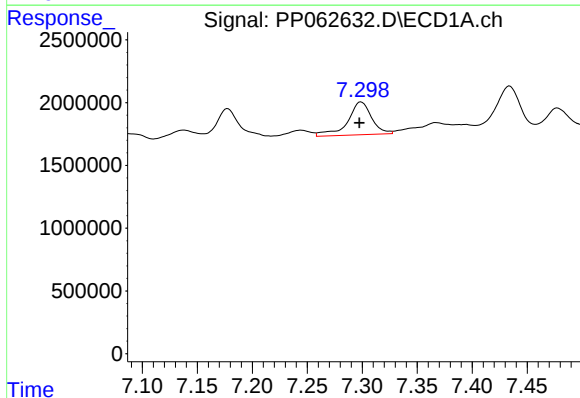


#29 AR-1254-4

R.T.: 7.299 min
Delta R.T.: 0.002 min
Response: 3949475
Conc: 43.83 ng/ml

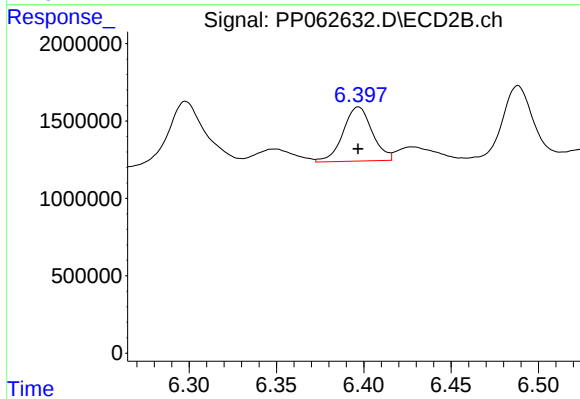

#29 AR-1254-4

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 4062144
Conc: 31.42 ng/ml

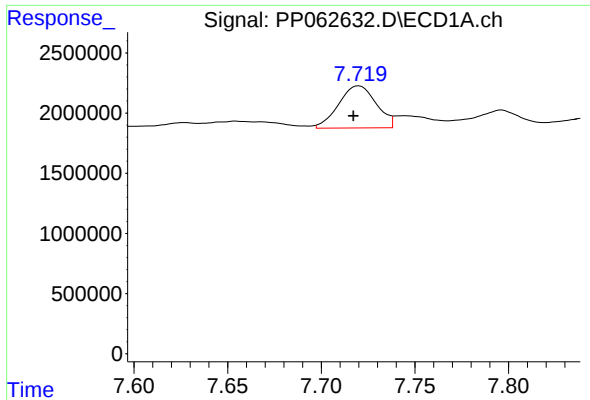


#30 AR-1254-5

R.T.: 7.719 min
Delta R.T.: 0.002 min
Response: 4842346
Conc: 49.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2023
Supervised By :Ankita Jodhani 12/28/2023

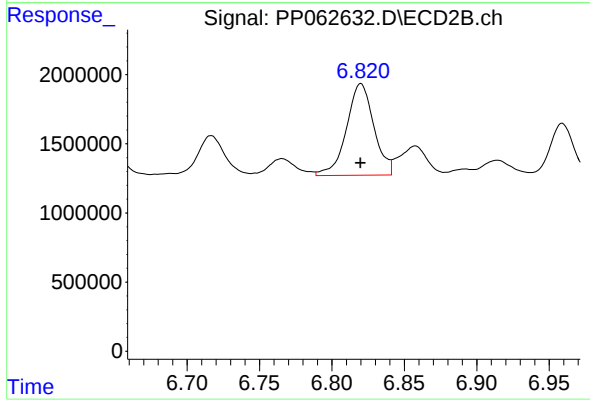

#30 AR-1254-5

R.T.: 6.820 min
Delta R.T.: 0.000 min
Response: 8726438
Conc: 45.48 ng/ml