

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122722\
 Data File : PP054073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2022 12:19
 Operator : YP\AJ
 Sample : N6197-03 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2022-60A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 03:00:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 14 05:38:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.588	4202687	2281365	2.002	1.461 #
2) SA Decachlor...	10.106	8.624	3293018	2580070	1.940	1.847
Target Compounds						
26) L6 AR-1254-1	6.369	5.483	141.9E6	134.4E6	1831.496	2051.940
27) L6 AR-1254-2	6.589	5.631	214.5E6	117.5E6	1843.873	2014.920
28) L6 AR-1254-3	6.955	6.037	210.8E6	176.8E6	1799.470	2009.608
29) L6 AR-1254-4	7.243	6.266	151.9E6	100.2E6	1915.924	2186.363
30) L6 AR-1254-5	7.664	6.686	180.8E6	162.7E6	1853.993	2087.879



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122722\
Data File : PP054073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2022 12:19
Operator : YP\AJ
Sample : N6197-03 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 03:00:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121322.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 14 05:38:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

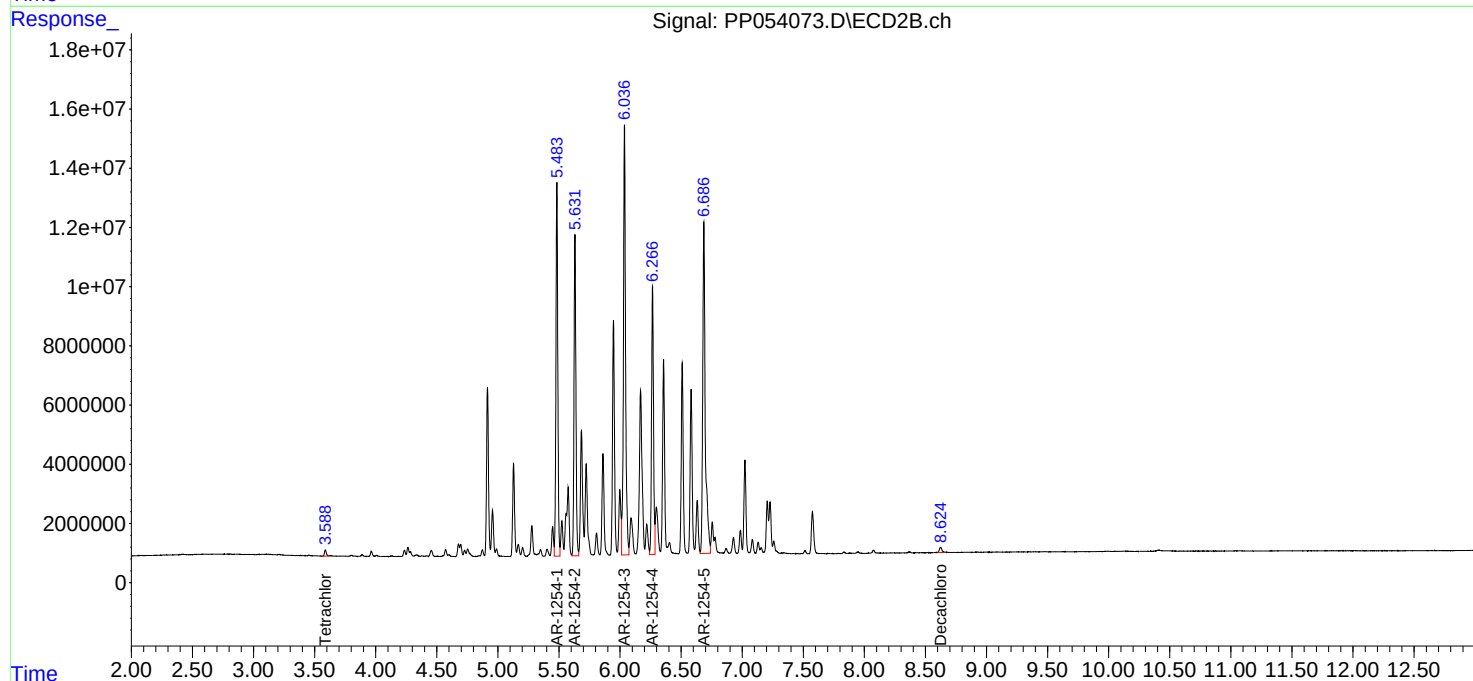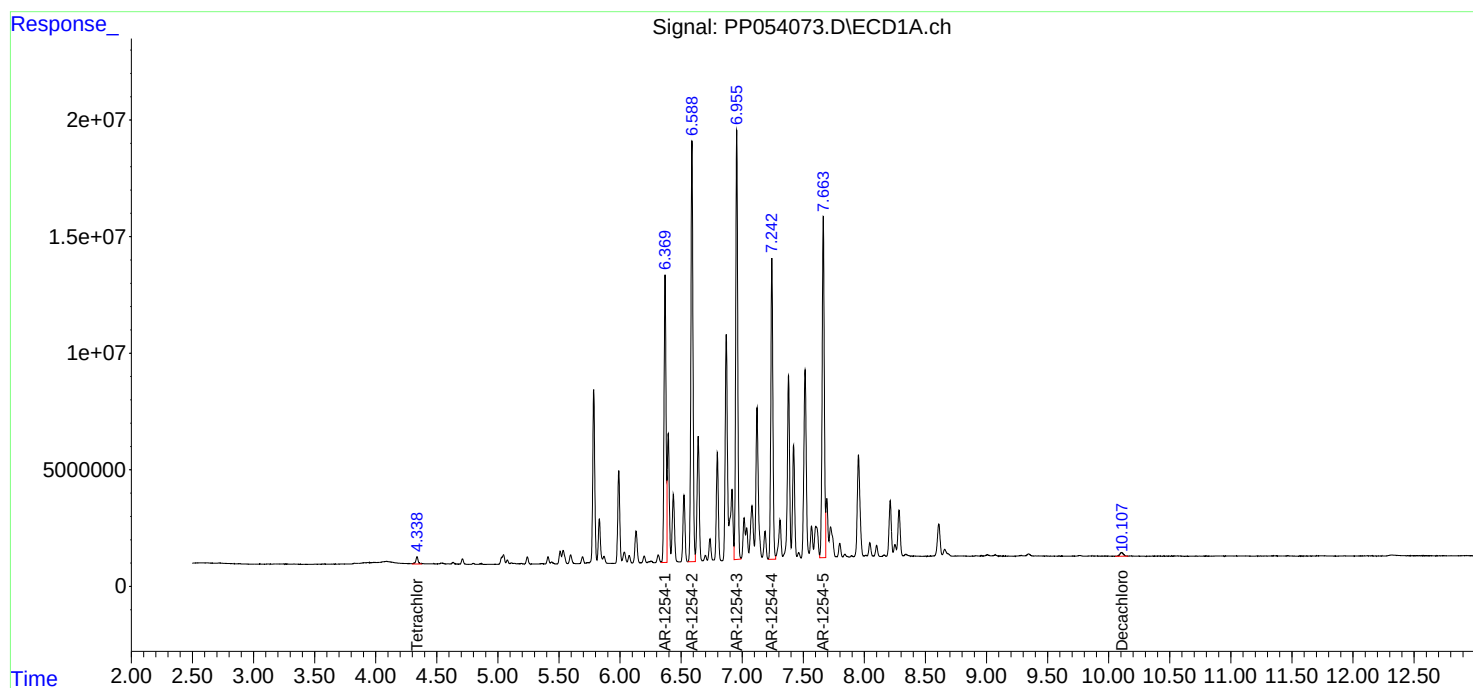


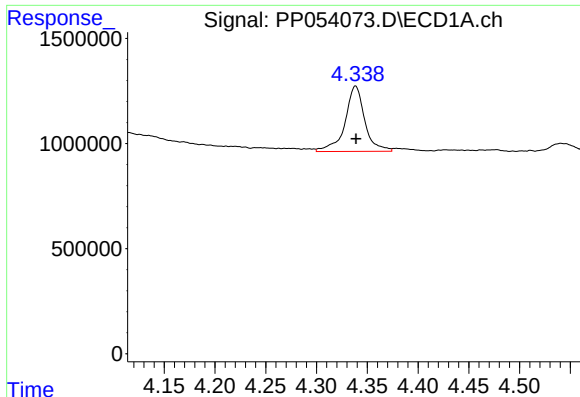

#1 Tetrachloro-m-xylene


R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 4202687
Conc: 2.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

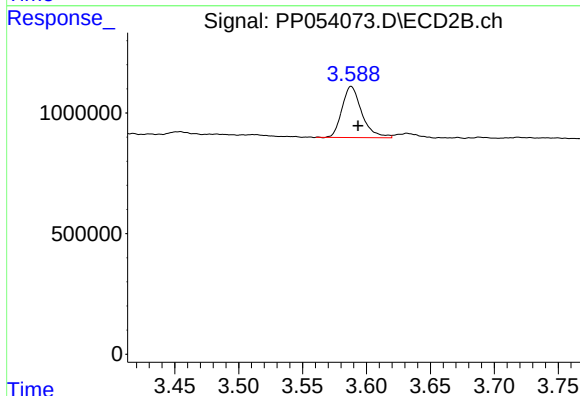


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: -0.005 min
Response: 2281365
Conc: 1.46 ng/ml

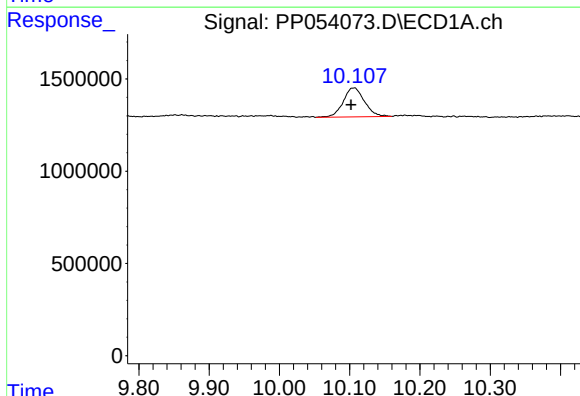


#2 Decachlorobiphenyl

R.T.: 10.106 min
Delta R.T.: 0.004 min
Response: 3293018
Conc: 1.94 ng/ml

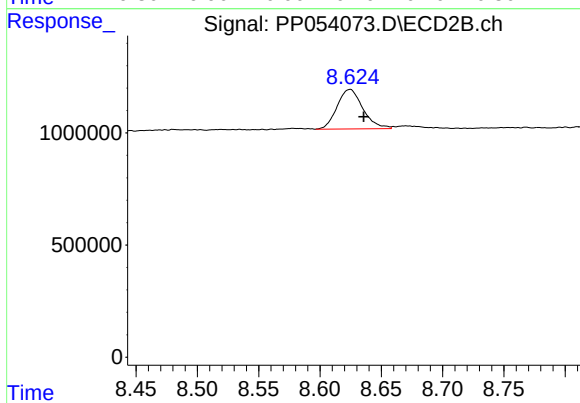

#2 Decachlorobiphenyl


R.T.: 8.624 min
Delta R.T.: -0.011 min
Response: 2580070
Conc: 1.85 ng/ml

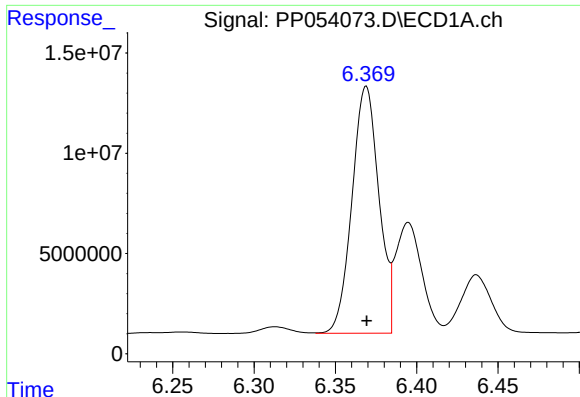

#26 AR-1254-1


R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 141927154
Conc: 1831.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

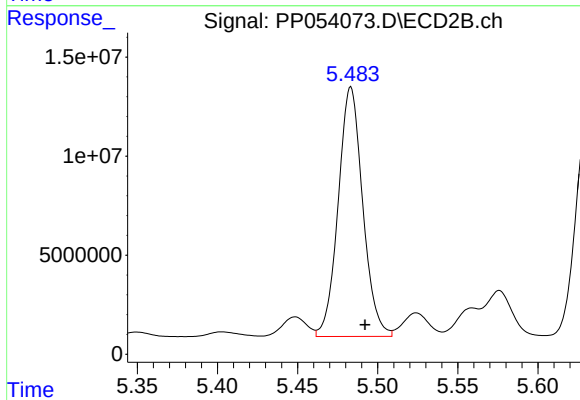


#26 AR-1254-1

R.T.: 5.483 min
Delta R.T.: -0.009 min
Response: 134367898
Conc: 2051.94 ng/ml

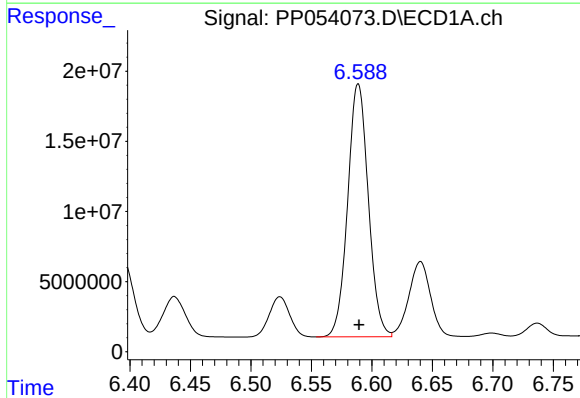


#27 AR-1254-2

R.T.: 6.589 min
Delta R.T.: 0.000 min
Response: 214528588
Conc: 1843.87 ng/ml

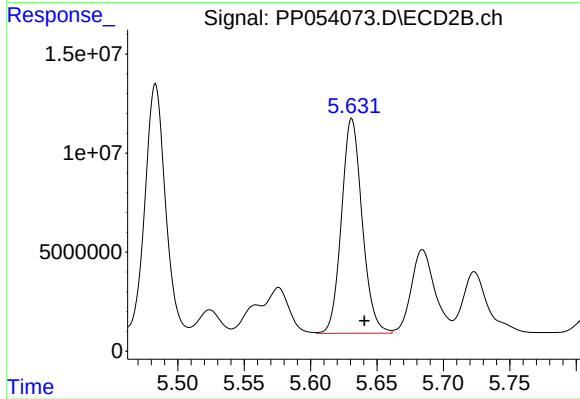

#27 AR-1254-2


R.T.: 5.631 min
Delta R.T.: -0.009 min
Response: 117509395
Conc: 2014.92 ng/ml

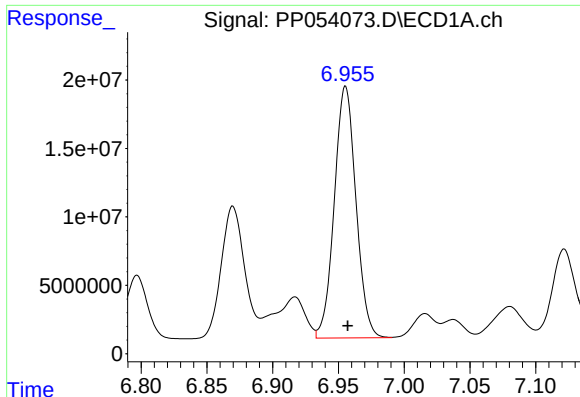

#28 AR-1254-3


R.T.: 6.955 min
Delta R.T.: -0.002 min
Response: 210767250
Conc: 1799.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

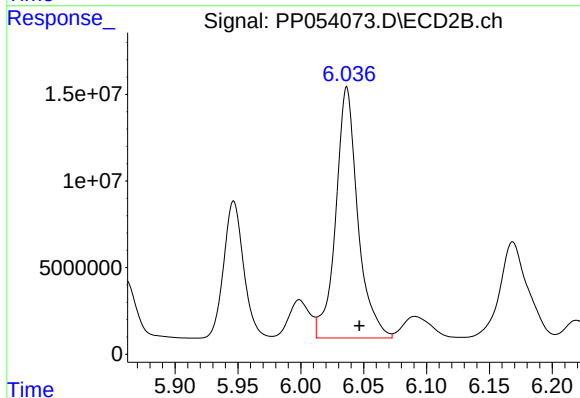


#28 AR-1254-3

R.T.: 6.037 min
Delta R.T.: -0.010 min
Response: 176789178
Conc: 2009.61 ng/ml

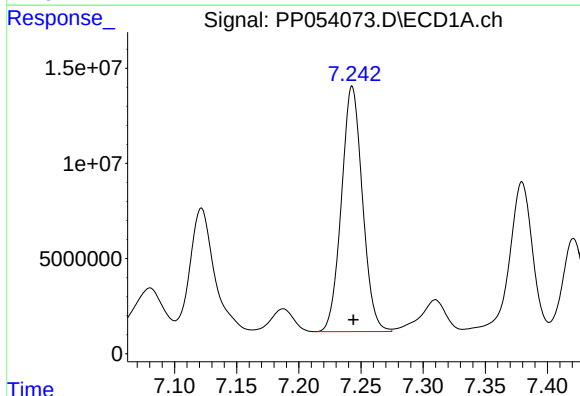


#29 AR-1254-4

R.T.: 7.243 min
Delta R.T.: -0.001 min
Response: 151890895
Conc: 1915.92 ng/ml

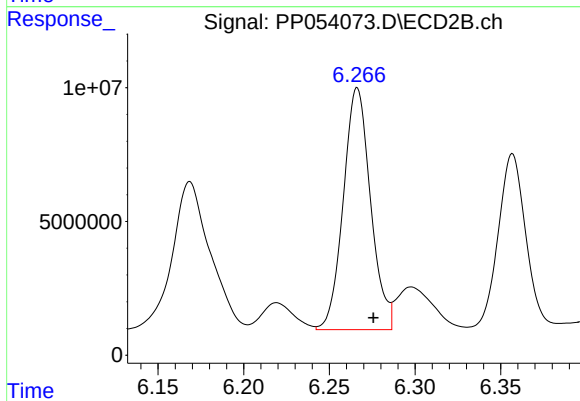

#29 AR-1254-4


R.T.: 6.266 min
Delta R.T.: -0.009 min
Response: 100168281
Conc: 2186.36 ng/ml

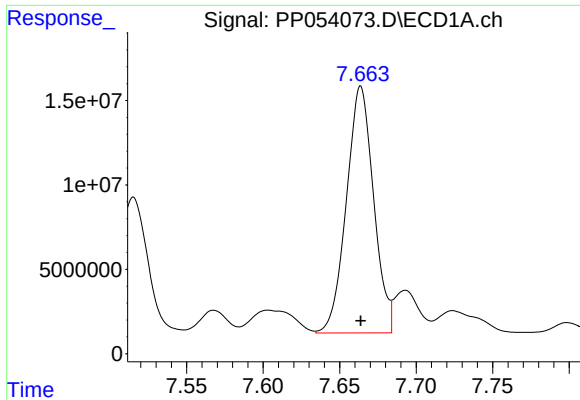

#30 AR-1254-5

R.T.: 7.664 min
Delta R.T.: 0.000 min
Response: 180810616
Conc: 1853.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-60A

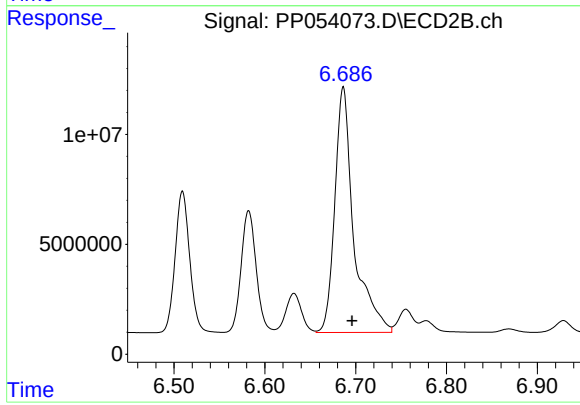

#30 AR-1254-5

R.T.: 6.686 min
Delta R.T.: -0.010 min
Response: 162716287
Conc: 2087.88 ng/ml