

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122723\
 Data File : PP062646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2023 10:53
 Operator : YP\AJ
 Sample : 05899-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GHL-SS-08

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:16:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:29:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.396	3.683	50903297	66909657	23.414m	22.421
2) SA Decachlor...	10.150	8.784	30296184	40506352	21.010m	15.912m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122723\
Data File : PP062646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2023 10:53
Operator : YP\AJ
Sample : 05899-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GHL-SS-08


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:16:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:29:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

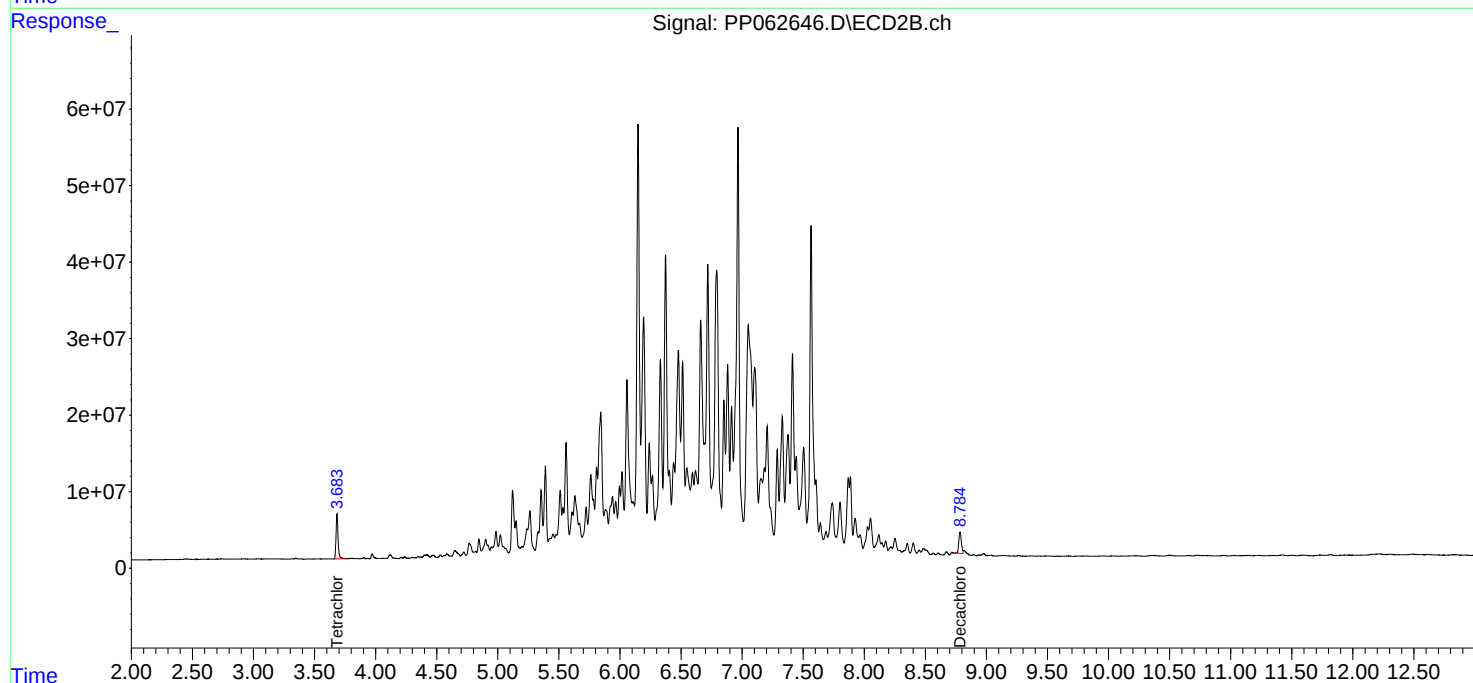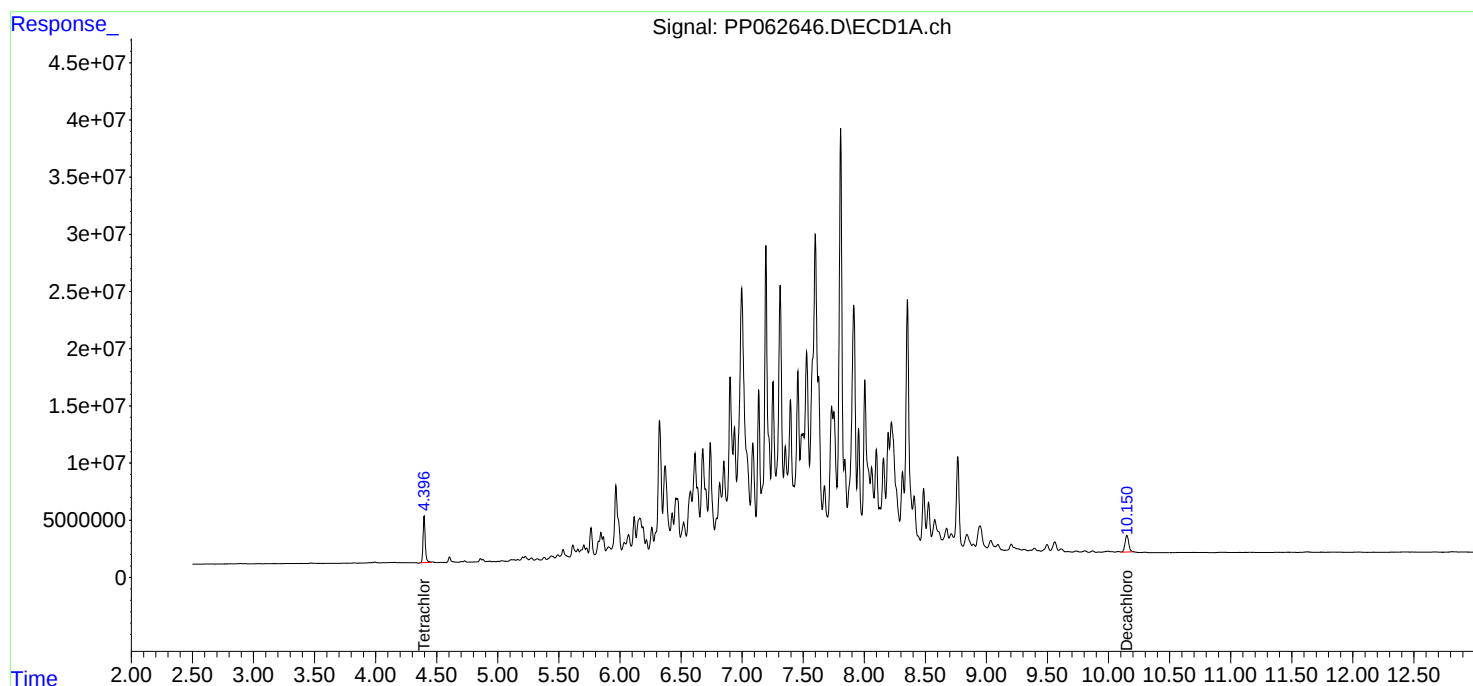

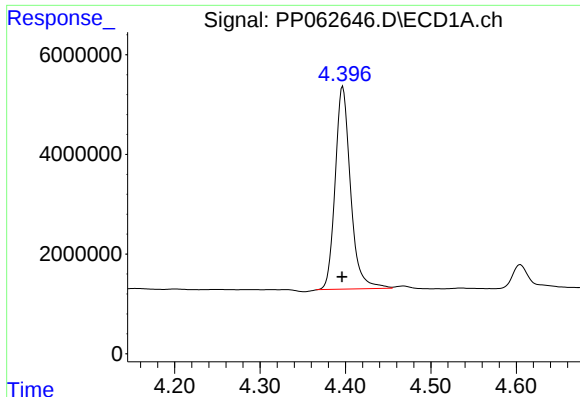


#1 Tetrachloro-m-xylene

R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 50903297
Conc: 23.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
GHL-SS-08


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

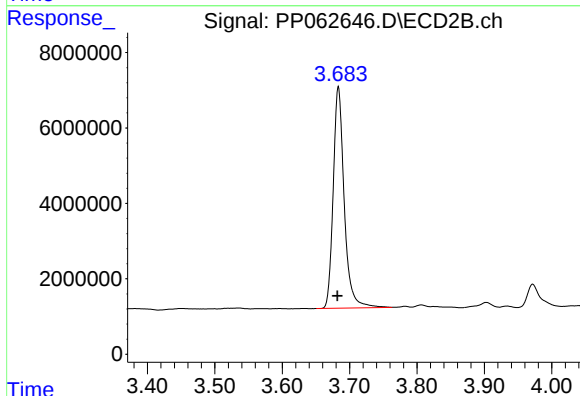


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: 0.002 min
Response: 66909657
Conc: 22.42 ng/ml

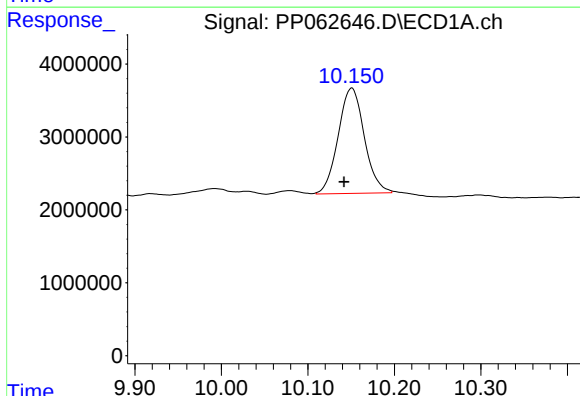

#2 Decachlorobiphenyl

R.T.: 10.150 min
Delta R.T.: 0.009 min
Response: 30296184
Conc: 21.01 ng/ml m

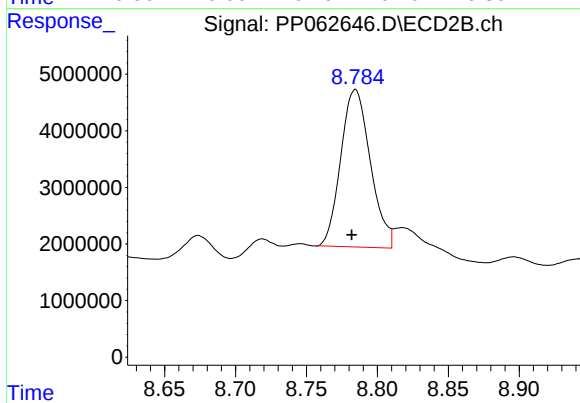

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: 0.002 min
Response: 40506352
Conc: 15.91 ng/ml m