

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122723\
 Data File : PP062650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2023 12:38
 Operator : YP\AJ
 Sample : 05899-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GHL-SS-10-0-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:18:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:29:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.685	50086725	60174286	23.038m	20.164
2) SA Decachlor...	10.158	8.787	31833592	40818301	22.076	16.034m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122723\
Data File : PP062650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2023 12:38
Operator : YP\AJ
Sample : 05899-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GHL-SS-10-0-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:18:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:29:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

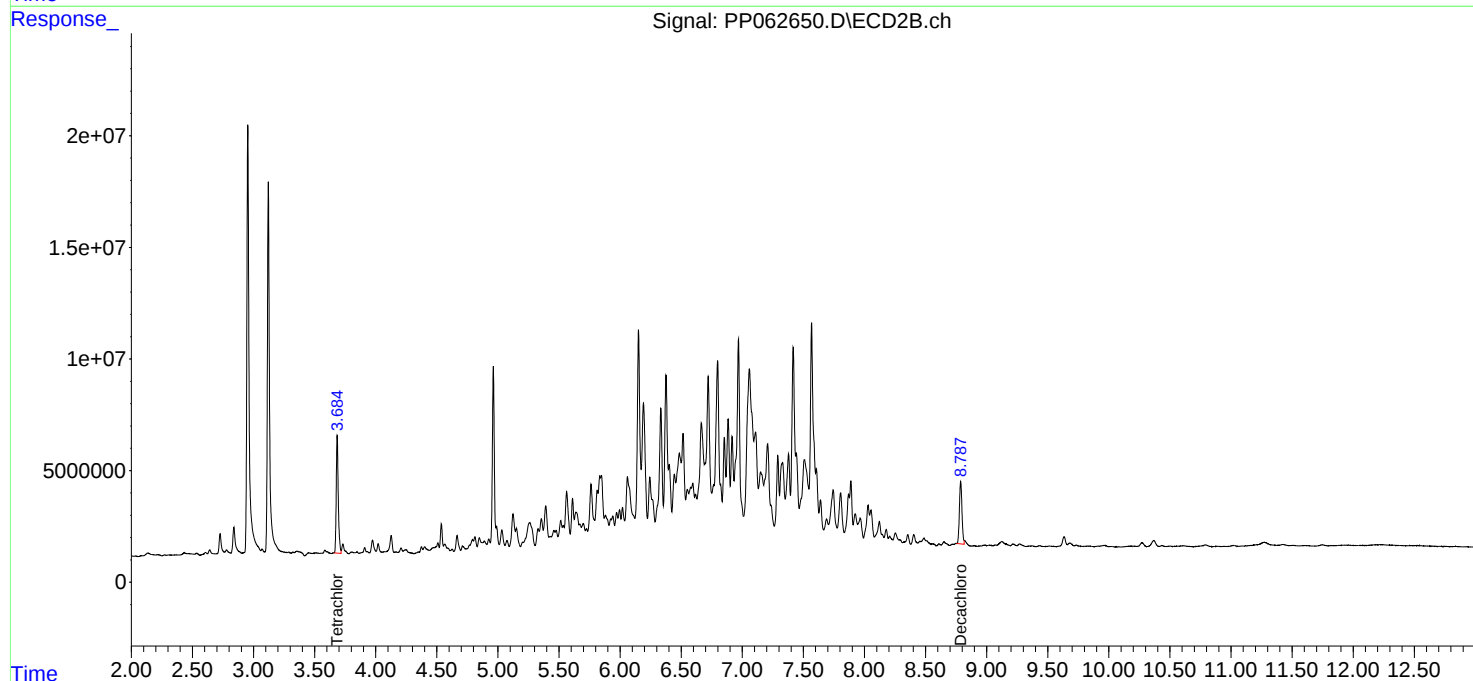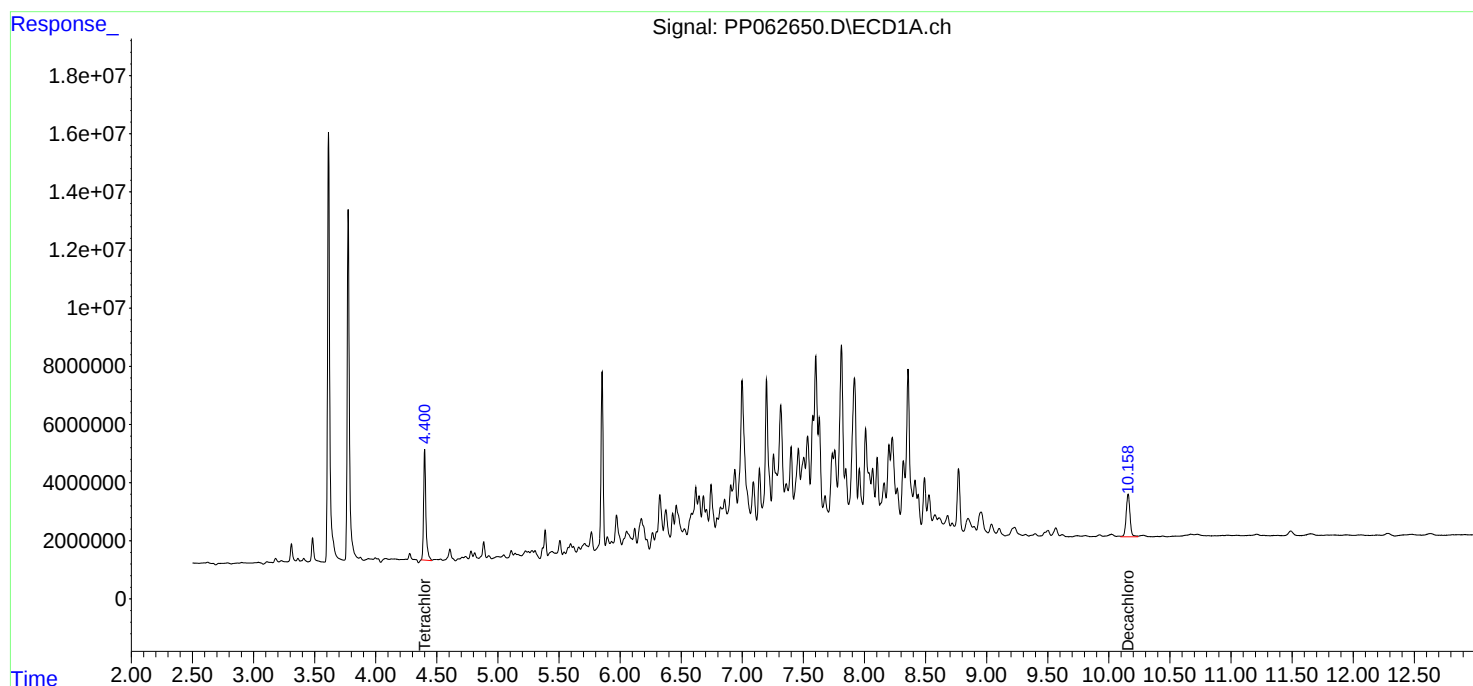

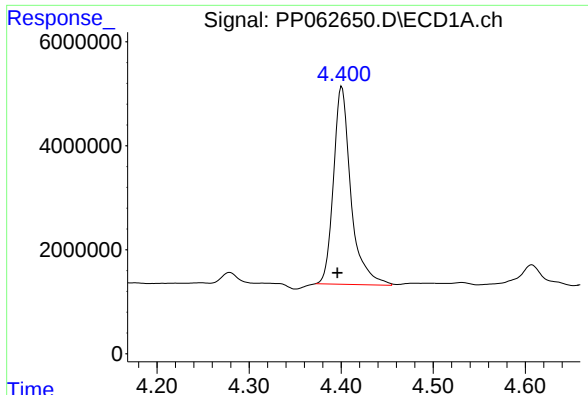


#1 Tetrachloro-m-xylene

R.T.: 4.400 min
Delta R.T.: 0.004 min
Response: 50086725
Conc: 23.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
GHL-SS-10-0-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

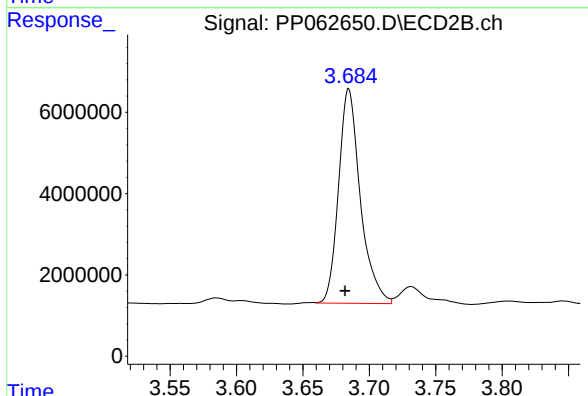


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.003 min
Response: 60174286
Conc: 20.16 ng/ml

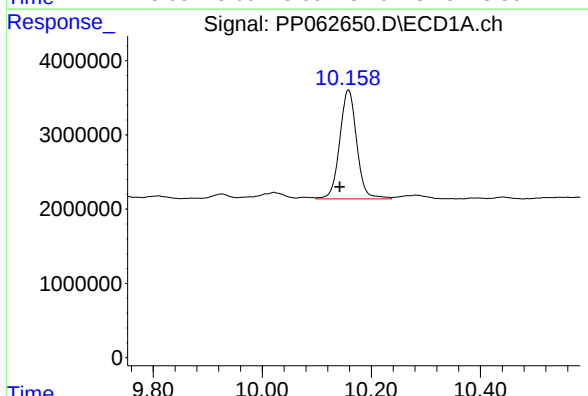

#2 Decachlorobiphenyl

R.T.: 10.158 min
Delta R.T.: 0.016 min
Response: 31833592
Conc: 22.08 ng/ml

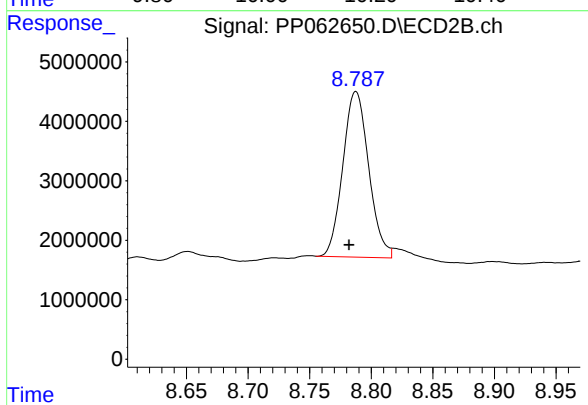

#2 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: 0.005 min
Response: 40818301
Conc: 16.03 ng/ml m