

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122723\
 Data File : PP062662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2023 16:10
 Operator : YP\AJ
 Sample : 05899-21
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GHL-SS-18-0-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:22:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:29:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.684	35208182	47992360	16.194	16.082m
2) SA Decachlor...	10.160	8.788	907.4E6	39162829	629.236	15.384m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122723\
Data File : PP062662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2023 16:10
Operator : YP\AJ
Sample : 05899-21
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GHL-SS-18-0-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:22:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:29:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

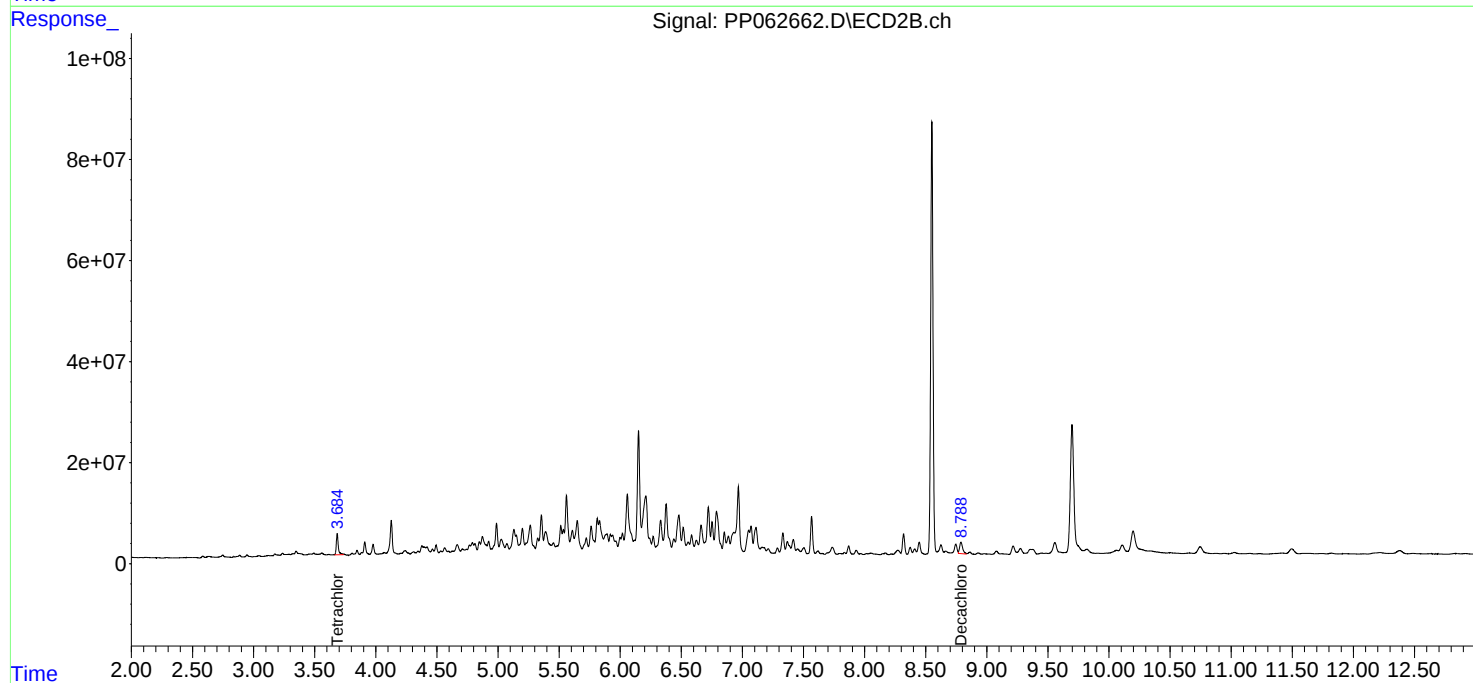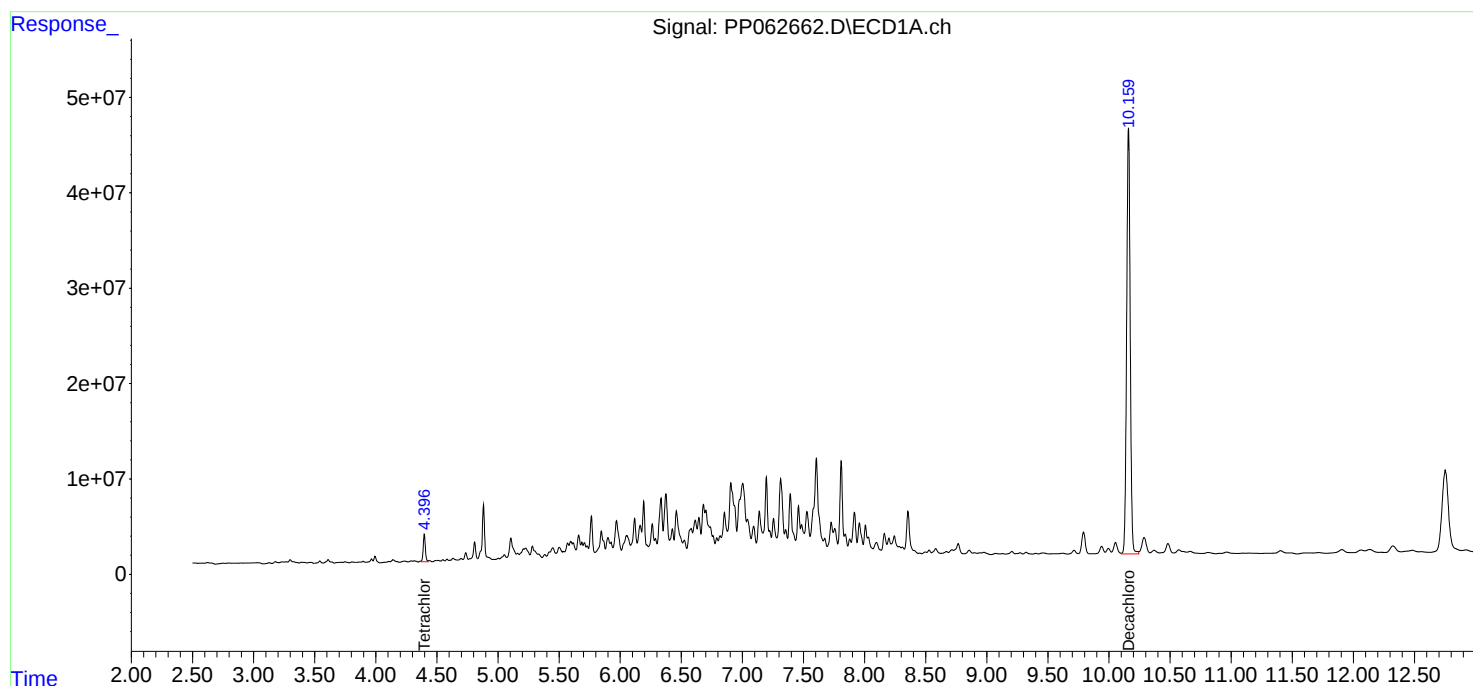

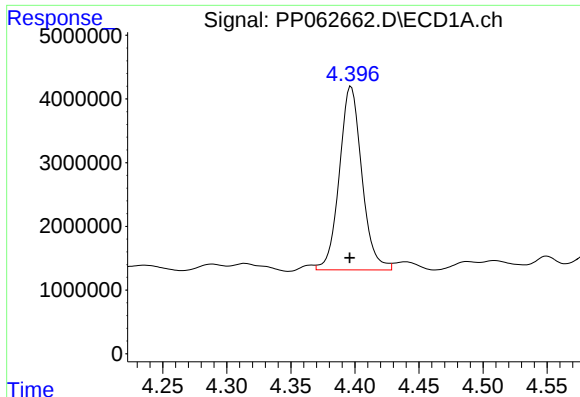


#1 Tetrachloro-m-xylene

R.T.: 4.397 min
Delta R.T.: 0.001 min
Response: 35208182
Conc: 16.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
GHL-SS-18-0-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :Ankita Jodhani 12/28/2023

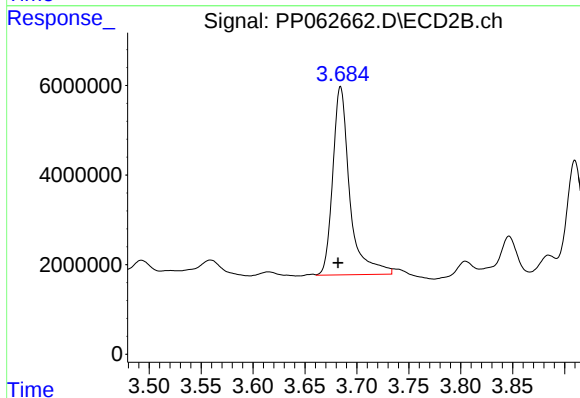


#1 Tetrachloro-m-xylene

R.T.: 3.684 min
Delta R.T.: 0.002 min
Response: 47992360
Conc: 16.08 ng/ml m

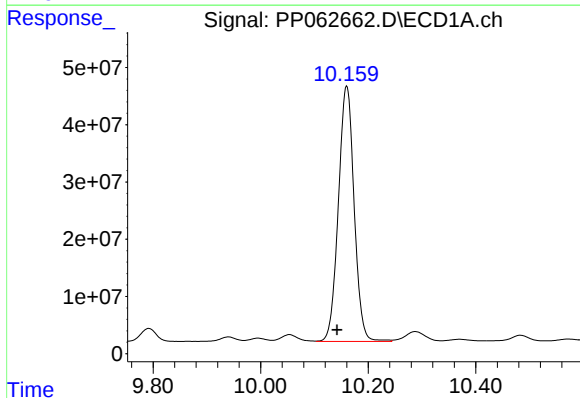

#2 Decachlorobiphenyl

R.T.: 10.160 min
Delta R.T.: 0.018 min
Response: 907361829
Conc: 629.24 ng/ml

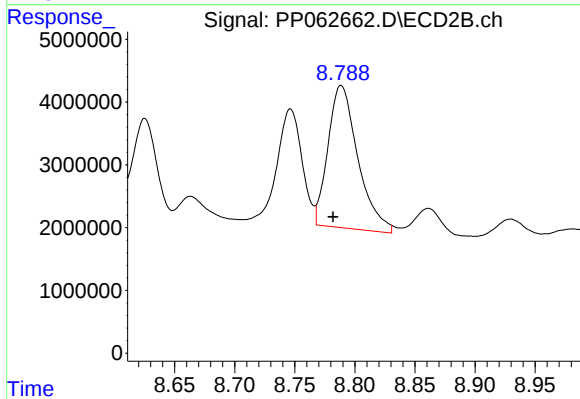

#2 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: 0.006 min
Response: 39162829
Conc: 15.38 ng/ml m