

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122820\
 Data File : PP032435.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Dec 2020 15:15
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 08:40:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 29 08:36:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	4.033	964149	973865	19.919	20.615
2) SA Decachlor...	10.590	9.313	1085408	896628	22.425	20.551

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP122820\
Data File : PP032435.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Dec 2020 15:15
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 08:40:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122820.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 29 08:36:39 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

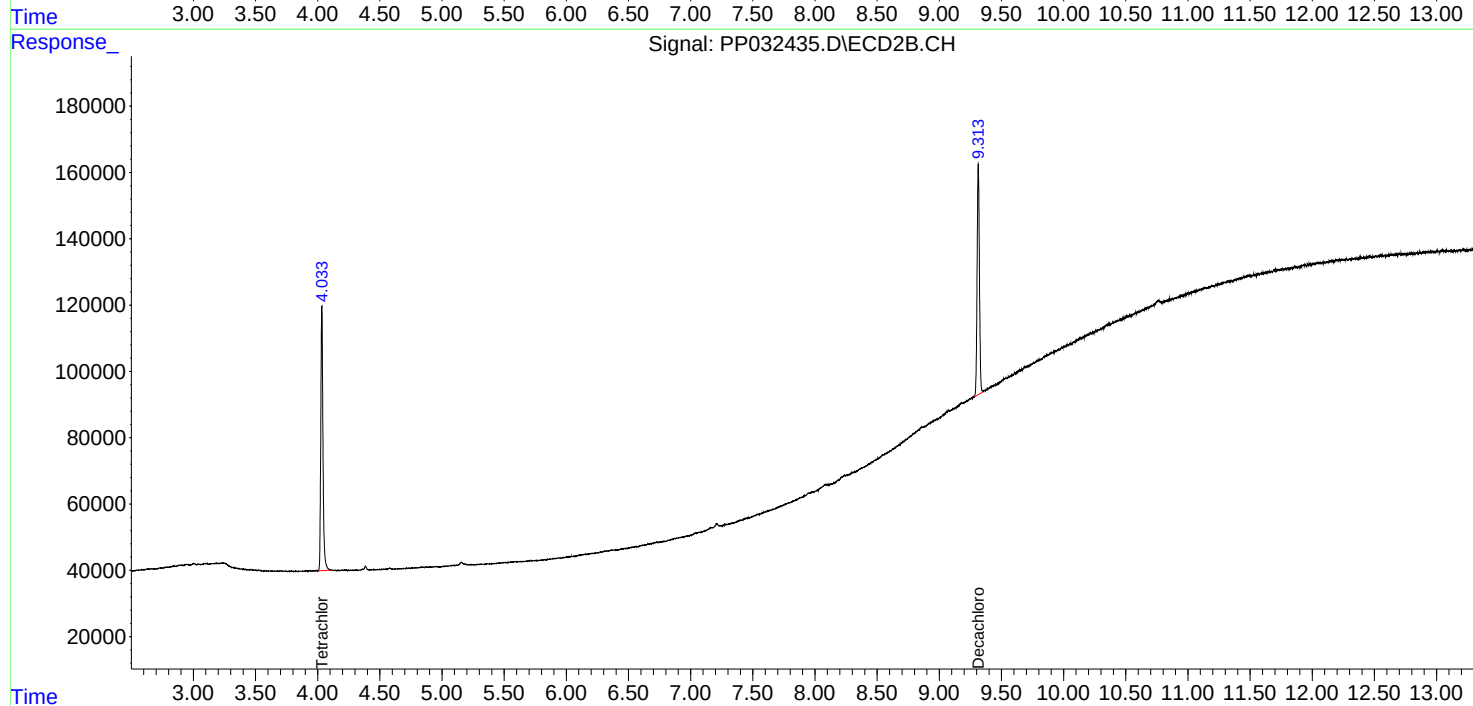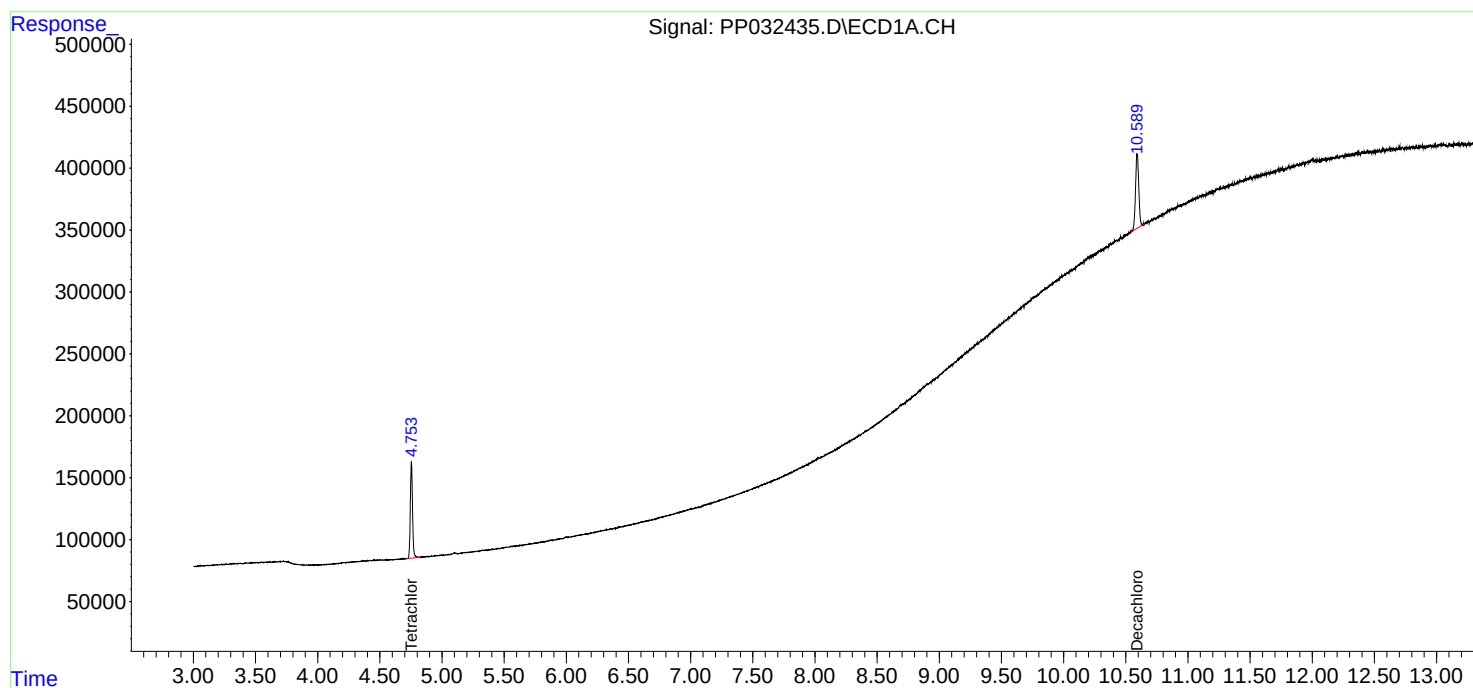


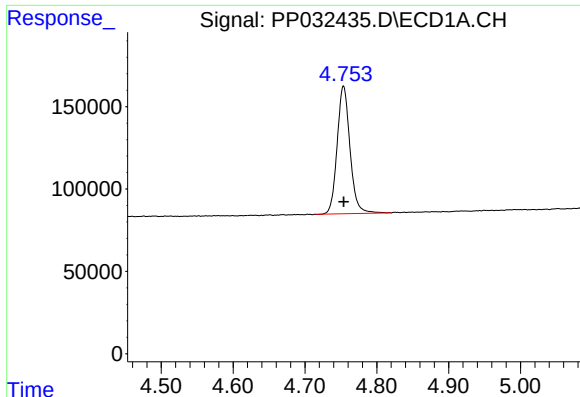

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: 0.000 min
Response: 964149
Conc: 19.92 ng/ml

Instrument :
ECD_P
ClientSampleId :

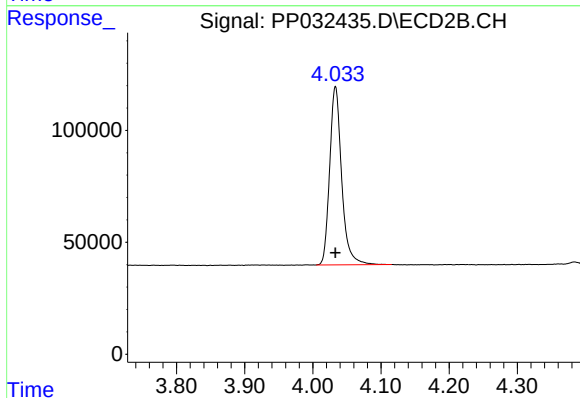


#1 Tetrachloro-m-xylene

R.T.: 4.033 min
Delta R.T.: 0.000 min
Response: 973865
Conc: 20.62 ng/ml

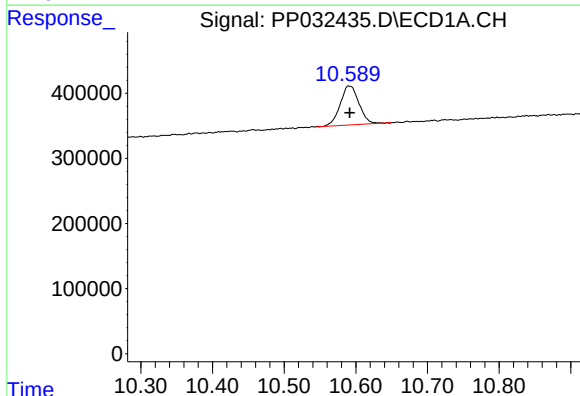

#2 Decachlorobiphenyl

R.T.: 10.590 min
Delta R.T.: -0.001 min
Response: 1085408
Conc: 22.43 ng/ml

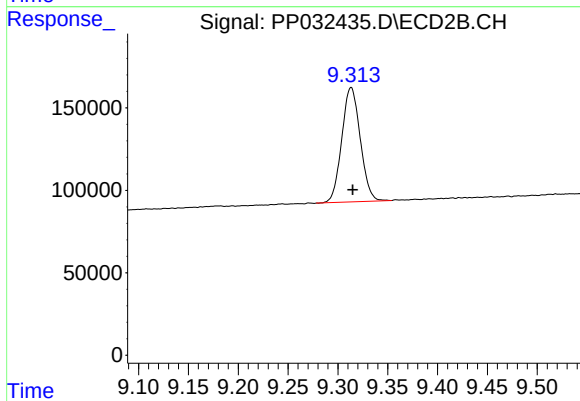

#2 Decachlorobiphenyl

R.T.: 9.313 min
Delta R.T.: -0.001 min
Response: 896628
Conc: 20.55 ng/ml