

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123020\
 Data File : PP032509.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Dec 2020 15:54
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 16:28:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 29 08:36:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.752	4.034	1286096	1140873	26.570	24.150
2)	SA Decachlor...	10.584	9.317	1070991	1007154	22.127	23.085
Target Compounds							
20)	L4 AR-1242-5	0.000	6.175f	0	94746	N.D.	86.289 #
25)	L5 AR-1248-5	0.000	6.175f	0	94746	N.D.	57.759 #
26)	L6 AR-1254-1	6.968	6.175f	-13436	94746	N.D.	38.603 #
28)	L6 AR-1254-3	7.570	0.000	147701	0	47.127	N.D. #
29)	L6 AR-1254-4	7.888f	0.000	447896	0	183.761	N.D. #
32)	L7 AR-1260-2	0.000	7.075	0	257276	N.D.	99.425 #
38)	L8 AR-1262-3	0.000	8.221	0	14594	N.D.	6.062 #
41)	L9 AR-1268-1	0.000	8.221	0	14594	N.D.	2.102 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123020\
Data File : PP032509.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Dec 2020 15:54
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 16:28:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122820.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 29 08:36:39 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

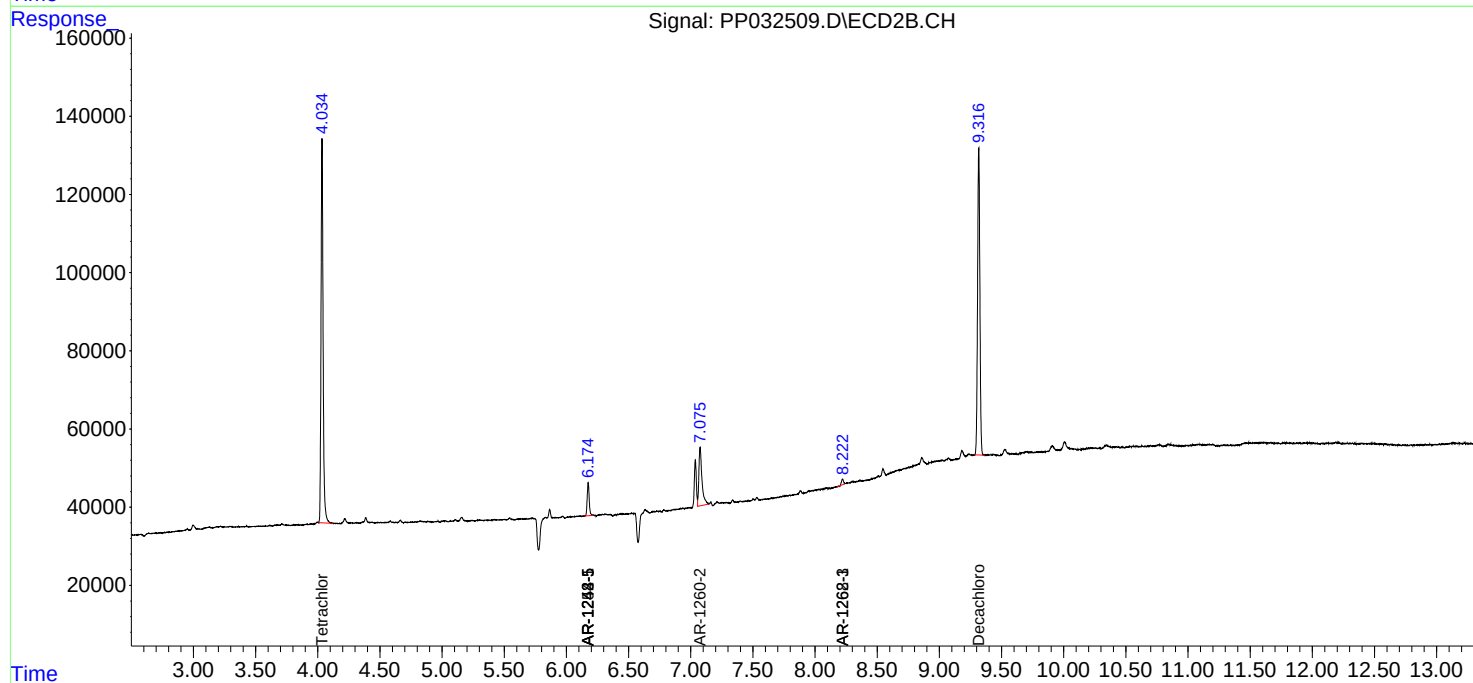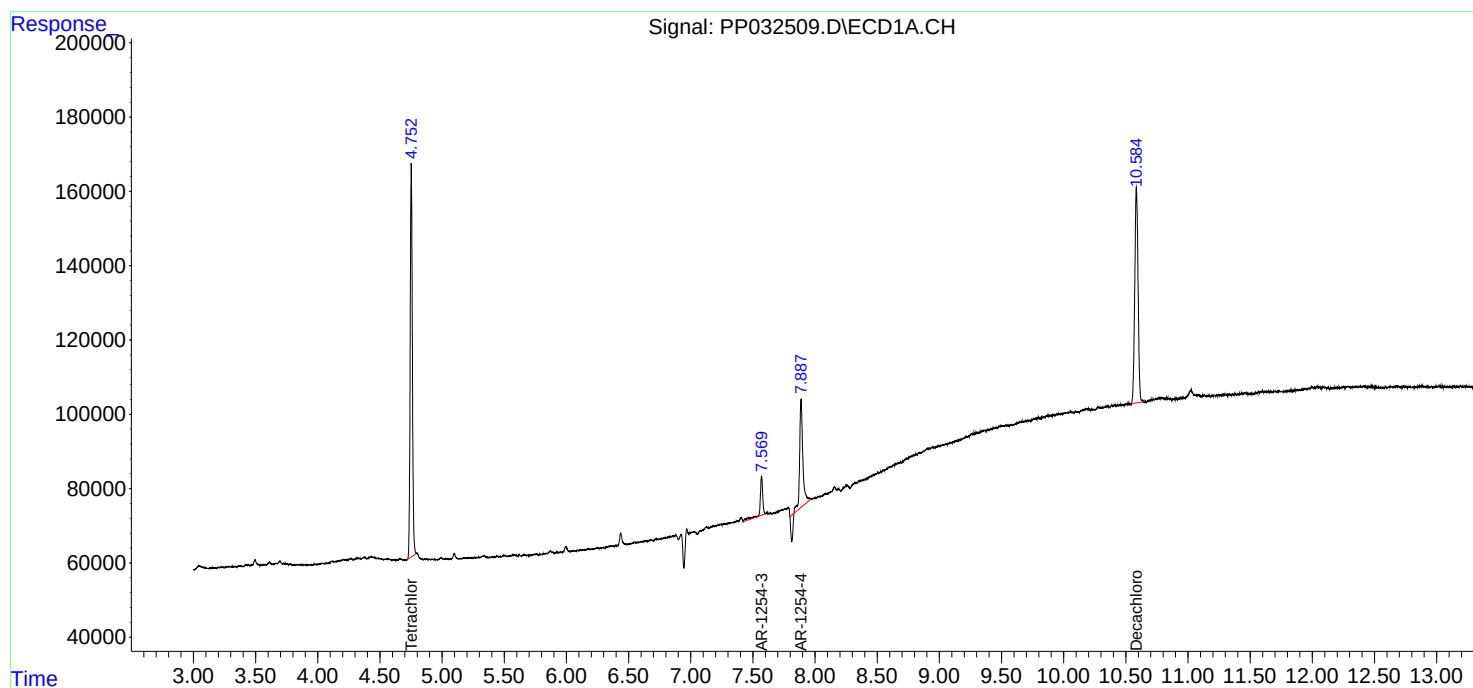


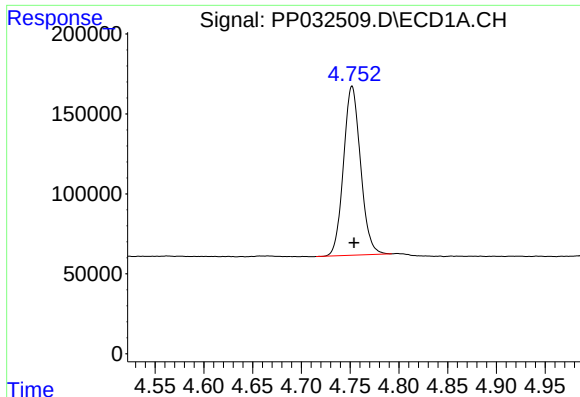

#1 Tetrachloro-m-xylene


R.T.: 4.752 min
Delta R.T.: -0.002 min
Response: 1286096
Conc: 26.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

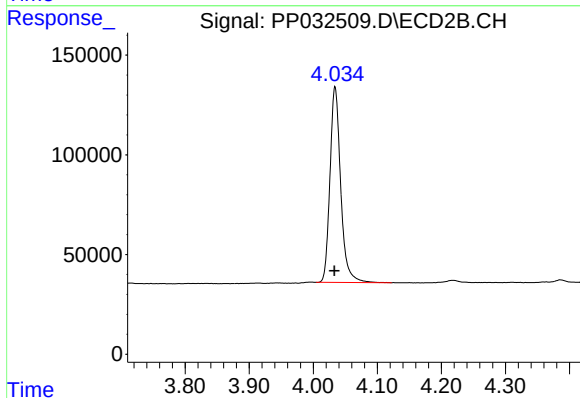


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: 0.001 min
Response: 1140873
Conc: 24.15 ng/ml

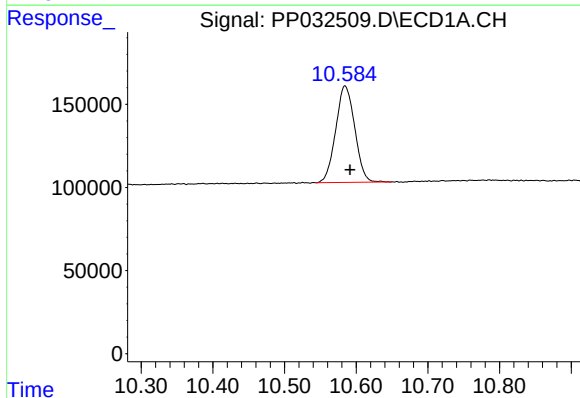


#2 Decachlorobiphenyl

R.T.: 10.584 min
Delta R.T.: -0.007 min
Response: 1070991
Conc: 22.13 ng/ml

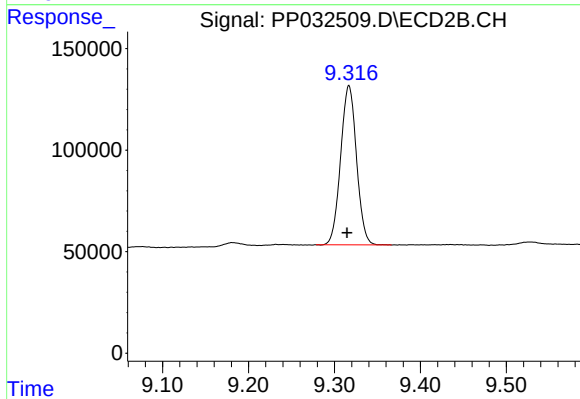

#2 Decachlorobiphenyl


R.T.: 9.317 min
Delta R.T.: 0.002 min
Response: 1007154
Conc: 23.08 ng/ml

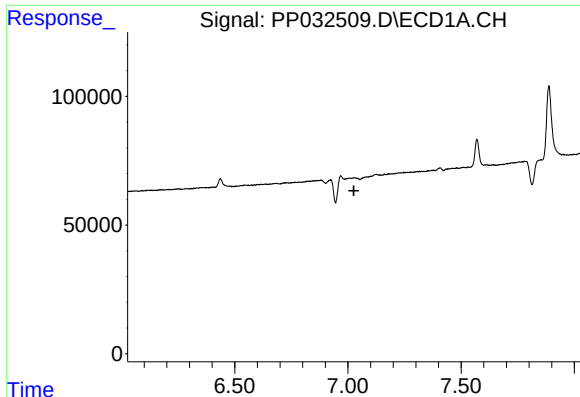

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.026 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

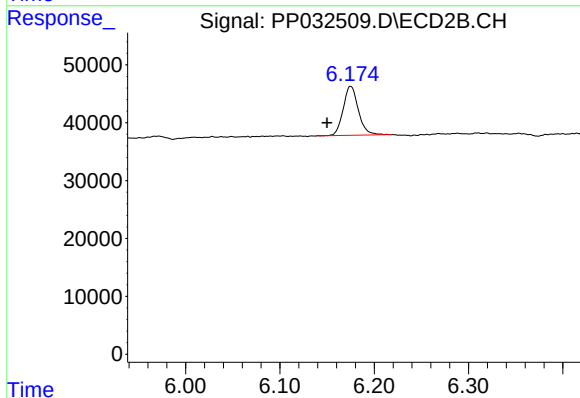


#20 AR-1242-5

R.T.: 6.175 min
Delta R.T.: 0.025 min
Response: 94746
Conc: 86.29 ng/ml

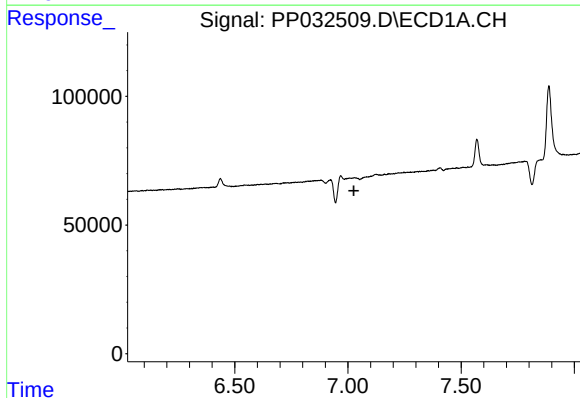


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.026 min
Response: 0
Conc: N.D.

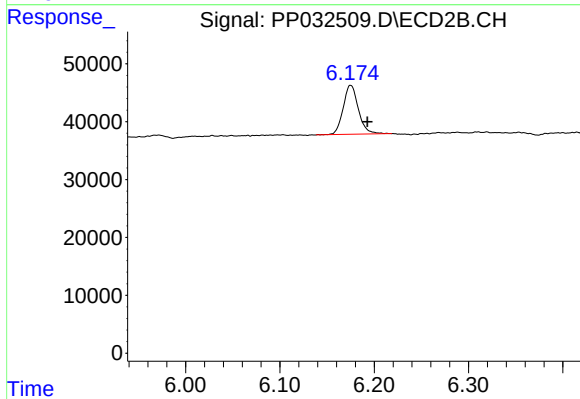

#25 AR-1248-5


R.T.: 6.175 min
Delta R.T.: -0.018 min
Response: 94746
Conc: 57.76 ng/ml

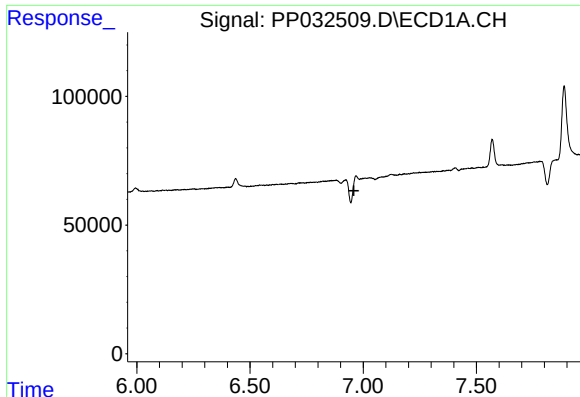

#26 AR-1254-1


R.T.: 6.968 min
Delta R.T.: 0.010 min
Response: -13436
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

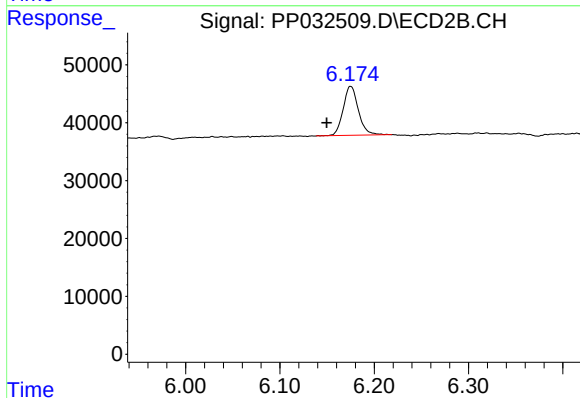


#26 AR-1254-1

R.T.: 6.175 min
Delta R.T.: 0.025 min
Response: 94746
Conc: 38.60 ng/ml

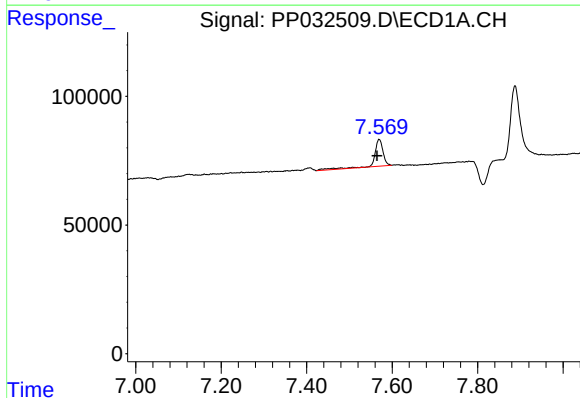


#28 AR-1254-3

R.T.: 7.570 min
Delta R.T.: 0.005 min
Response: 147701
Conc: 47.13 ng/ml

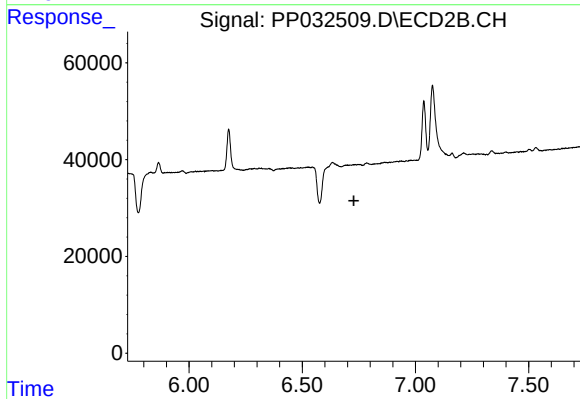

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.728 min
Response: 0
Conc: N.D.

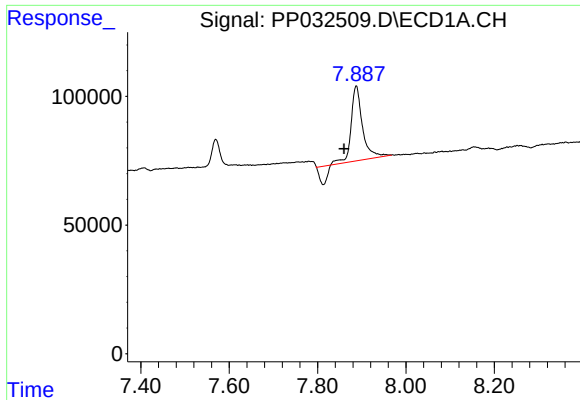

#29 AR-1254-4


R.T.: 7.888 min
Delta R.T.: 0.028 min
Response: 447896
Conc: 183.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

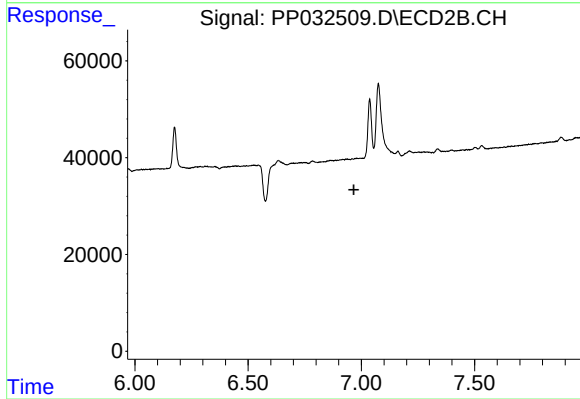


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

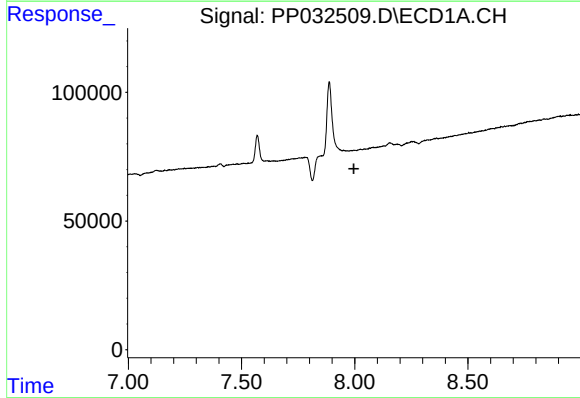


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.997 min
Response: 0
Conc: N.D.

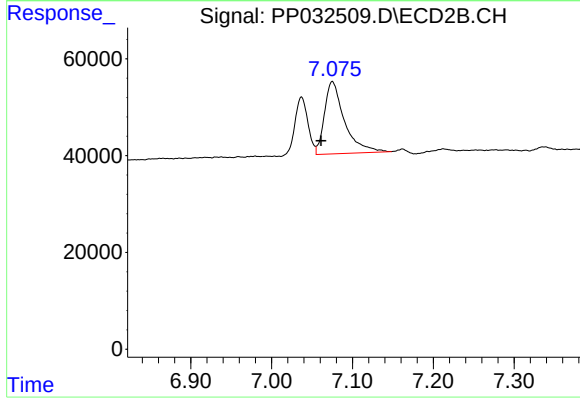

#32 AR-1260-2


R.T.: 7.075 min
Delta R.T.: 0.014 min
Response: 257276
Conc: 99.42 ng/ml

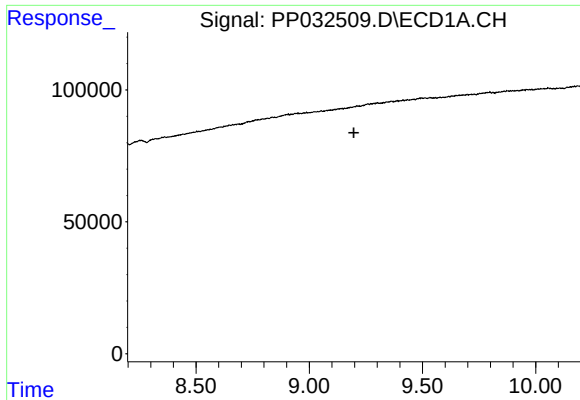

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

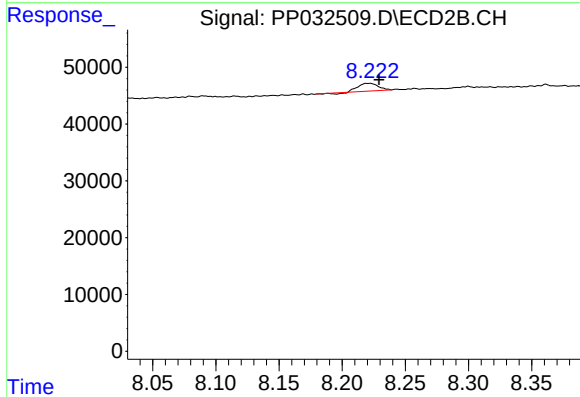


#38 AR-1262-3

R.T.: 8.221 min
Delta R.T.: -0.008 min
Response: 14594
Conc: 6.06 ng/ml

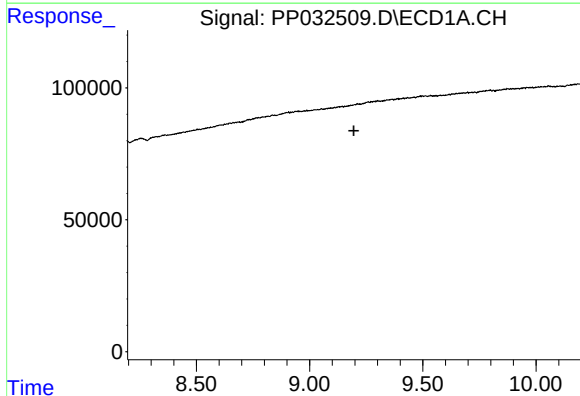

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.196 min
Response: 0
Conc: N.D.

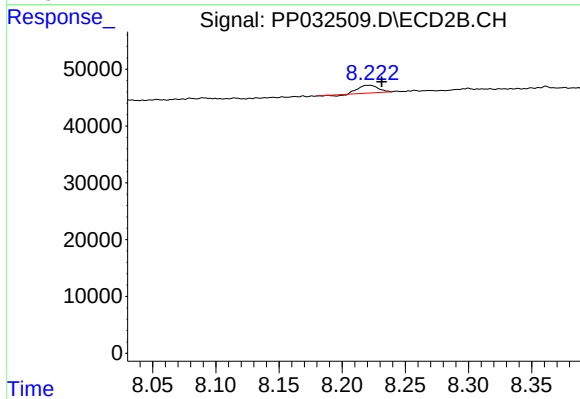

#41 AR-1268-1

R.T.: 8.221 min
Delta R.T.: -0.010 min
Response: 14594
Conc: 2.10 ng/ml