

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123020\
 Data File : PP032501.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Dec 2020 12:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 12:51:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 29 08:36:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.758	4.032	1232499	1059504	25.463	22.428
2) SA Decachlor...	10.591	9.316	1135179	1062737	23.454	24.359

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123020\
Data File : PP032501.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Dec 2020 12:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 12:51:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122820.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 29 08:36:39 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

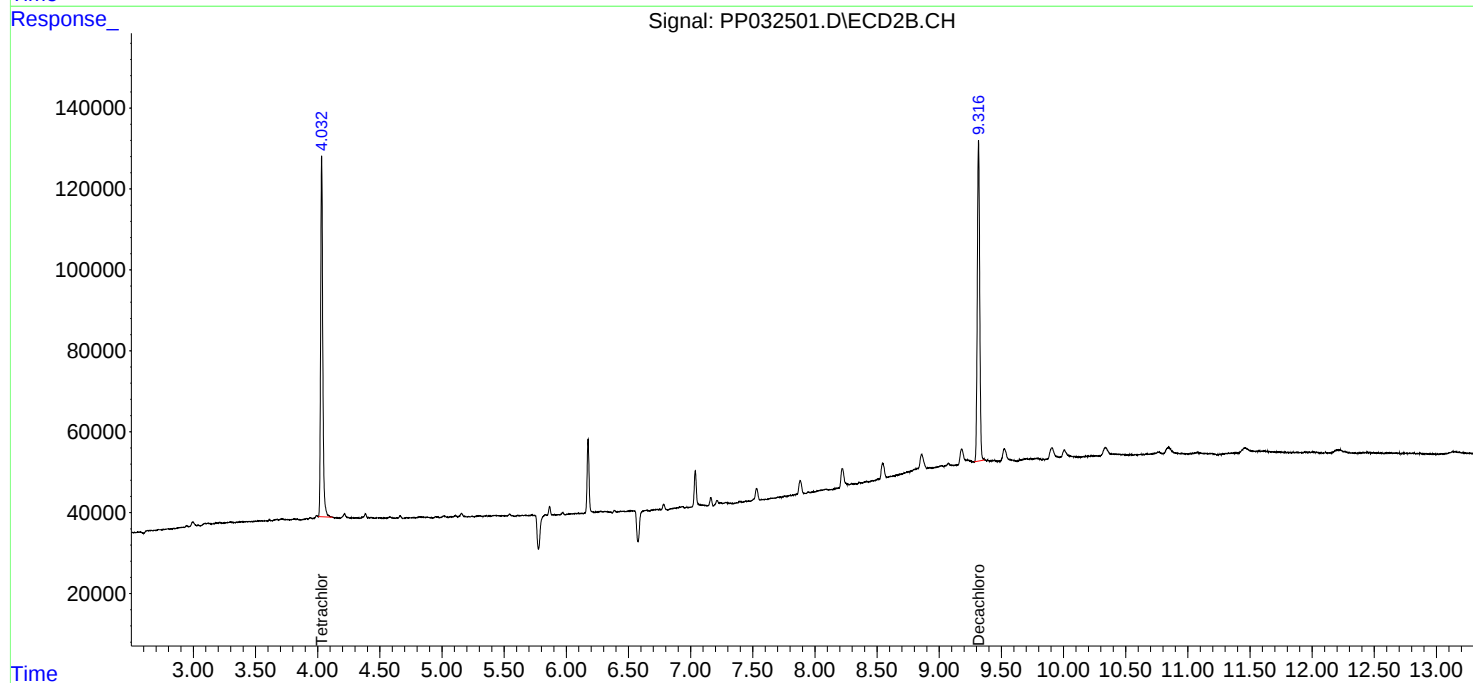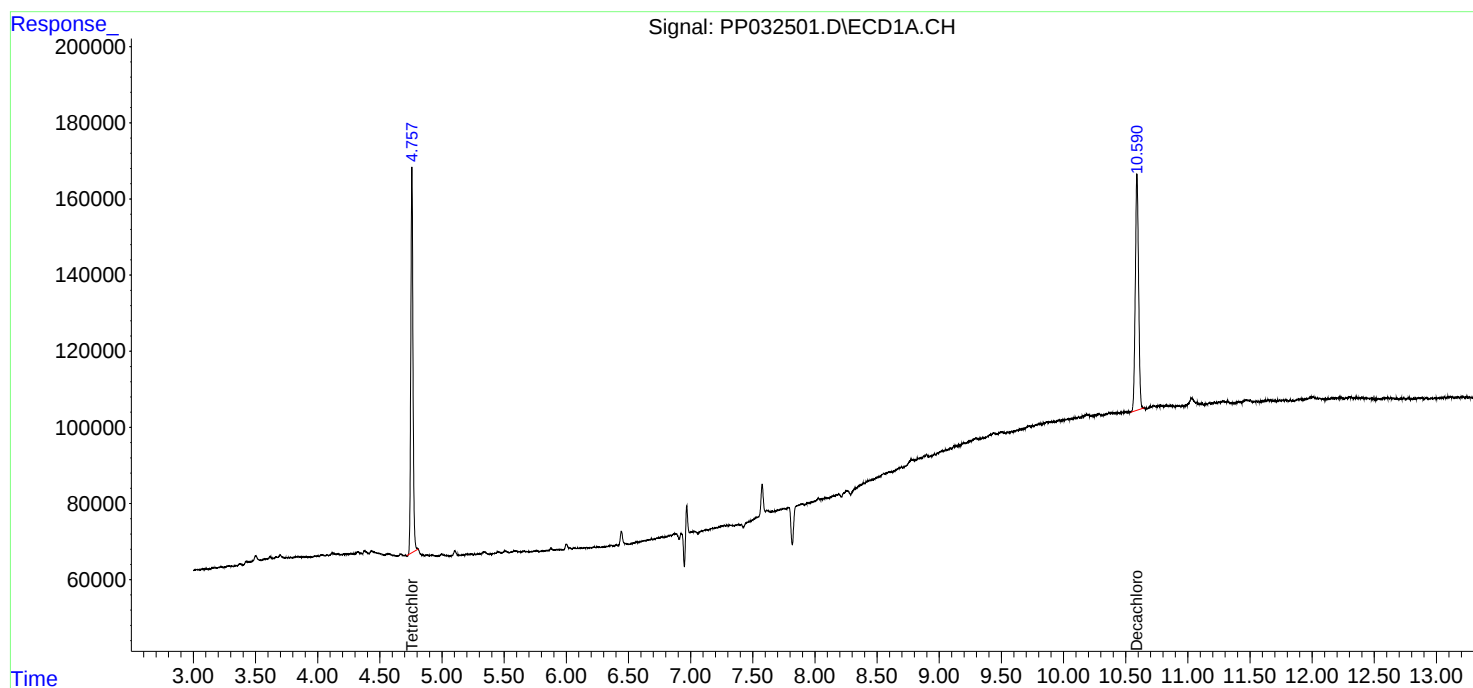


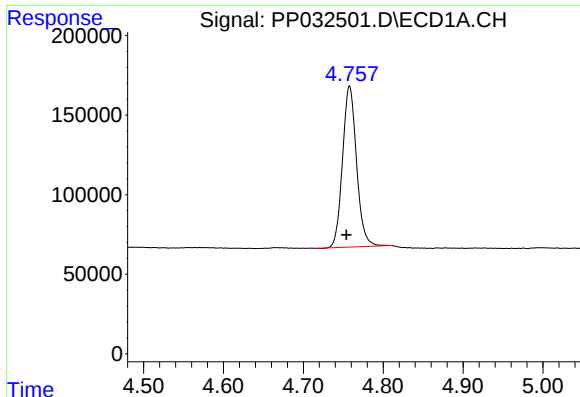

#1 Tetrachloro-m-xylene


R.T.: 4.758 min
Delta R.T.: 0.004 min
Response: 1232499
Conc: 25.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

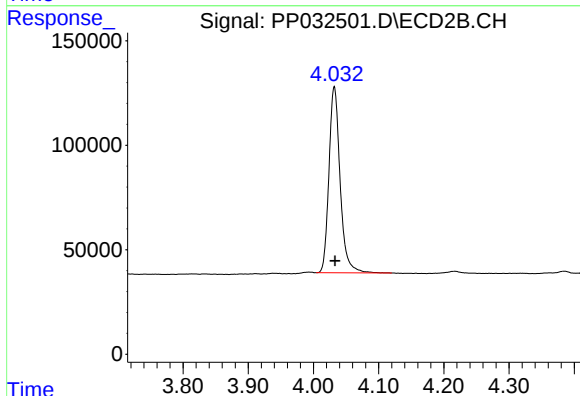


#1 Tetrachloro-m-xylene

R.T.: 4.032 min
Delta R.T.: -0.001 min
Response: 1059504
Conc: 22.43 ng/ml

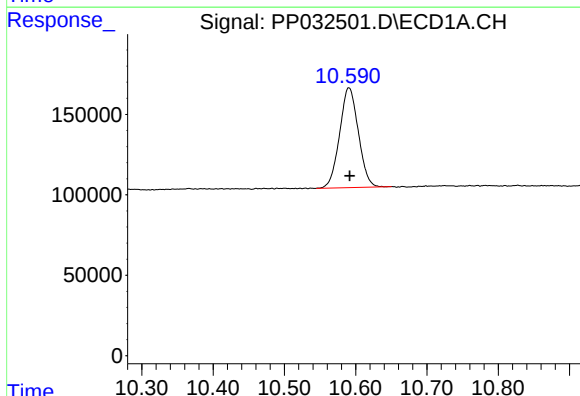

#2 Decachlorobiphenyl

R.T.: 10.591 min
Delta R.T.: 0.000 min
Response: 1135179
Conc: 23.45 ng/ml

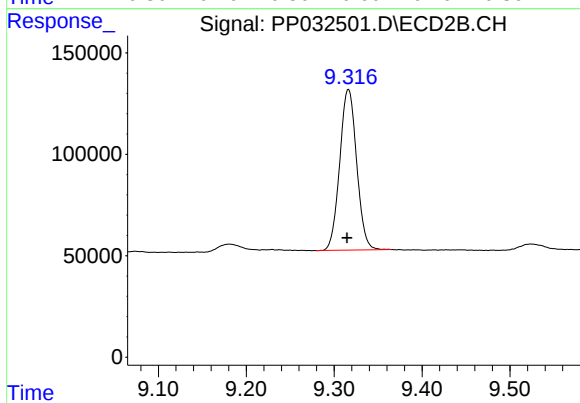

#2 Decachlorobiphenyl

R.T.: 9.316 min
Delta R.T.: 0.002 min
Response: 1062737
Conc: 24.36 ng/ml