

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123021\
 Data File : PP042406.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Dec 2021 12:46
 Operator : AJ\MA
 Sample : M5196-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMPOSITE-SAMPLE-2-SHALLOW

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 09:46:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 24 23:47:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.918	4.055	292358	492088	22.267	21.545
2) SA Decachlor...	10.912	9.399	292984	375762	24.054	23.236

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123021\
Data File : PP042406.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Dec 2021 12:46
Operator : AJ\MA
Sample : M5196-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
COMPOSITE-SAMPLE-2-SHALLOW

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 09:46:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 24 23:47:53 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

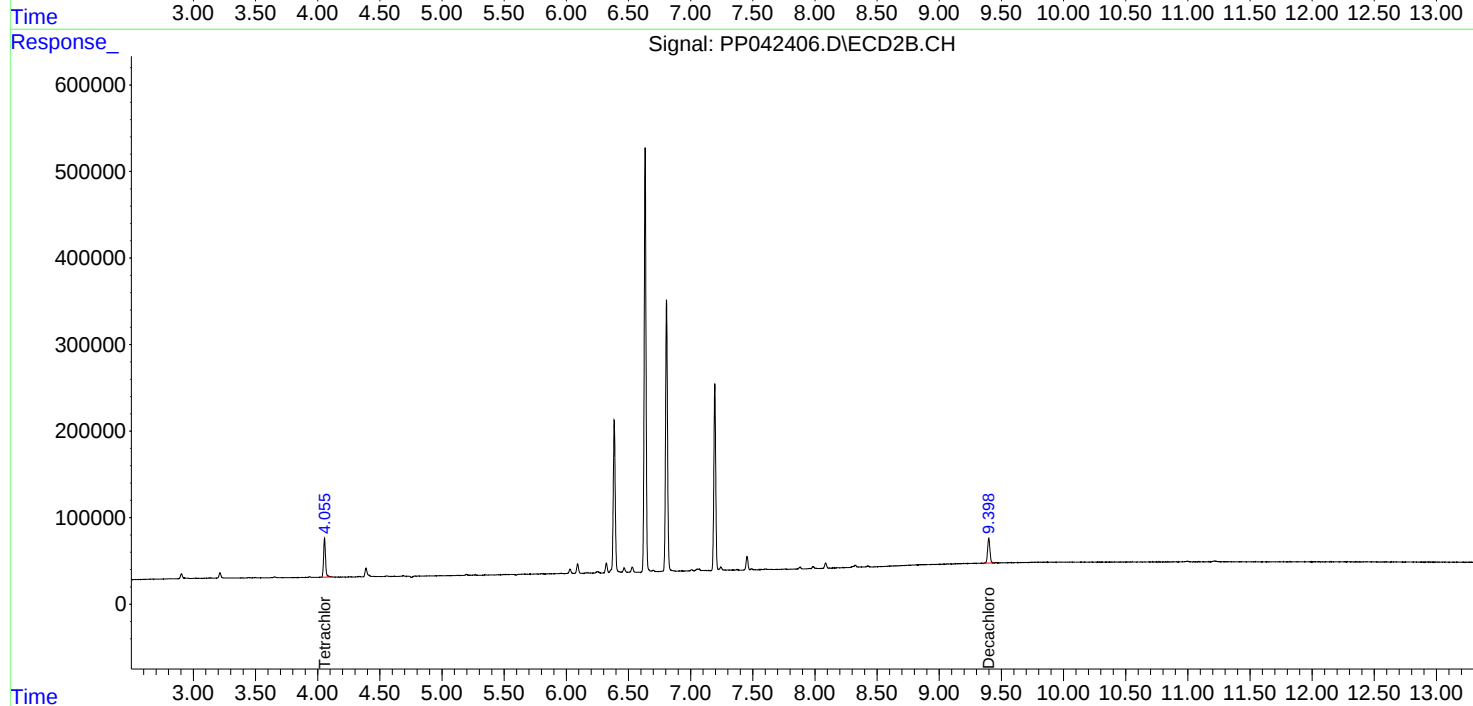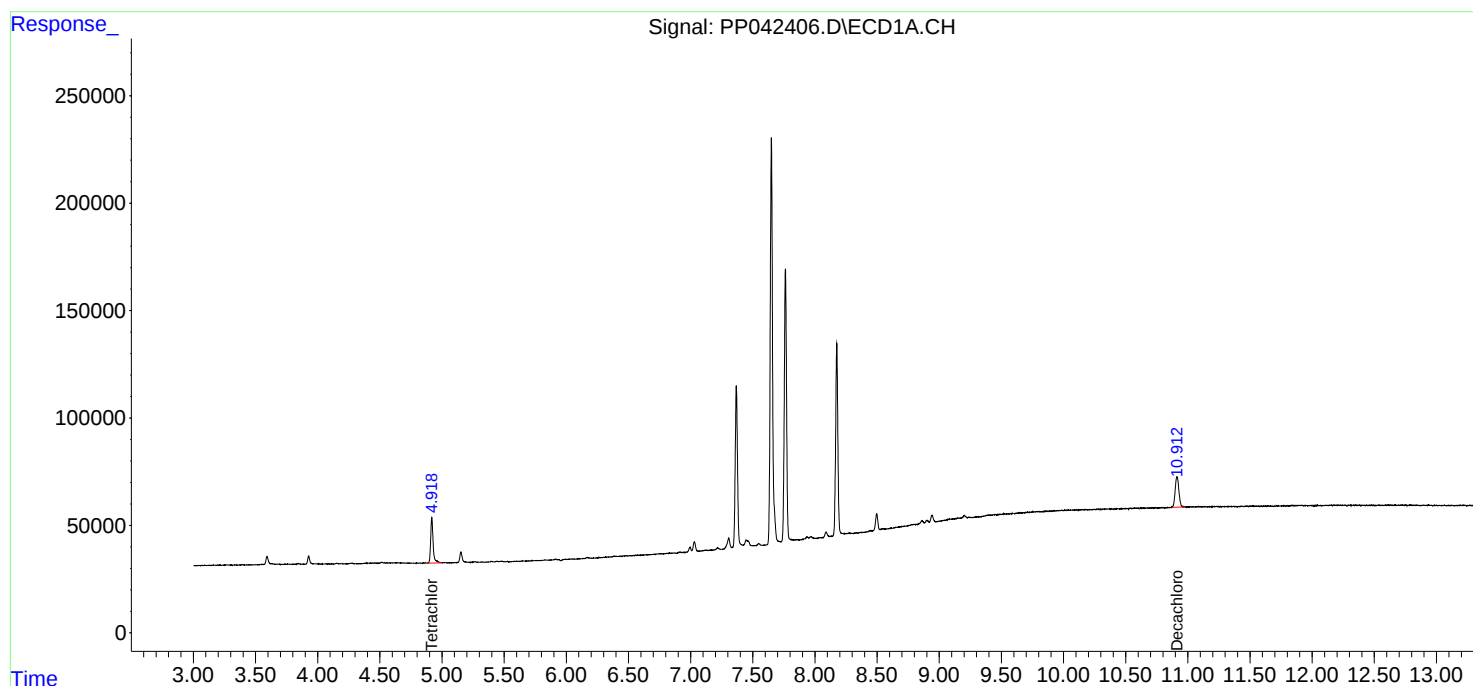


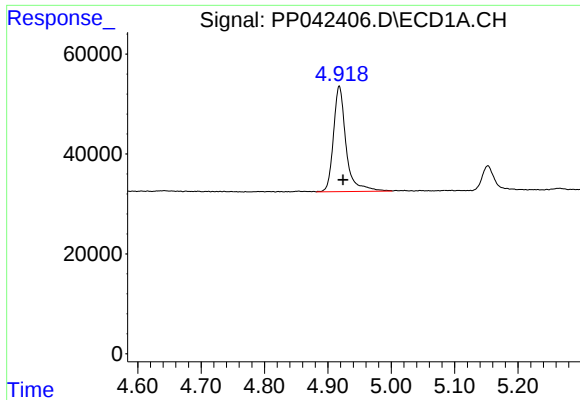

#1 Tetrachloro-m-xylene


R.T.: 4.918 min
Delta R.T.: -0.006 min
Response: 292358
Conc: 22.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMPOSITE-SAMPLE-2-SHALLOW

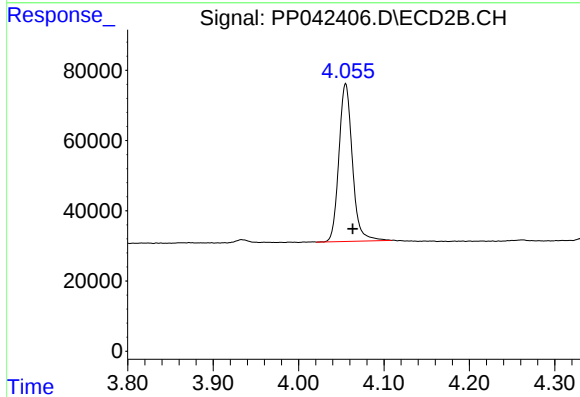


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: -0.008 min
Response: 492088
Conc: 21.55 ng/ml

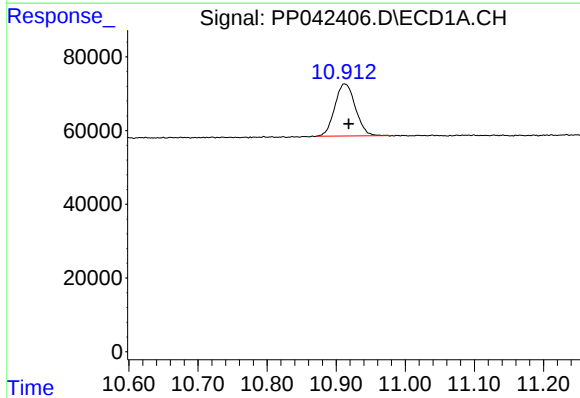

#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: -0.006 min
Response: 292984
Conc: 24.05 ng/ml

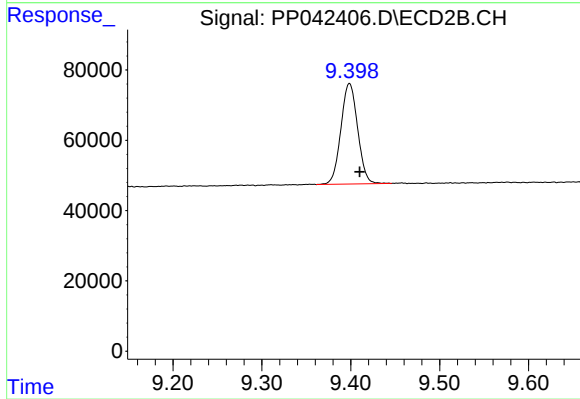

#2 Decachlorobiphenyl

R.T.: 9.399 min
Delta R.T.: -0.011 min
Response: 375762
Conc: 23.24 ng/ml