

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123021\
 Data File : PP042407.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Dec 2021 13:03
 Operator : AJ\MA
 Sample : M5196-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMPOSITE-SAMPLE-2-DEEP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 09:47:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 24 23:47:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.918	4.055	280561	476423	21.368	20.860
2)	SA Decachlor...	10.912	9.398	278269	360029	22.846	22.263

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123021\
Data File : PP042407.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Dec 2021 13:03
Operator : AJ\MA
Sample : M5196-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
COMPOSITE-SAMPLE-2-DEEP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 09:47:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 24 23:47:53 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

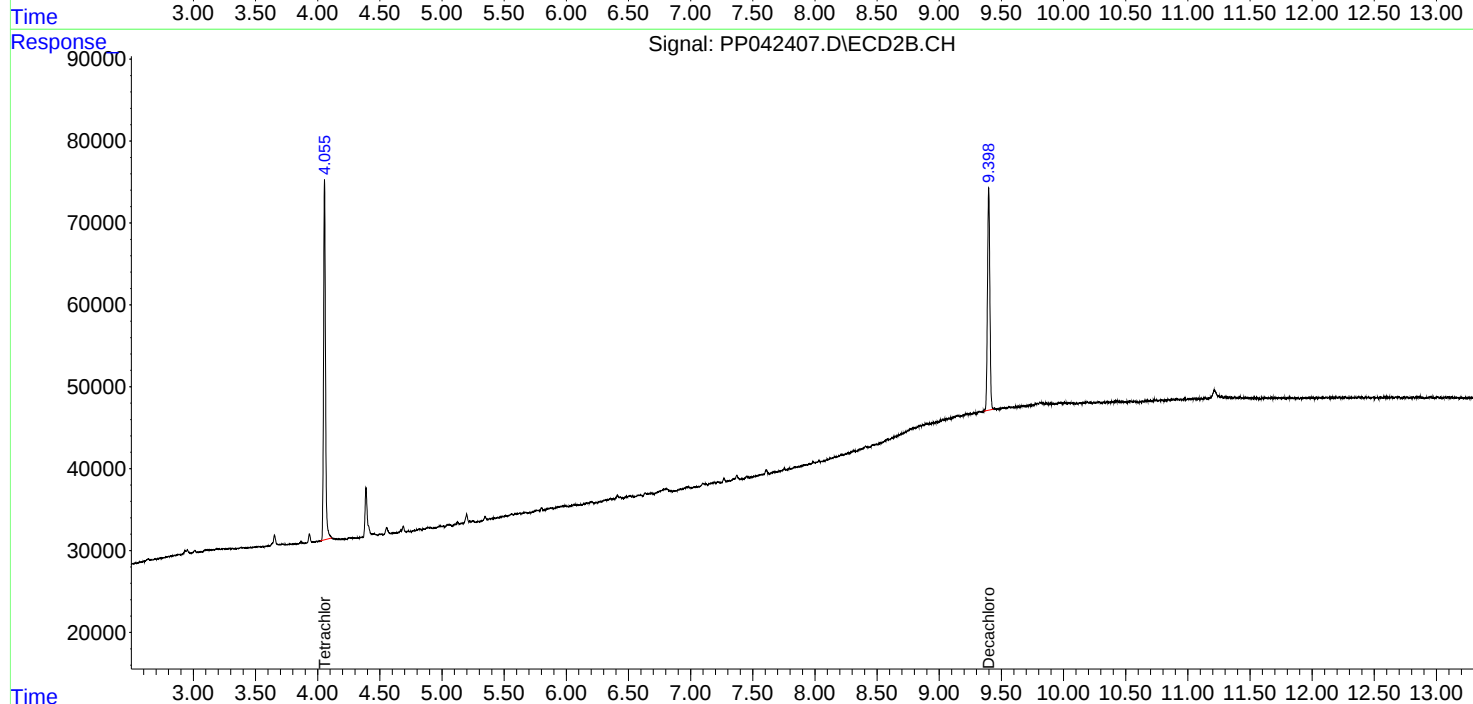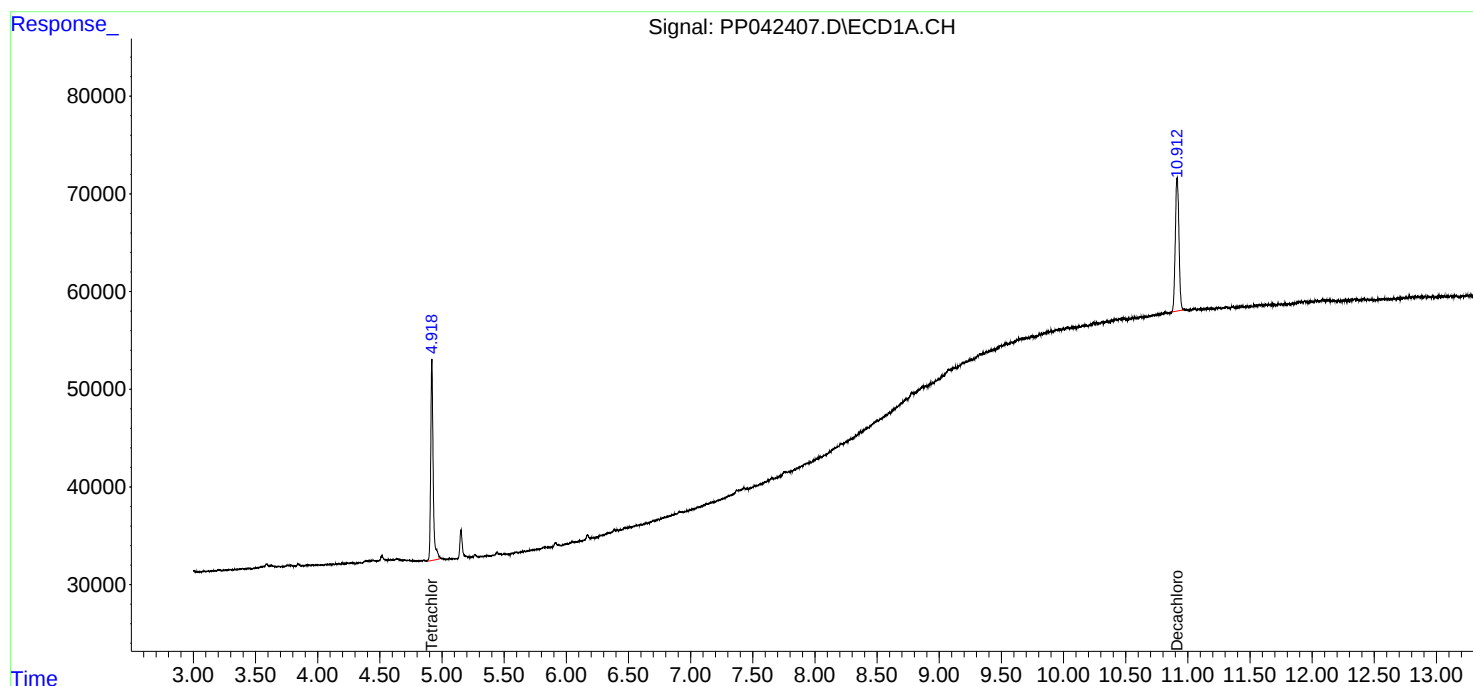


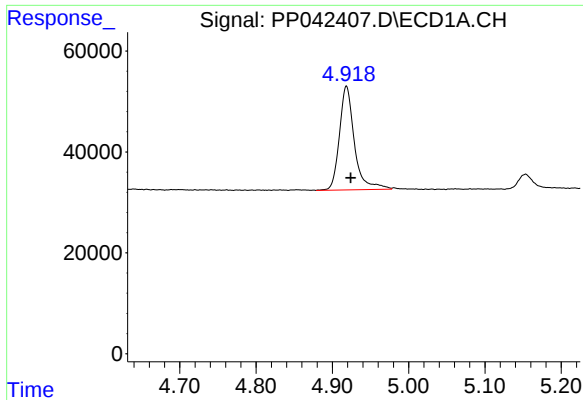

#1 Tetrachloro-m-xylene


R.T.: 4.918 min
Delta R.T.: -0.006 min
Response: 280561
Conc: 21.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMPOSITE-SAMPLE-2-DEEP

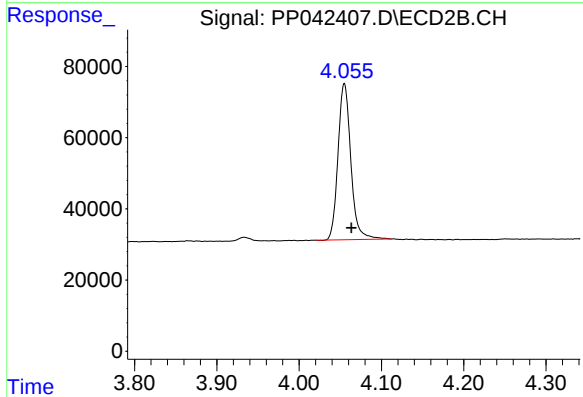


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: -0.008 min
Response: 476423
Conc: 20.86 ng/ml

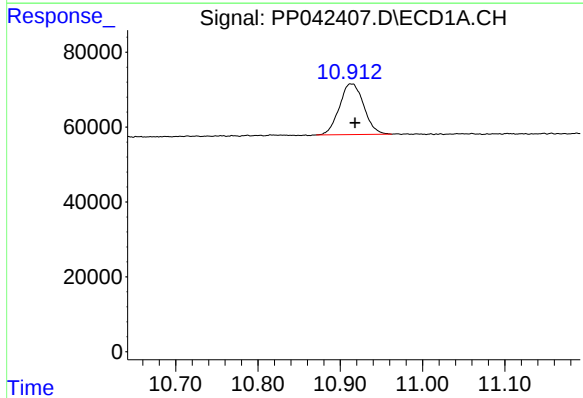

#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: -0.006 min
Response: 278269
Conc: 22.85 ng/ml

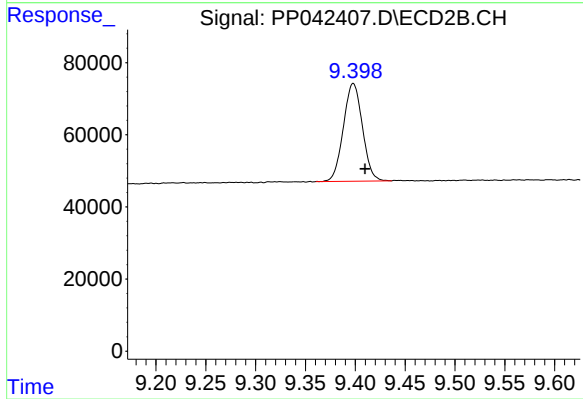

#2 Decachlorobiphenyl

R.T.: 9.398 min
Delta R.T.: -0.012 min
Response: 360029
Conc: 22.26 ng/ml