

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123021\
 Data File : PP042422.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Dec 2021 17:13
 Operator : AJ\MA
 Sample : M5256-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BU-03-122921

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 01:24:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 24 23:47:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.917	4.054	269618	466272	20.535	20.415
2)	SA Decachlor...	10.911	9.396f	224528	267345	18.434	16.532

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123021\
Data File : PP042422.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Dec 2021 17:13
Operator : AJ\MA
Sample : M5256-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BU-03-122921

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 01:24:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 24 23:47:53 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

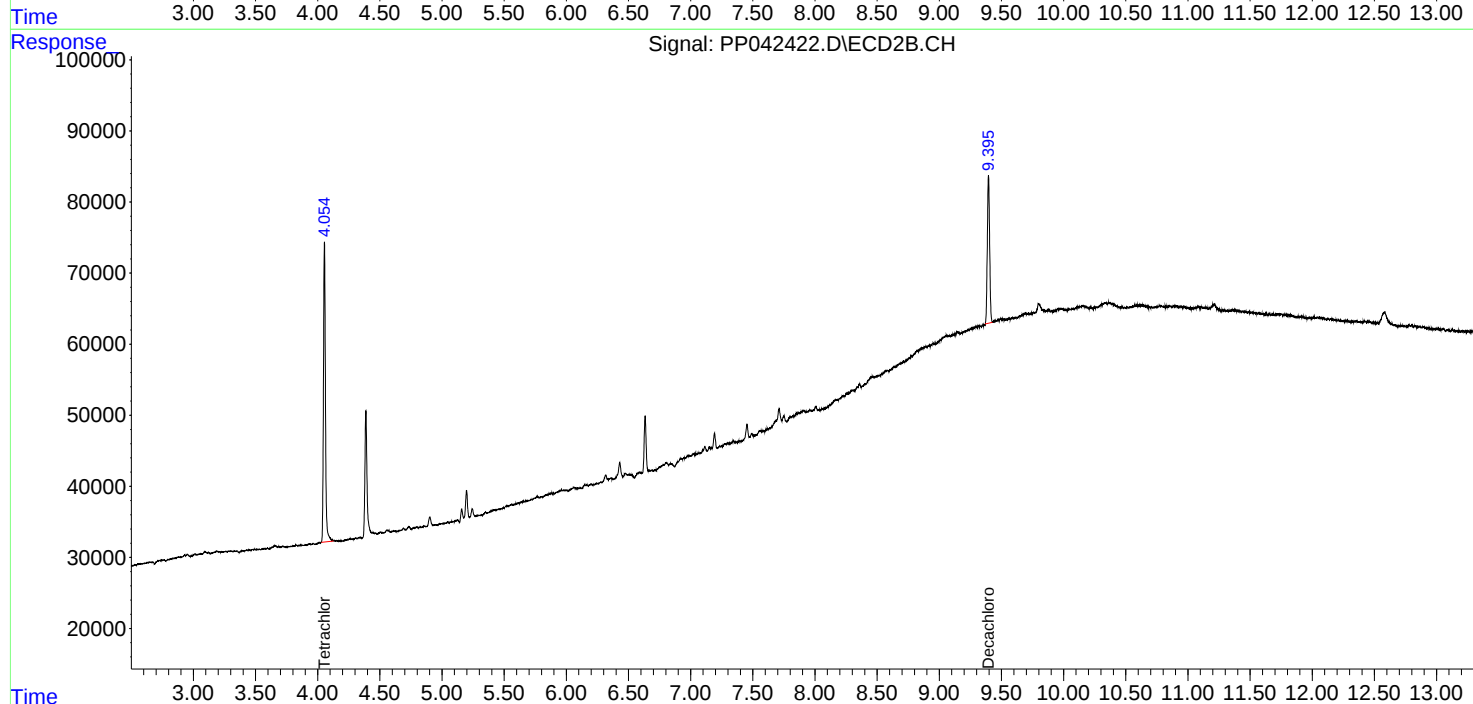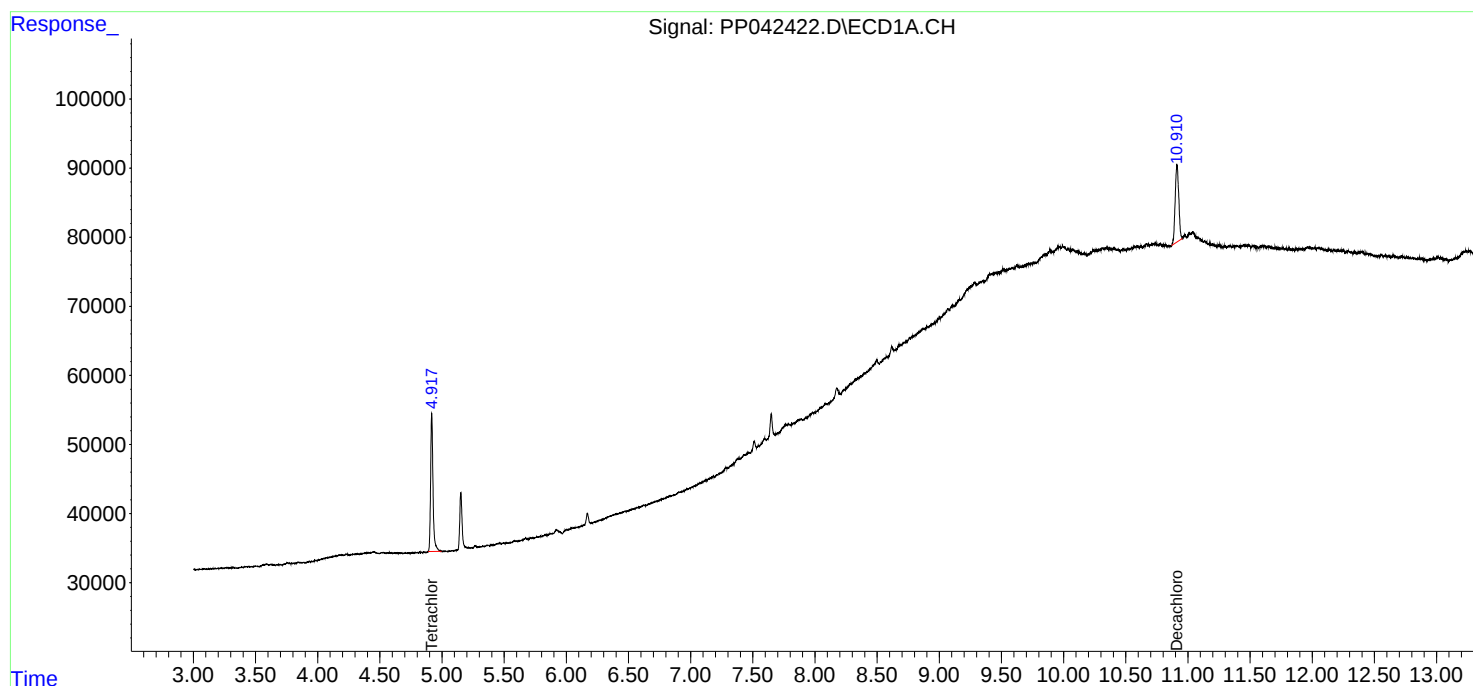


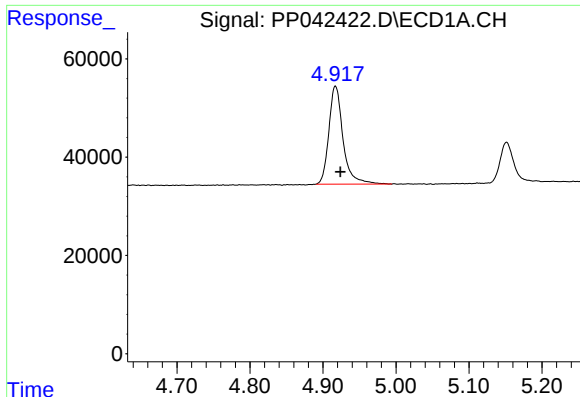

#1 Tetrachloro-m-xylene


R.T.: 4.917 min
Delta R.T.: -0.007 min
Response: 269618
Conc: 20.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
BU-03-122921

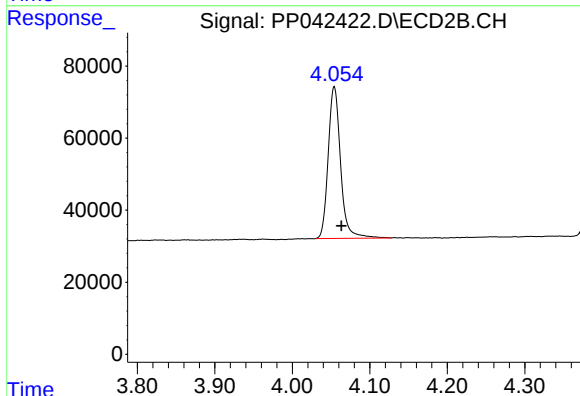


#1 Tetrachloro-m-xylene

R.T.: 4.054 min
Delta R.T.: -0.009 min
Response: 466272
Conc: 20.42 ng/ml

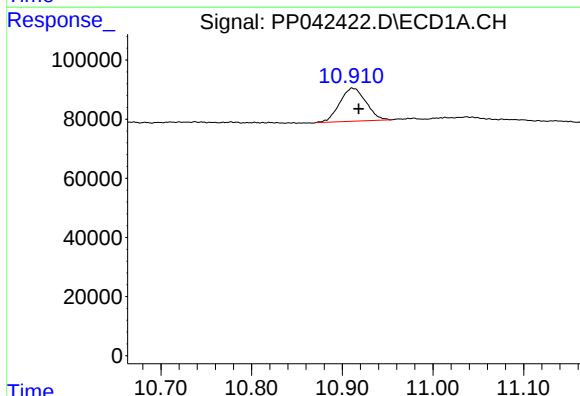

#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.007 min
Response: 224528
Conc: 18.43 ng/ml

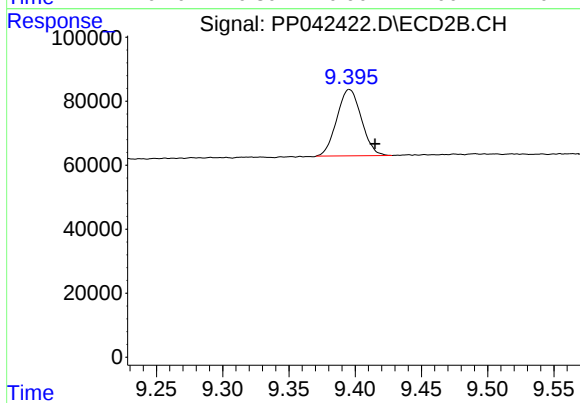

#2 Decachlorobiphenyl

R.T.: 9.396 min
Delta R.T.: -0.019 min
Response: 267345
Conc: 16.53 ng/ml