

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123120\
 Data File : PP032514.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Dec 2020 10:03
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 12:00:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 29 08:36:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	4.034	1476742	1192741	30.509	25.248
2) SA Decachlor...	10.600	9.321	1264400	1128783	26.123	25.873

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP123120\
Data File : PP032514.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Dec 2020 10:03
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 12:00:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122820.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 29 08:36:39 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

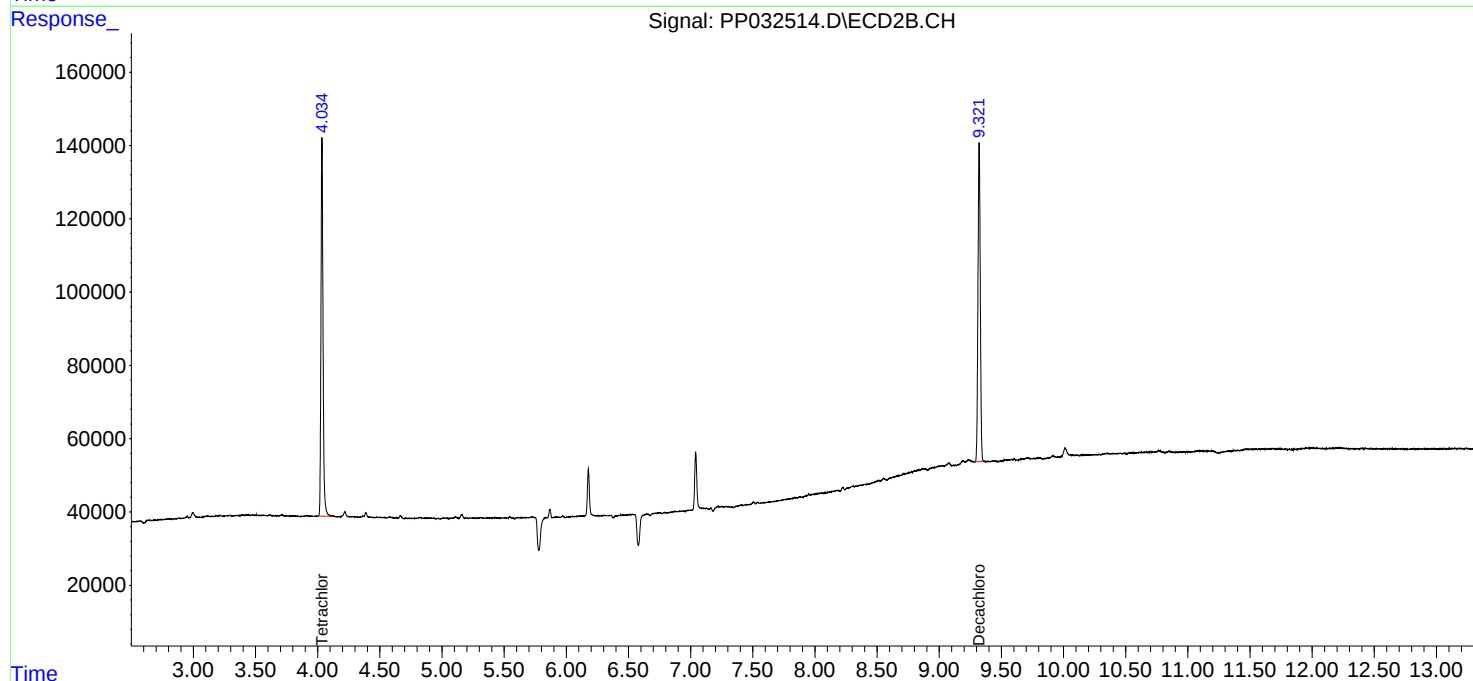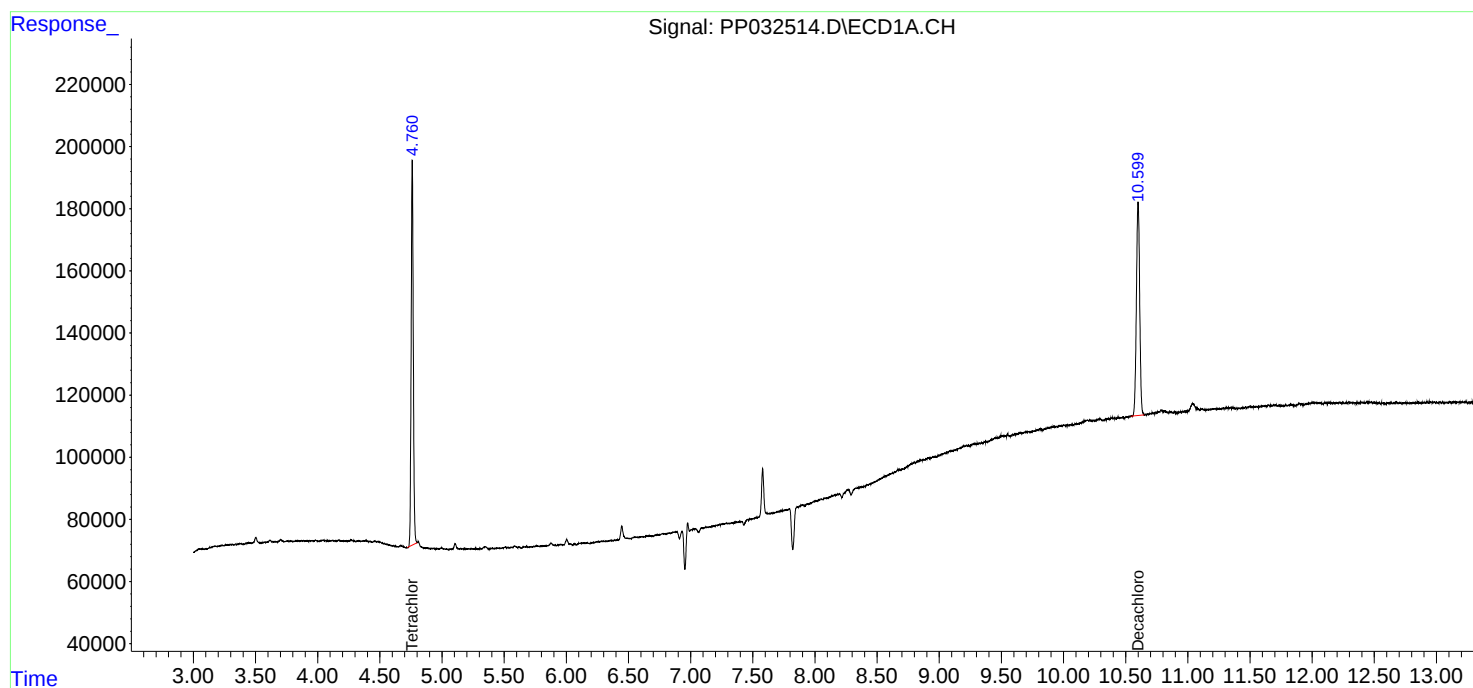


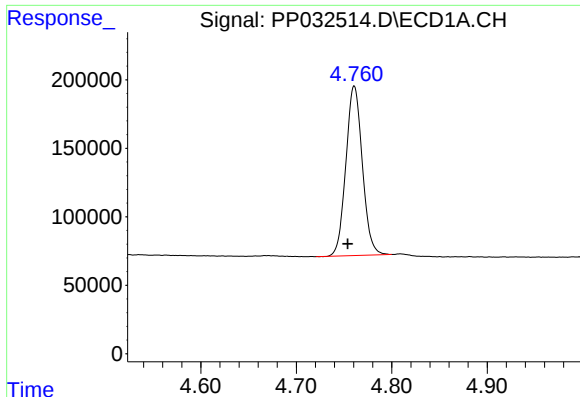

#1 Tetrachloro-m-xylene


R.T.: 4.761 min
Delta R.T.: 0.007 min
Response: 1476742
Conc: 30.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

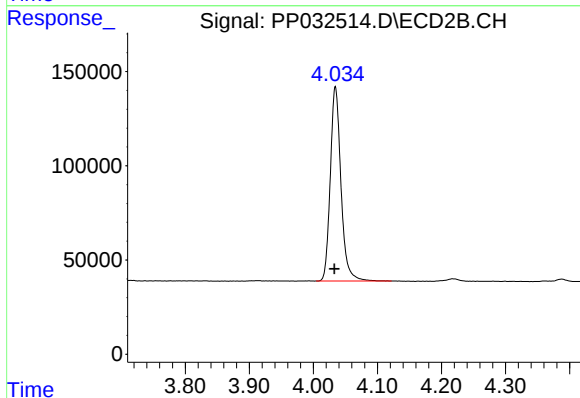


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: 0.001 min
Response: 1192741
Conc: 25.25 ng/ml

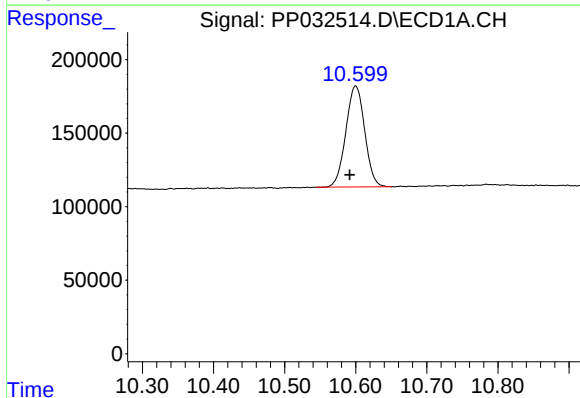

#2 Decachlorobiphenyl

R.T.: 10.600 min
Delta R.T.: 0.008 min
Response: 1264400
Conc: 26.12 ng/ml

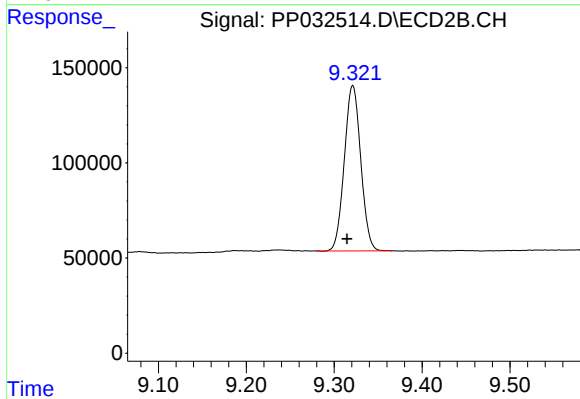

#2 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: 0.006 min
Response: 1128783
Conc: 25.87 ng/ml