

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091225\
 Data File : PP075105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2025 11:48
 Operator : YP\AJ
 Sample : Q3073-02 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BEL-25-0023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/15/2025
 Supervised By :mohammad ahmed 09/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 12:37:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.651	3.794	4122002	7246589	3.369m	1.499m#
2) SA Decachlor...	10.426	8.803	2680768	15156022	2.715m	2.021 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091225\
Data File : PP075105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2025 11:48
Operator : YP\AJ
Sample : Q3073-02 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BEL-25-0023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/15/2025
Supervised By :mohammad ahmed 09/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 12:37:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

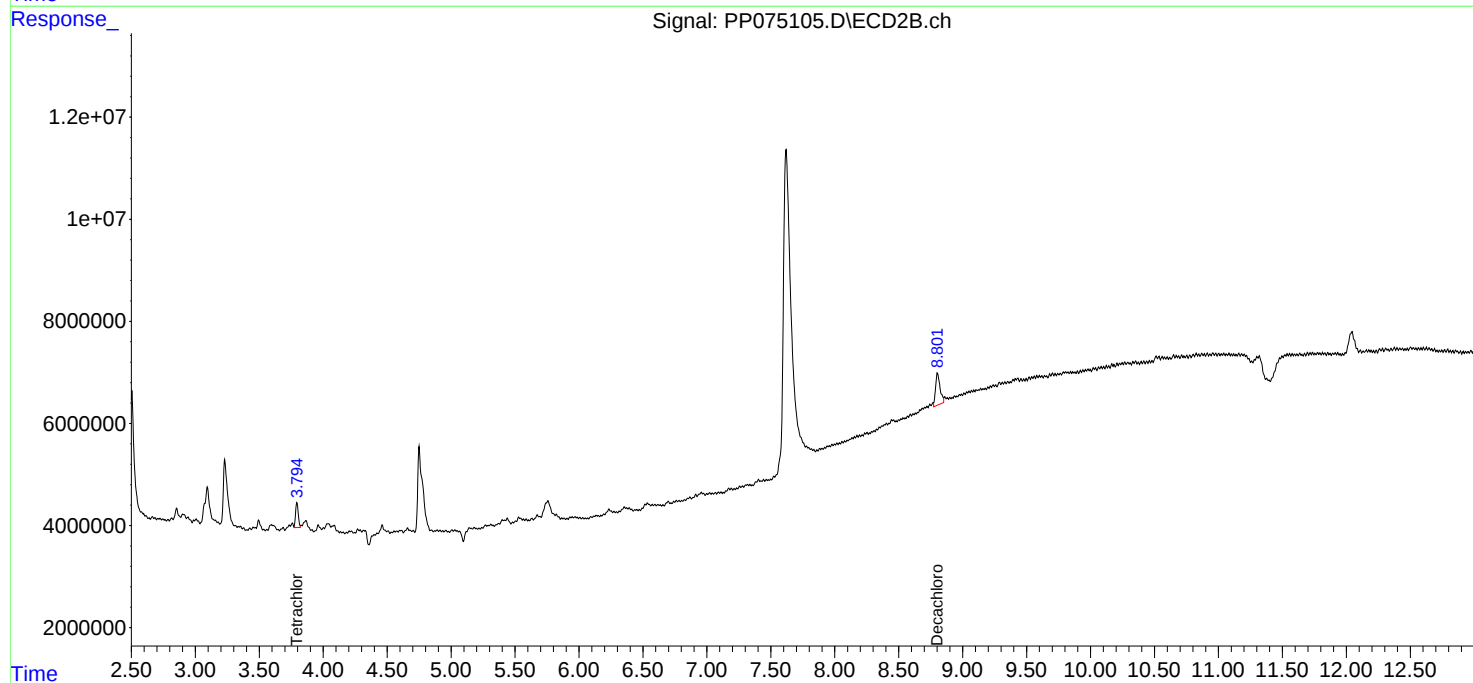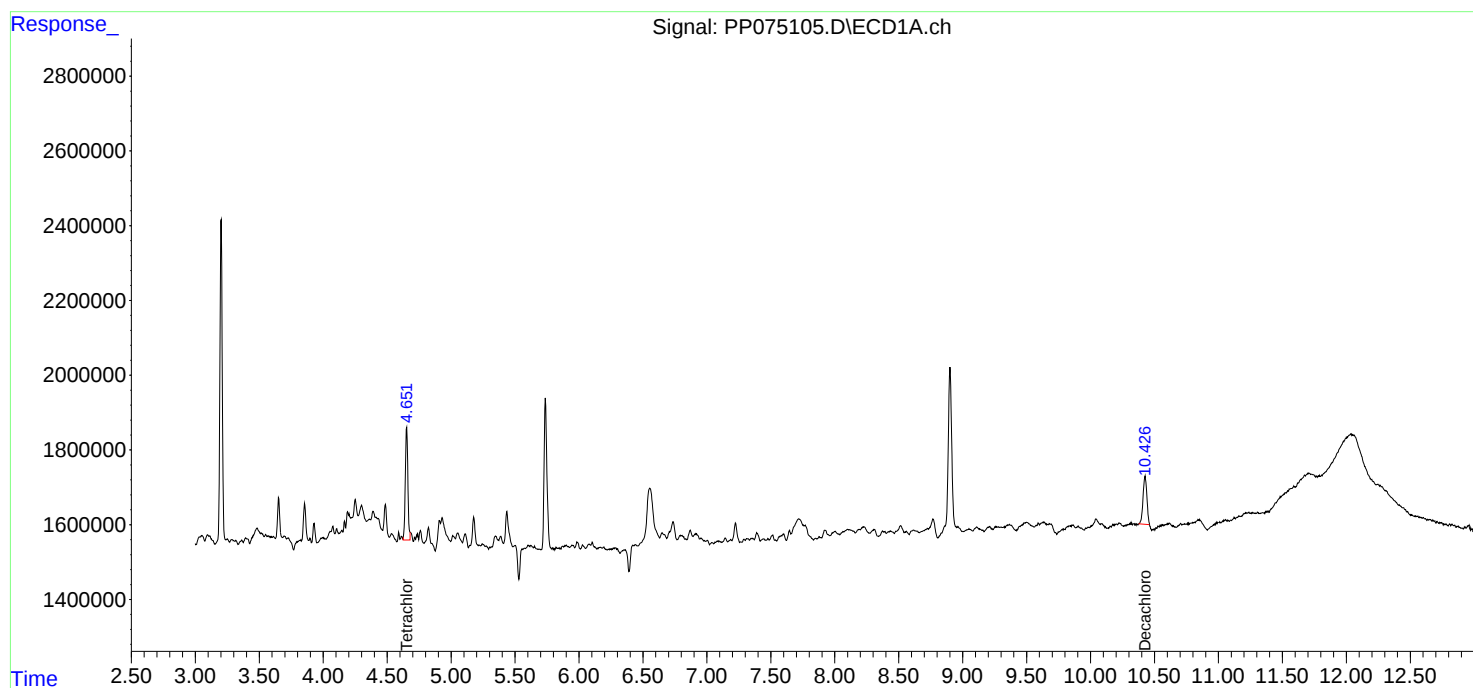

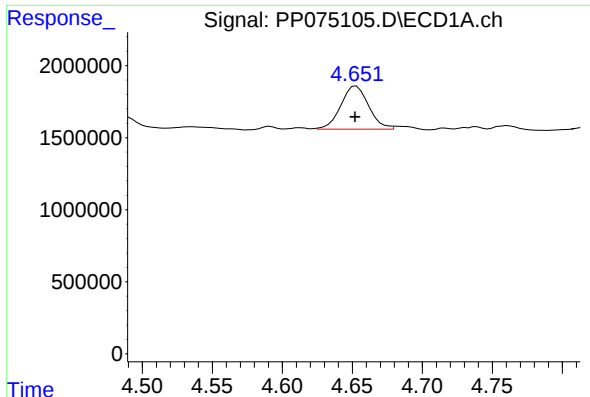


#1 Tetrachloro-m-xylene

R.T.: 4.651 min
Delta R.T.: 0.000 min
Response: 4122002
Conc: 3.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
BEL-25-0023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/15/2025
Supervised By :mohammad ahmed 09/16/2025

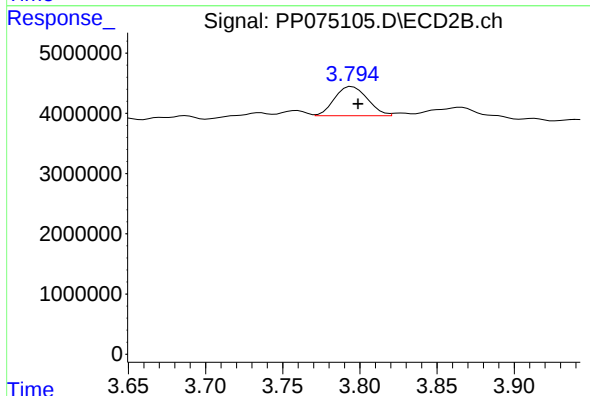


#1 Tetrachloro-m-xylene

R.T.: 3.794 min
Delta R.T.: -0.005 min
Response: 7246589
Conc: 1.50 ng/ml m

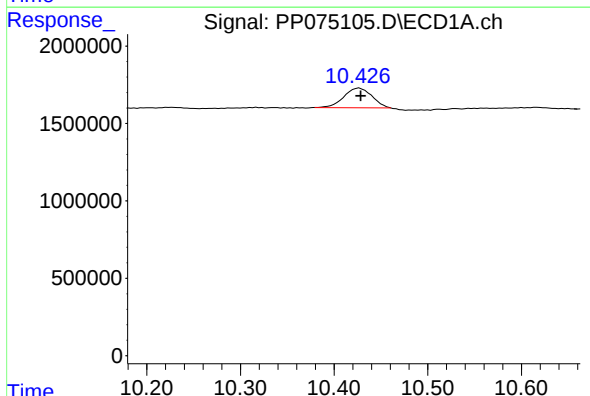

#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.003 min
Response: 2680768
Conc: 2.71 ng/ml m

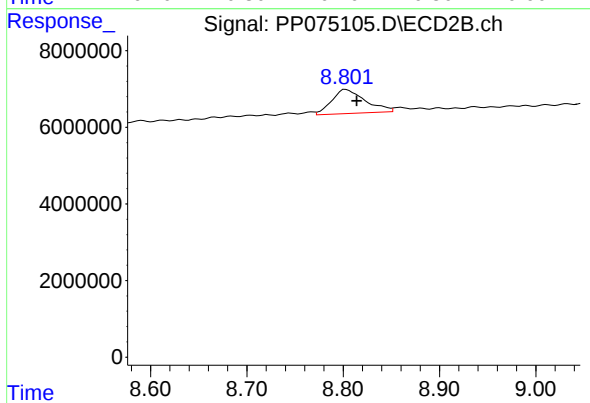

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.011 min
Response: 15156022
Conc: 2.02 ng/ml