

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040219\
 Data File : PP029677.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2019 7:36
 Operator : EI\MA
 Sample : HEXANE
 Misc : hexane
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 07:41:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040219.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 03 07:41:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
16)	T	DCPA	18.057	0.000	129067	0 0.344 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040219\
Data File : PP029677.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2019 7:36
Operator : EI\MA
Sample : HEXANE
Misc : hexane
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 07:41:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040219.M
Quant Title : 8080.M
QLast Update : Wed Apr 03 07:41:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

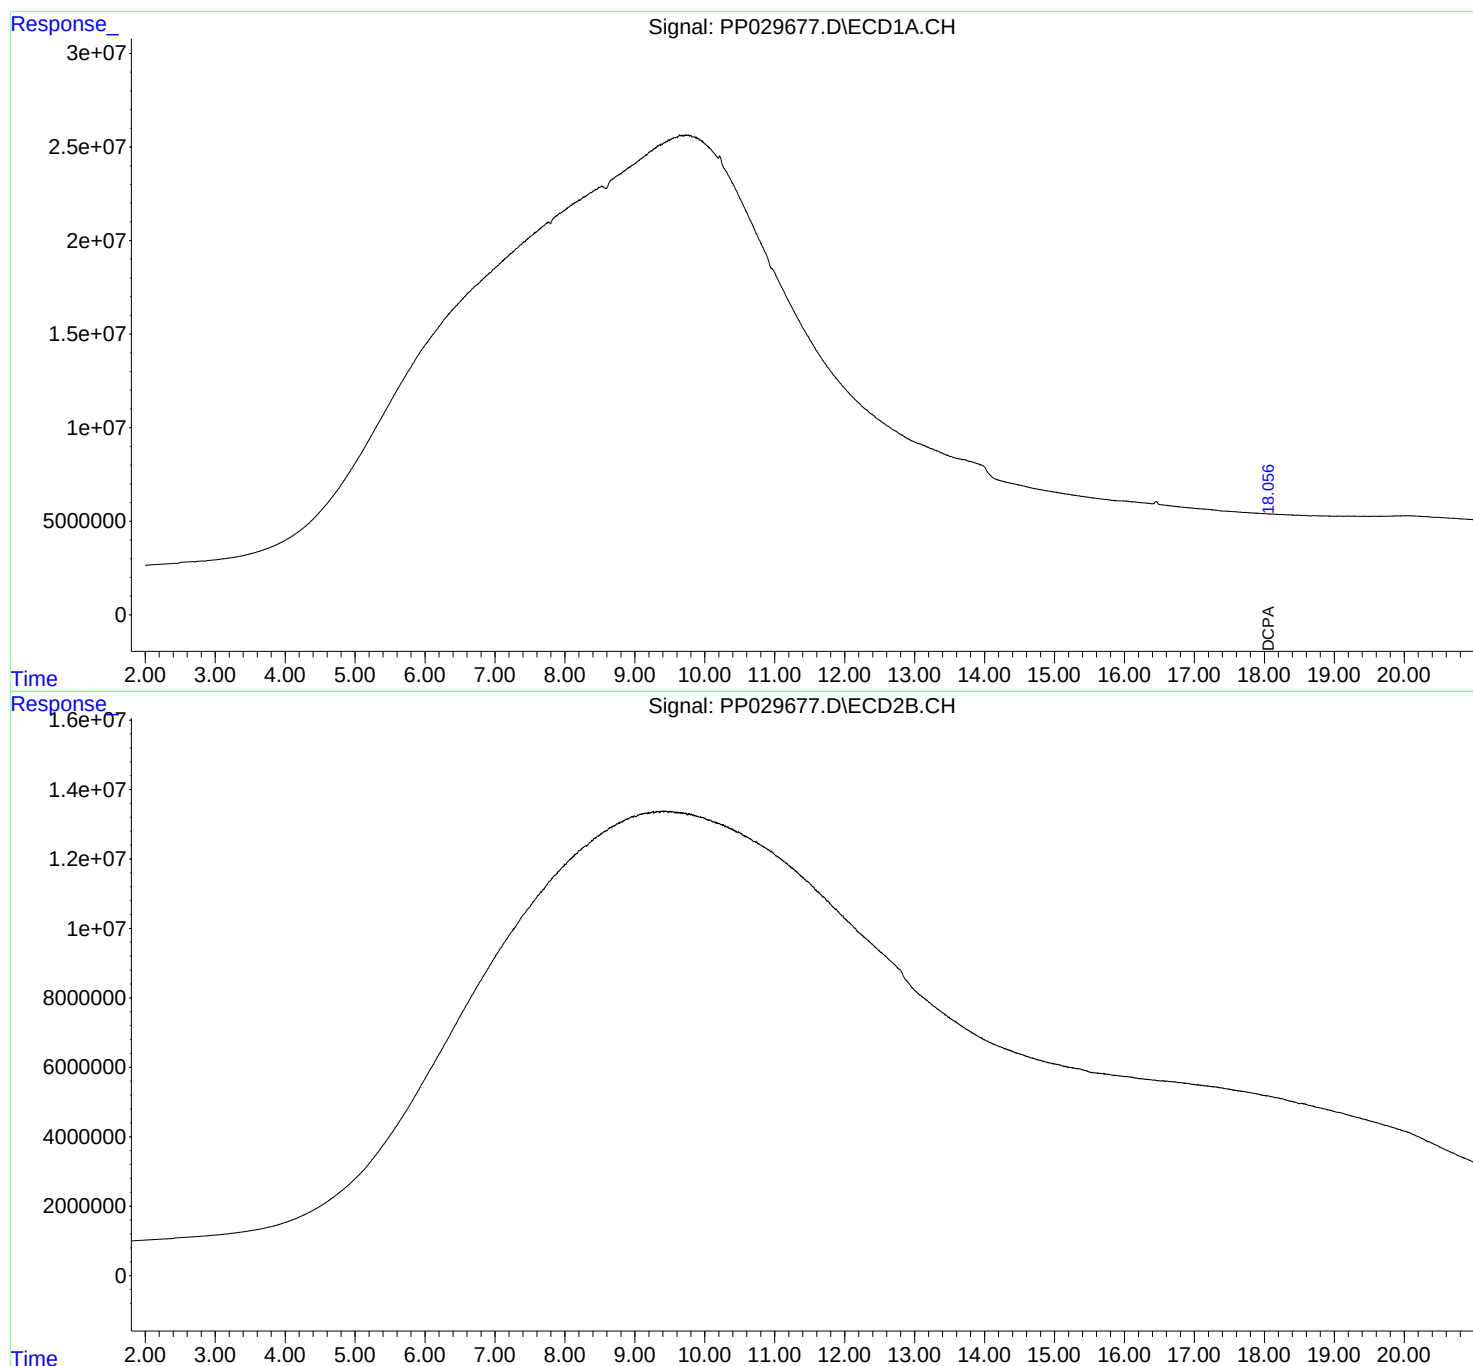


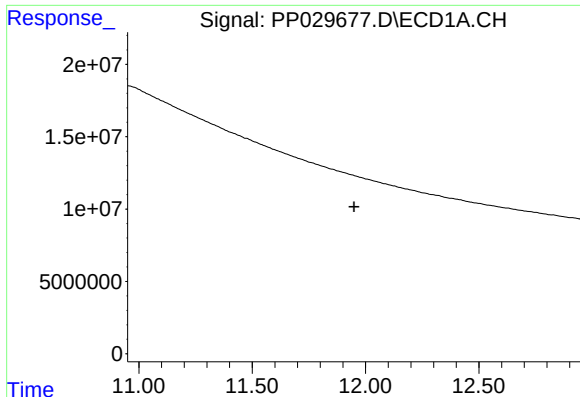

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

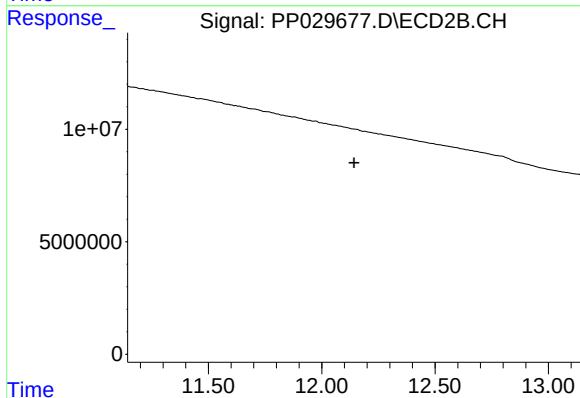


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 12.143 min
Response: 0
Conc: N.D.

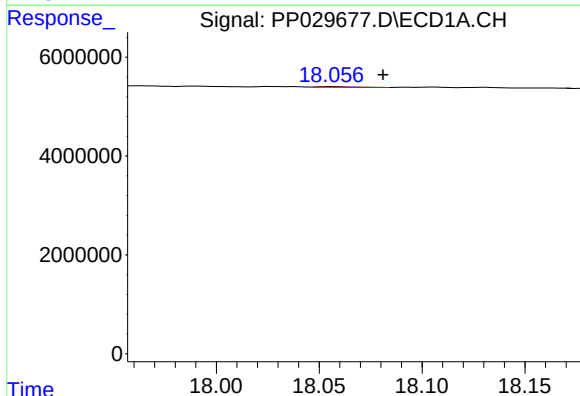

#16 DCPA

R.T.: 18.057 min
Delta R.T.: -0.024 min
Response: 129067
Conc: 0.34 ng/ml

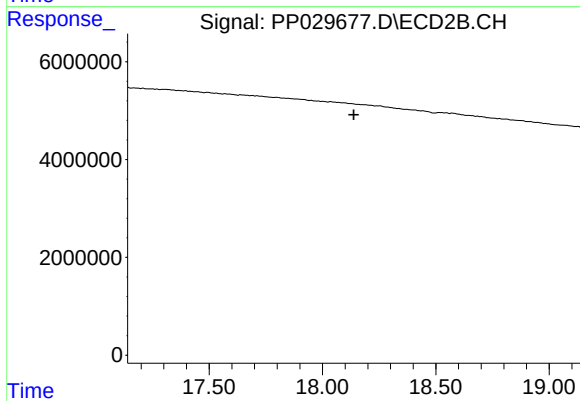

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.138 min
Response: 0
Conc: N.D.