



MCPA

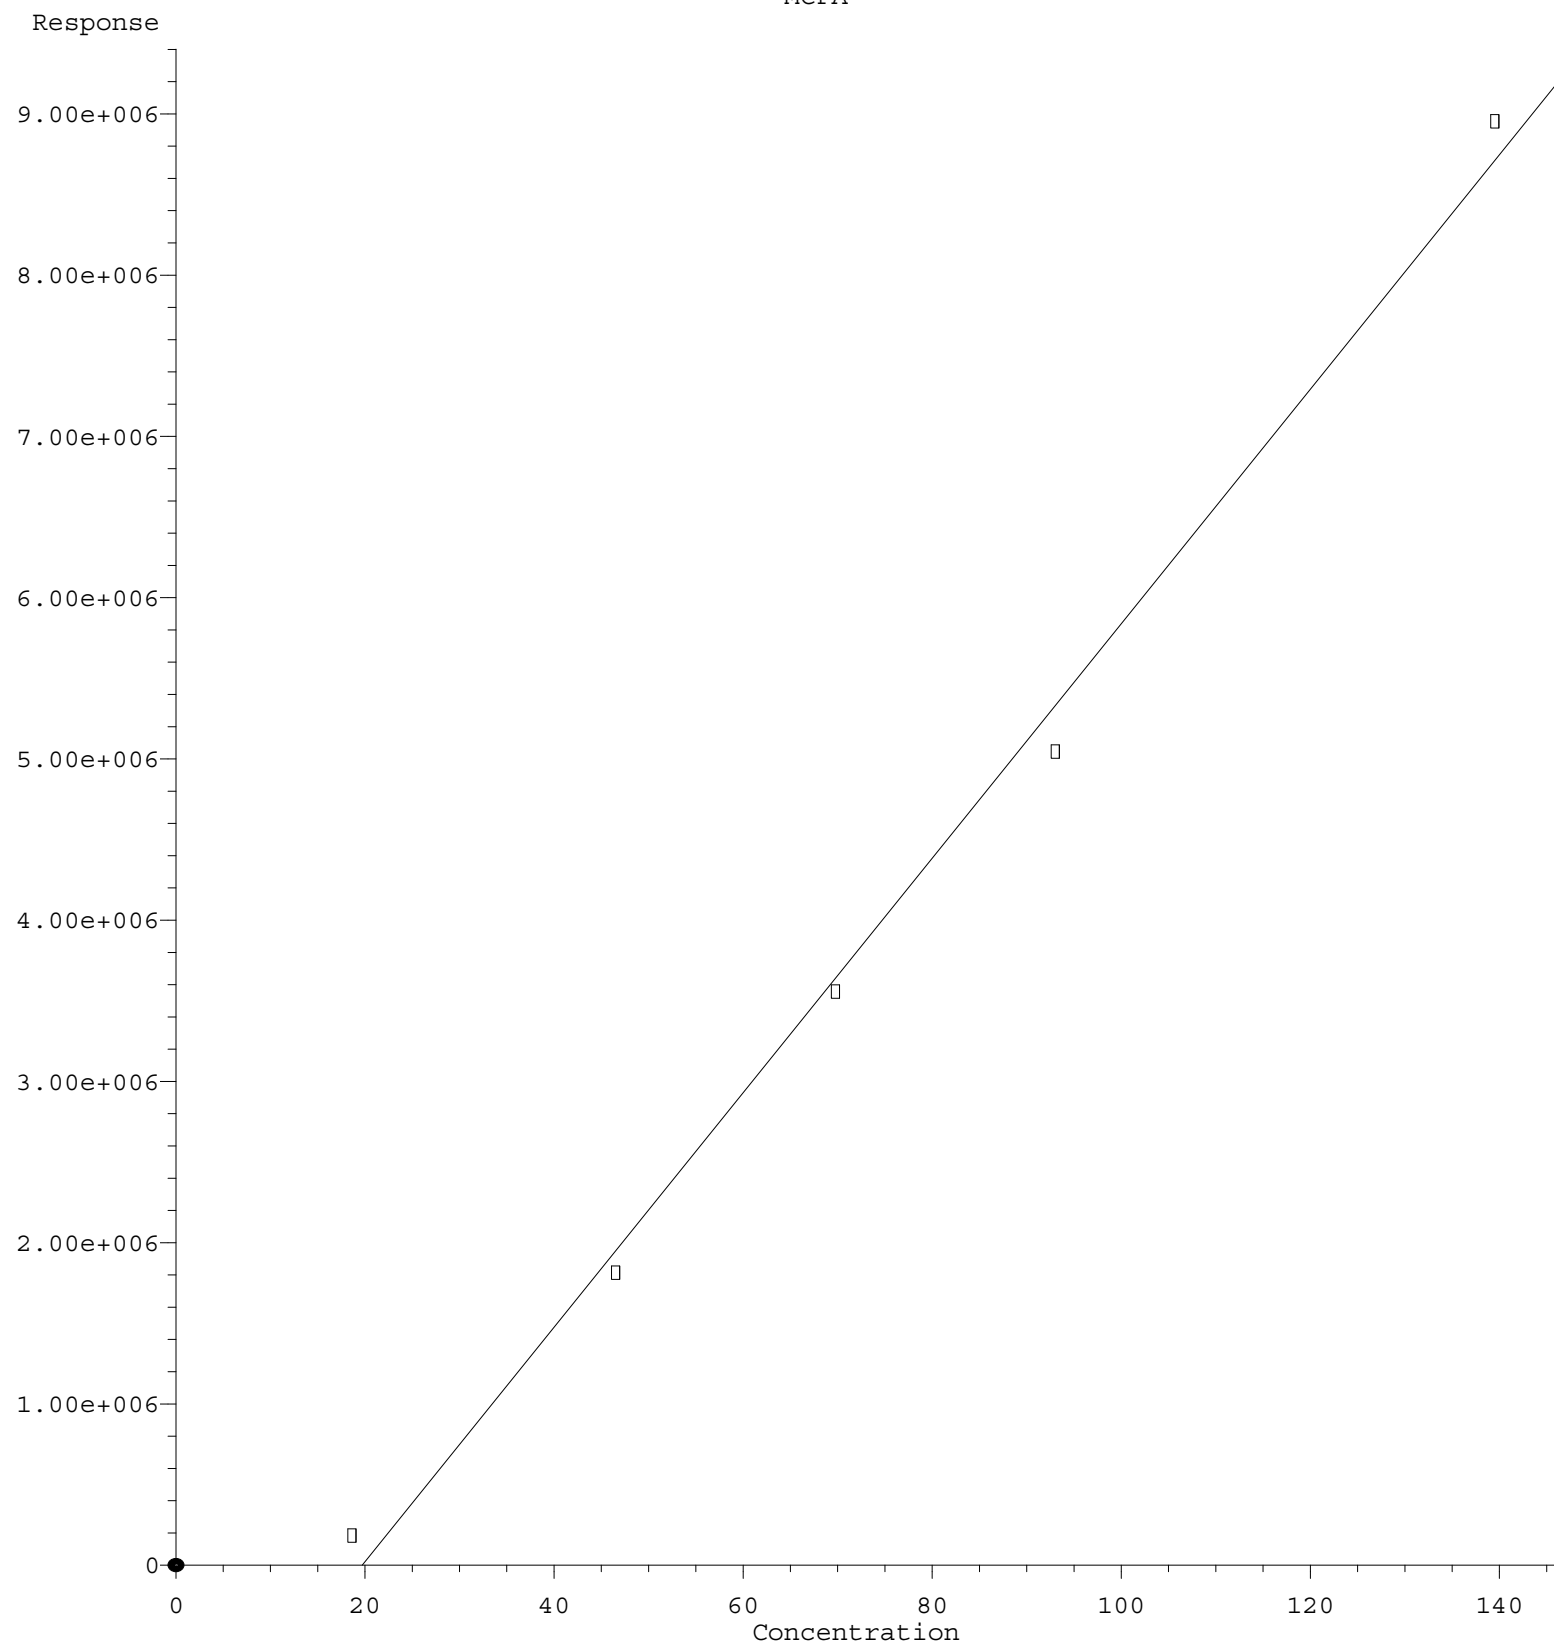


Response = 7.271e+004 * Amt - 1.431e+006
Coef of Det (r^2) = 0.994815 Curve Fit: Linear
Method Name: Z:\pestpcbsrv\HPCHEM1\ECD P\methods\PP040219.M
Calibration Table Last Updated: Wed Apr 03 07:41:20 2019


MCP

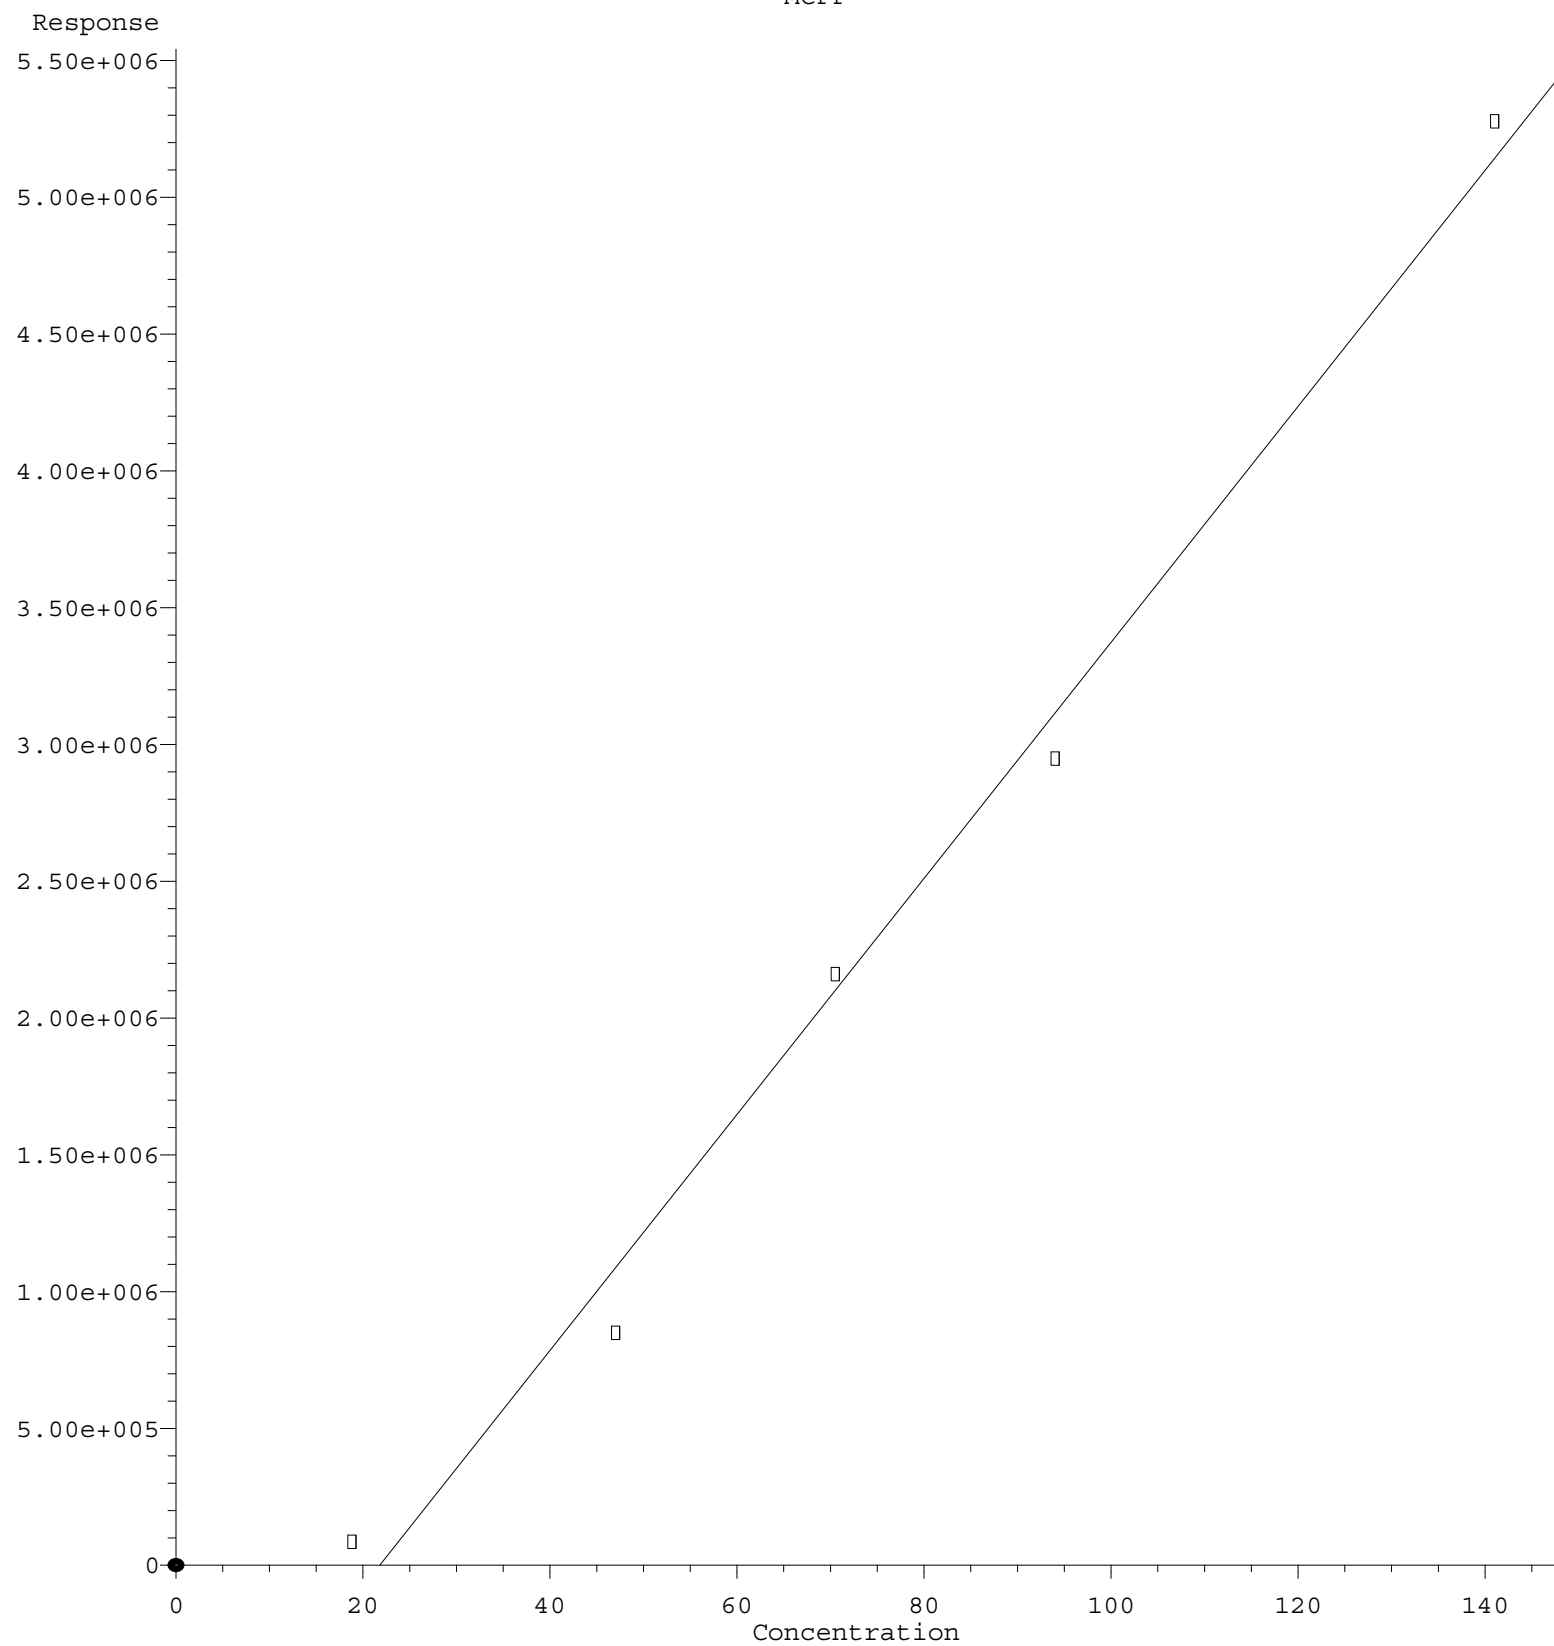

Response = $4.315 \times 10^4 \times \text{Amt} - 9.401 \times 10^5$
Coef of Det (r^2) = 0.990655 Curve Fit: Linear
Method Name: Z:\pestpcbsrv\HPCHEM1\ECD P\methods\PP040219.M
Calibration Table Last Updated: Wed Apr 03 07:41:20 2019

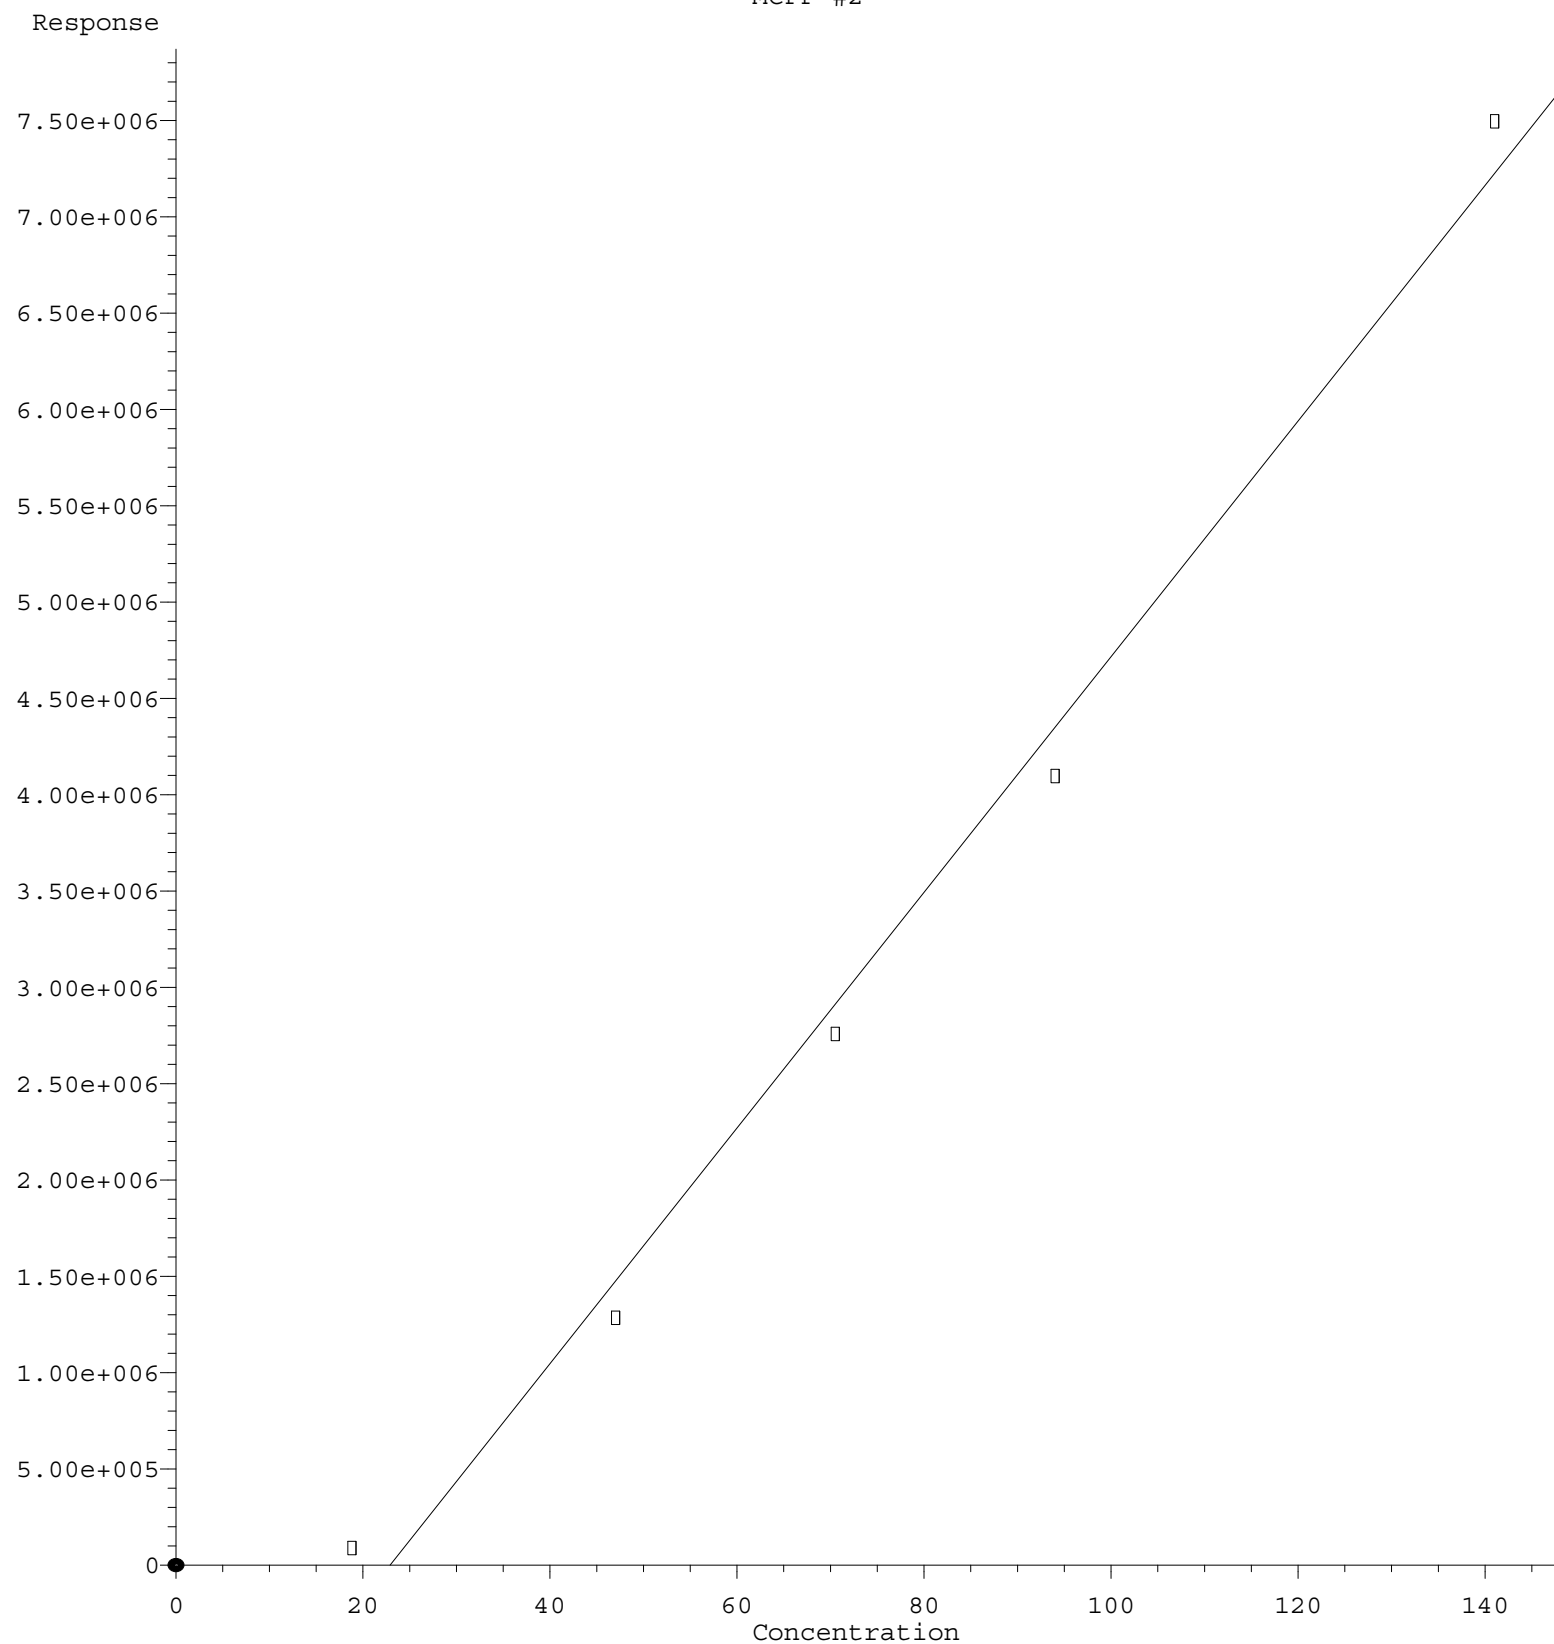

Response = 6.117e+004 * Amt - 1.398e+006
Coef of Det (r^2) = 0.990462 Curve Fit: Linear
Method Name: Z:\pestpcbsrv\HPCHEM1\ECD P\methods\PP040219.M
Calibration Table Last Updated: Wed Apr 03 07:41:20 2019

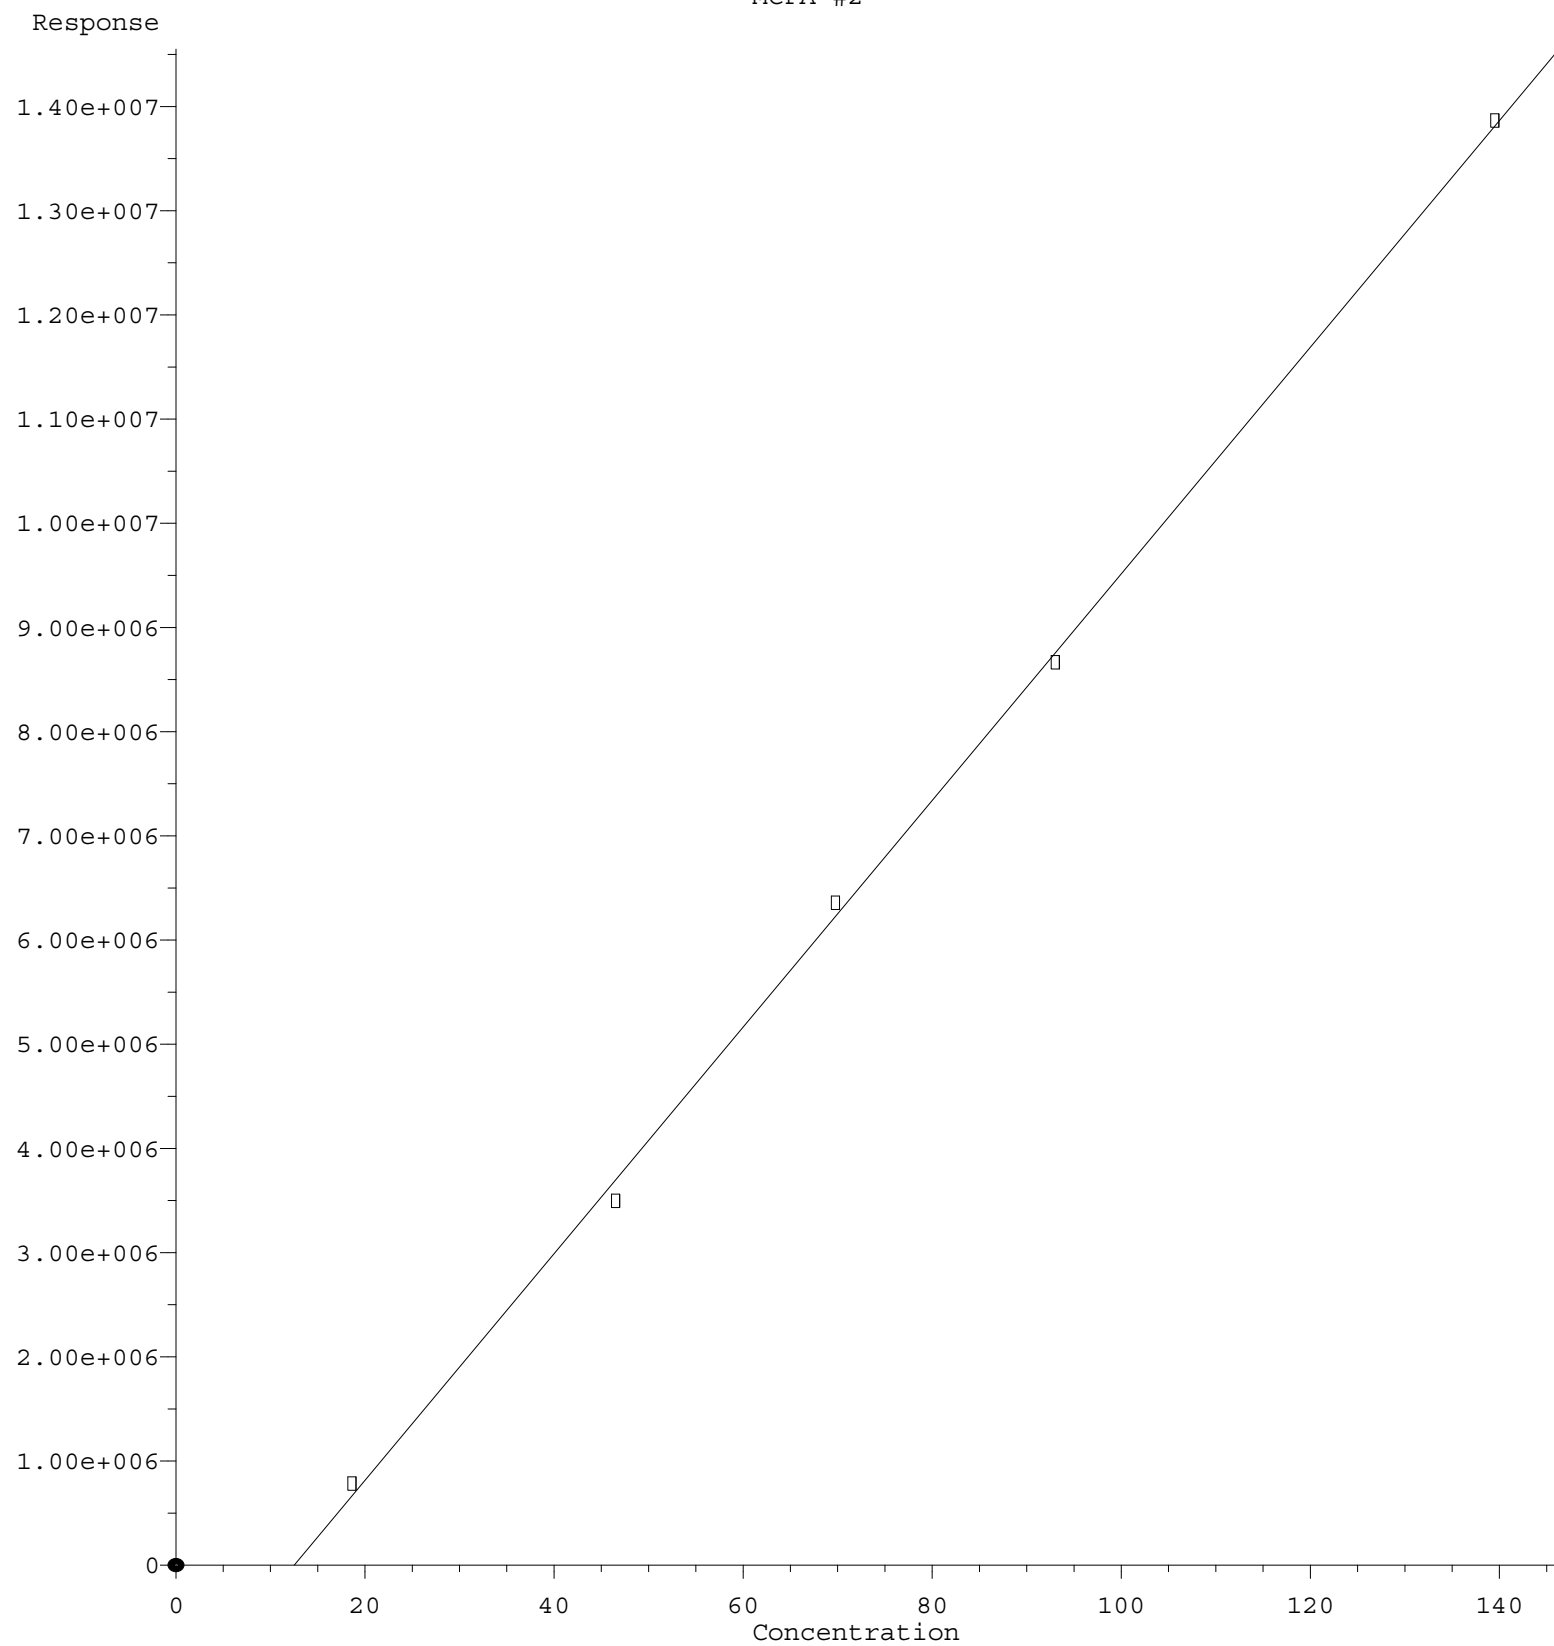

Response = 1.088e+005 * Amt - 1.358e+006
Coef of Det (r^2) = 0.999172 Curve Fit: Linear
Method Name: Z:\pestpcbsrv\HPCHEM1\ECD P\methods\PP040219.M
Calibration Table Last Updated: Wed Apr 03 07:41:20 2019