

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040419\
 Data File : PP029703.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2019 19:23
 Operator : EI\MA
 Sample : K2199-02
 Misc : hexane
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OR-02-040219-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:15:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040219.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 03 07:41:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.950	12.146	5934591	6400325	183.249	156.093
Target Compounds							
2) T	3,5-DICHL...	10.317	0.000	239382	0	3.318	N.D. #
5) T	DICAMBA	12.249	12.412	343463	1346334	2.062	9.527 #
6) T	MCP	12.552	0.000	41968	0	22.759	N.D. #
8) T	DICHLORPROP	13.398	13.578	2280974	1829791	50.690	46.755
13) T	2,4-DB	16.236	0.000	7821693	0	306.968	N.D. #
14) T	DINOSEB	17.731	16.840	18766807	25670942	95.163	169.969 #
15) T	Picloram	17.502	0.000	10991057	0	34.185	N.D. #
16) T	DCPA	18.050	0.000	10602277	0	28.264	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040419\
Data File : PP029703.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2019 19:23
Operator : EI\MA
Sample : K2199-02
Misc : hexane
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
OR-02-040219-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:15:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040219.M
Quant Title : 8080.M
QLast Update : Wed Apr 03 07:41:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

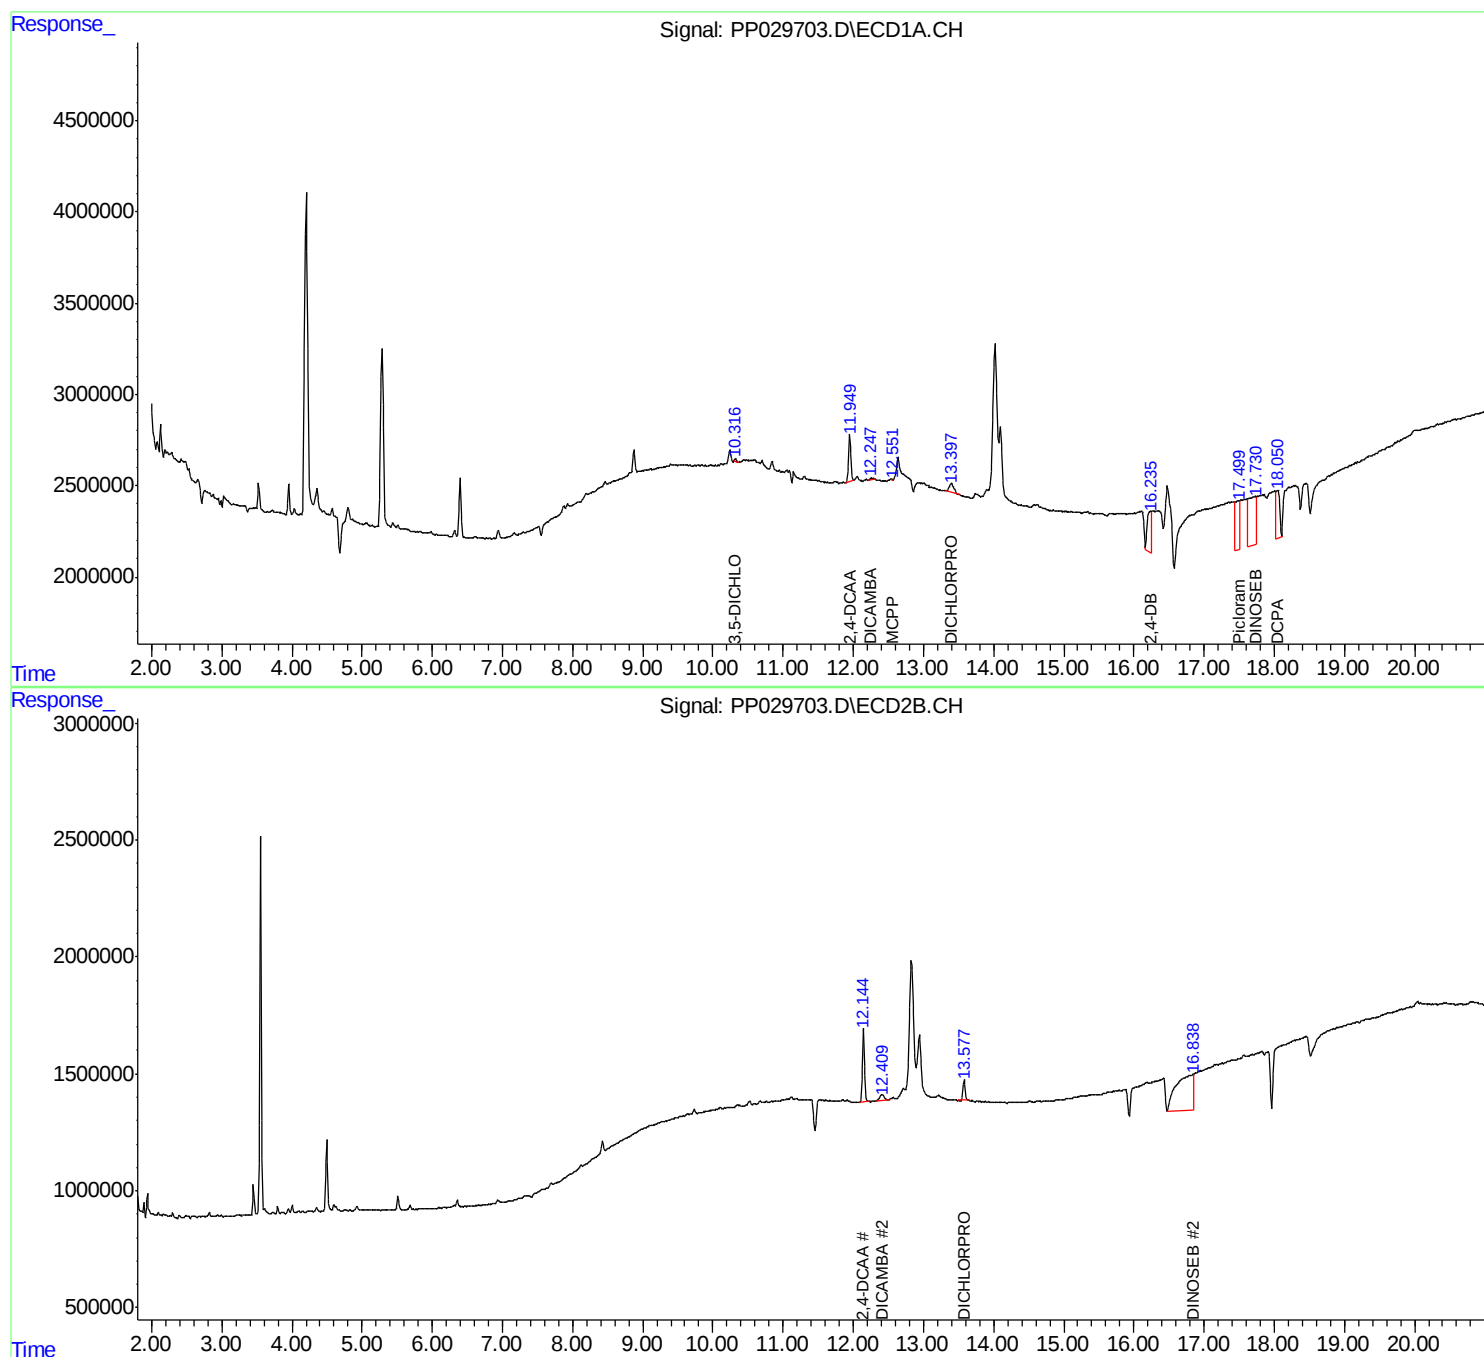


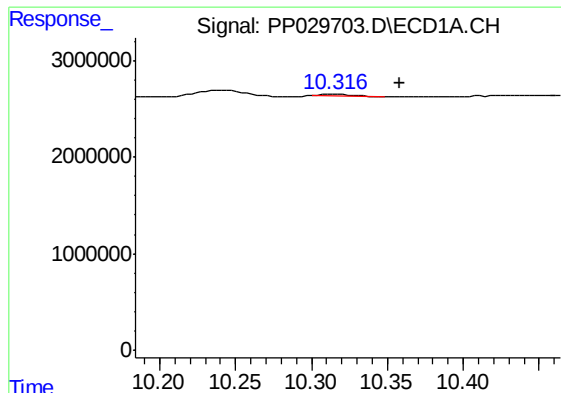

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 10.317 min
Delta R.T.: -0.041 min
Response: 239382
Conc: 3.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
OR-02-040219-A

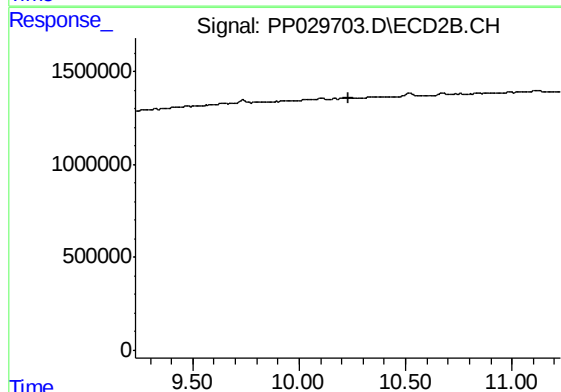


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.230 min
Response: 0
Conc: N.D.

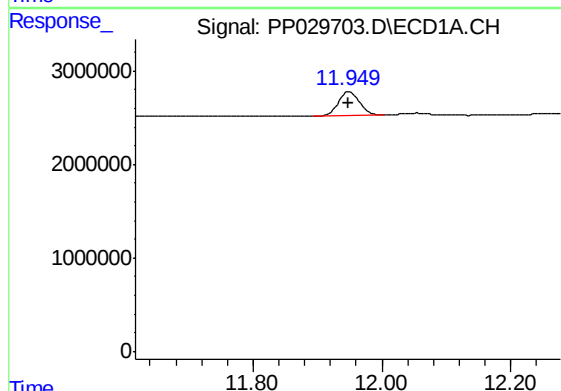


#4 2,4-DCAA

R.T.: 11.950 min
Delta R.T.: 0.000 min
Response: 5934591
Conc: 183.25 ng/ml

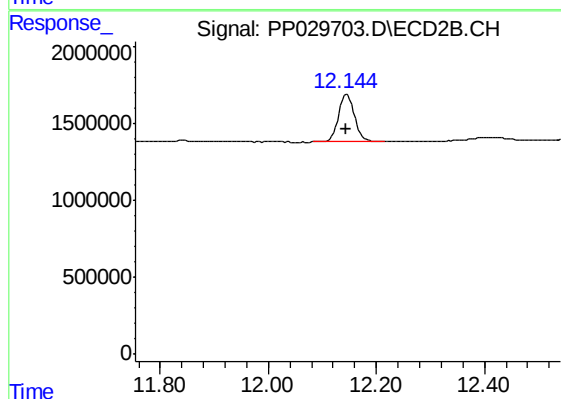

#4 2,4-DCAA


R.T.: 12.146 min
Delta R.T.: 0.003 min
Response: 6400325
Conc: 156.09 ng/ml

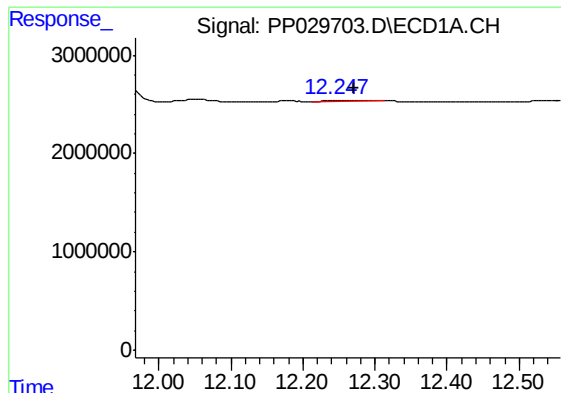

#5 DICAMBA


R.T.: 12.249 min
Delta R.T.: -0.021 min
Response: 343463
Conc: 2.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
OR-02-040219-A

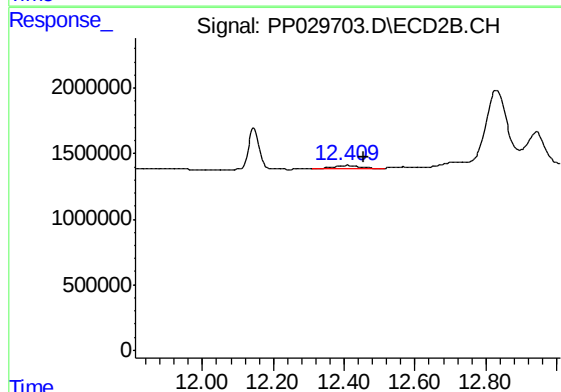


#5 DICAMBA

R.T.: 12.412 min
Delta R.T.: -0.043 min
Response: 1346334
Conc: 9.53 ng/ml

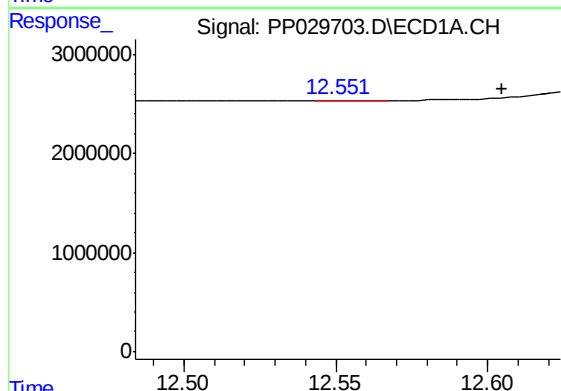


#6 MCPP

R.T.: 12.552 min
Delta R.T.: -0.053 min
Response: 41968
Conc: 22.76 ug/ml

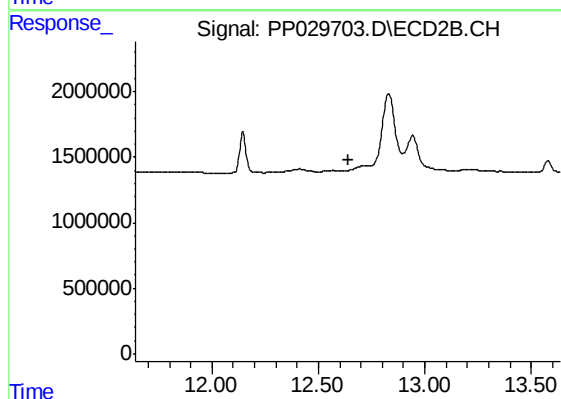

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 12.639 min
Response: 0
Conc: N.D.

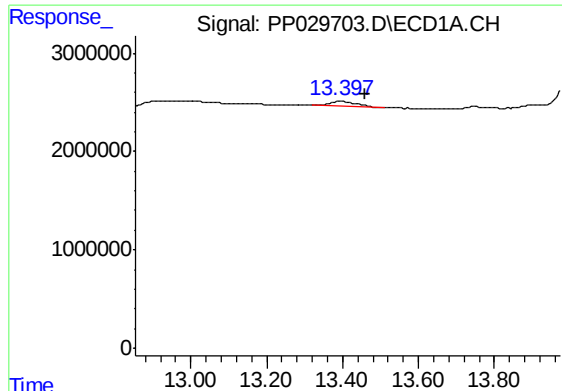

#8 DICHLORPROP


R.T.: 13.398 min
Delta R.T.: -0.063 min
Response: 2280974
Conc: 50.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
OR-02-040219-A

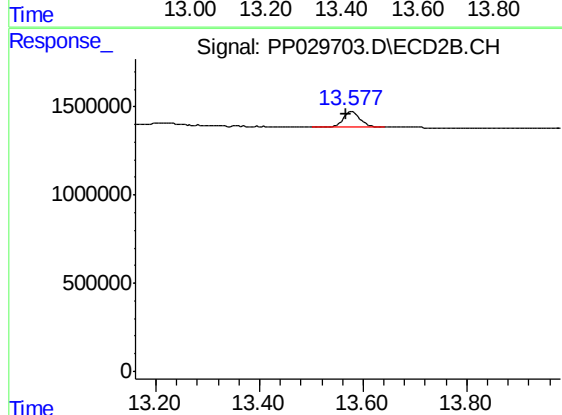


#8 DICHLORPROP

R.T.: 13.578 min
Delta R.T.: 0.012 min
Response: 1829791
Conc: 46.76 ng/ml

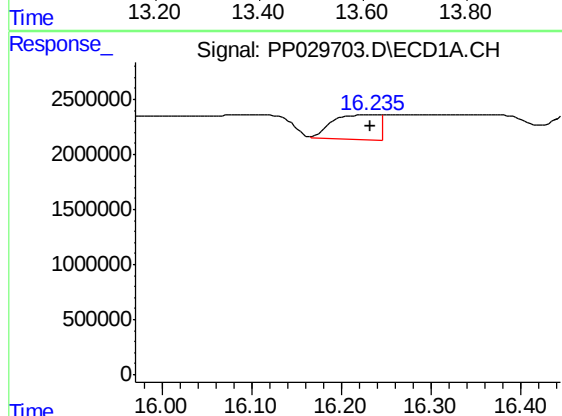


#13 2,4-DB

R.T.: 16.236 min
Delta R.T.: 0.004 min
Response: 7821693
Conc: 306.97 ng/ml

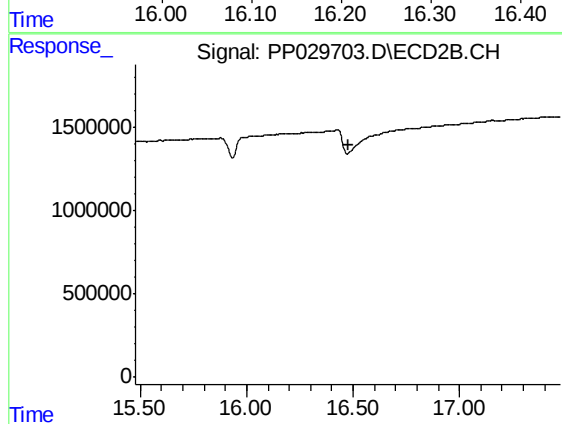

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 16.476 min
Response: 0
Conc: N.D.

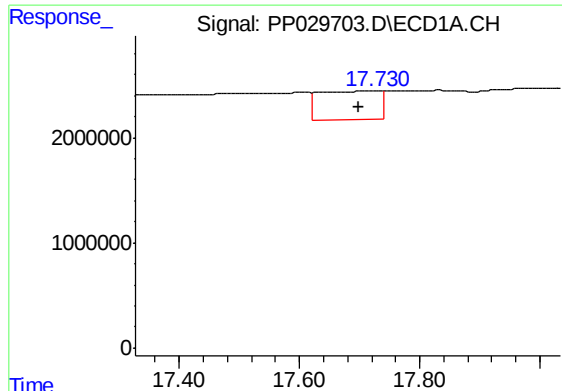

#14 DINOSEB


R.T.: 17.731 min
Delta R.T.: 0.032 min
Response: 18766807
Conc: 95.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
OR-02-040219-A

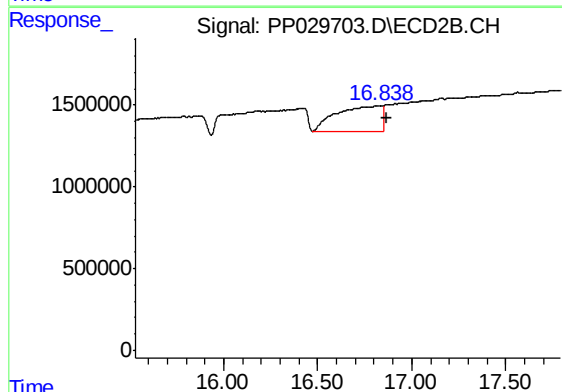


#14 DINOSEB

R.T.: 16.840 min
Delta R.T.: -0.027 min
Response: 25670942
Conc: 169.97 ng/ml

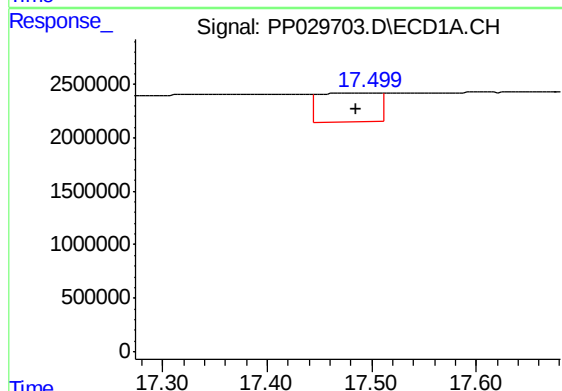


#15 Picloram

R.T.: 17.502 min
Delta R.T.: 0.017 min
Response: 10991057
Conc: 34.19 ng/ml

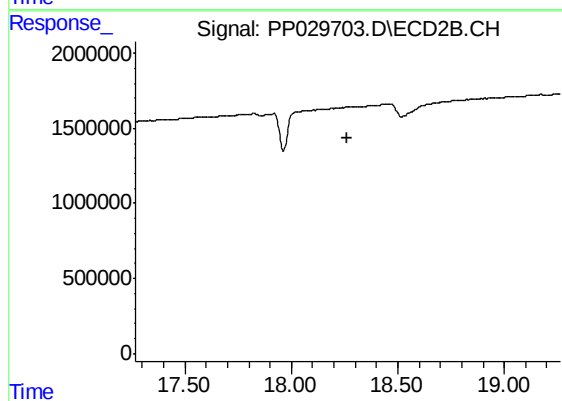

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 18.265 min
Response: 0
Conc: N.D.

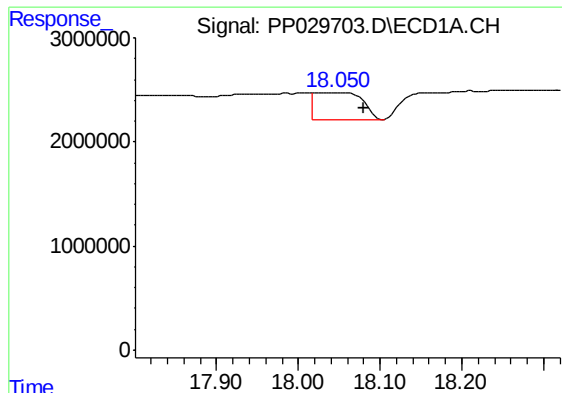

#16 DCPA

R.T.: 18.050 min
Delta R.T.: -0.031 min
Response: 10602277
Conc: 28.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
OR-02-040219-A

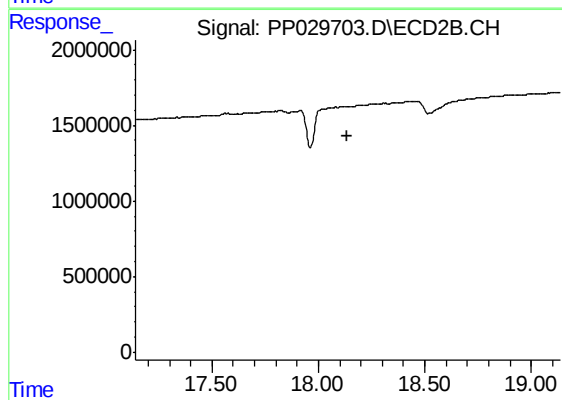

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.138 min
Response: 0
Conc: N.D.