

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040419\
 Data File : PP029719.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2019 2:11
 Operator : EI\MA
 Sample : I.BLK
 Misc : hexane
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:33:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040219.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 03 07:41:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.946	12.143	18380028	21291891	567.541	519.272
Target Compounds							
5) T	DICAMBA	0.000	12.424	0	1197836	N.D.	8.476 #
8) T	DICHLORPROP	13.399	0.000	1906572	0	42.370	N.D. #
11) T	2,4,5-TP ...	15.093	15.244	293020	123846	0.996	0.587 #
13) T	2,4-DB	16.244	0.000	275590	0	10.816	N.D. #
14) T	DINOSEB	17.694	16.909	86267	246376	0.437	1.631 #
15) T	Picloram	17.491	18.281	726302	244182	2.259	1.080 #
16) T	DCPA	18.078	18.150	1013473	206112	2.702	0.755 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040419\
Data File : PP029719.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2019 2:11
Operator : EI\MA
Sample : I.BLK
Misc : hexane
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:33:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040219.M
Quant Title : 8080.M
QLast Update : Wed Apr 03 07:41:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

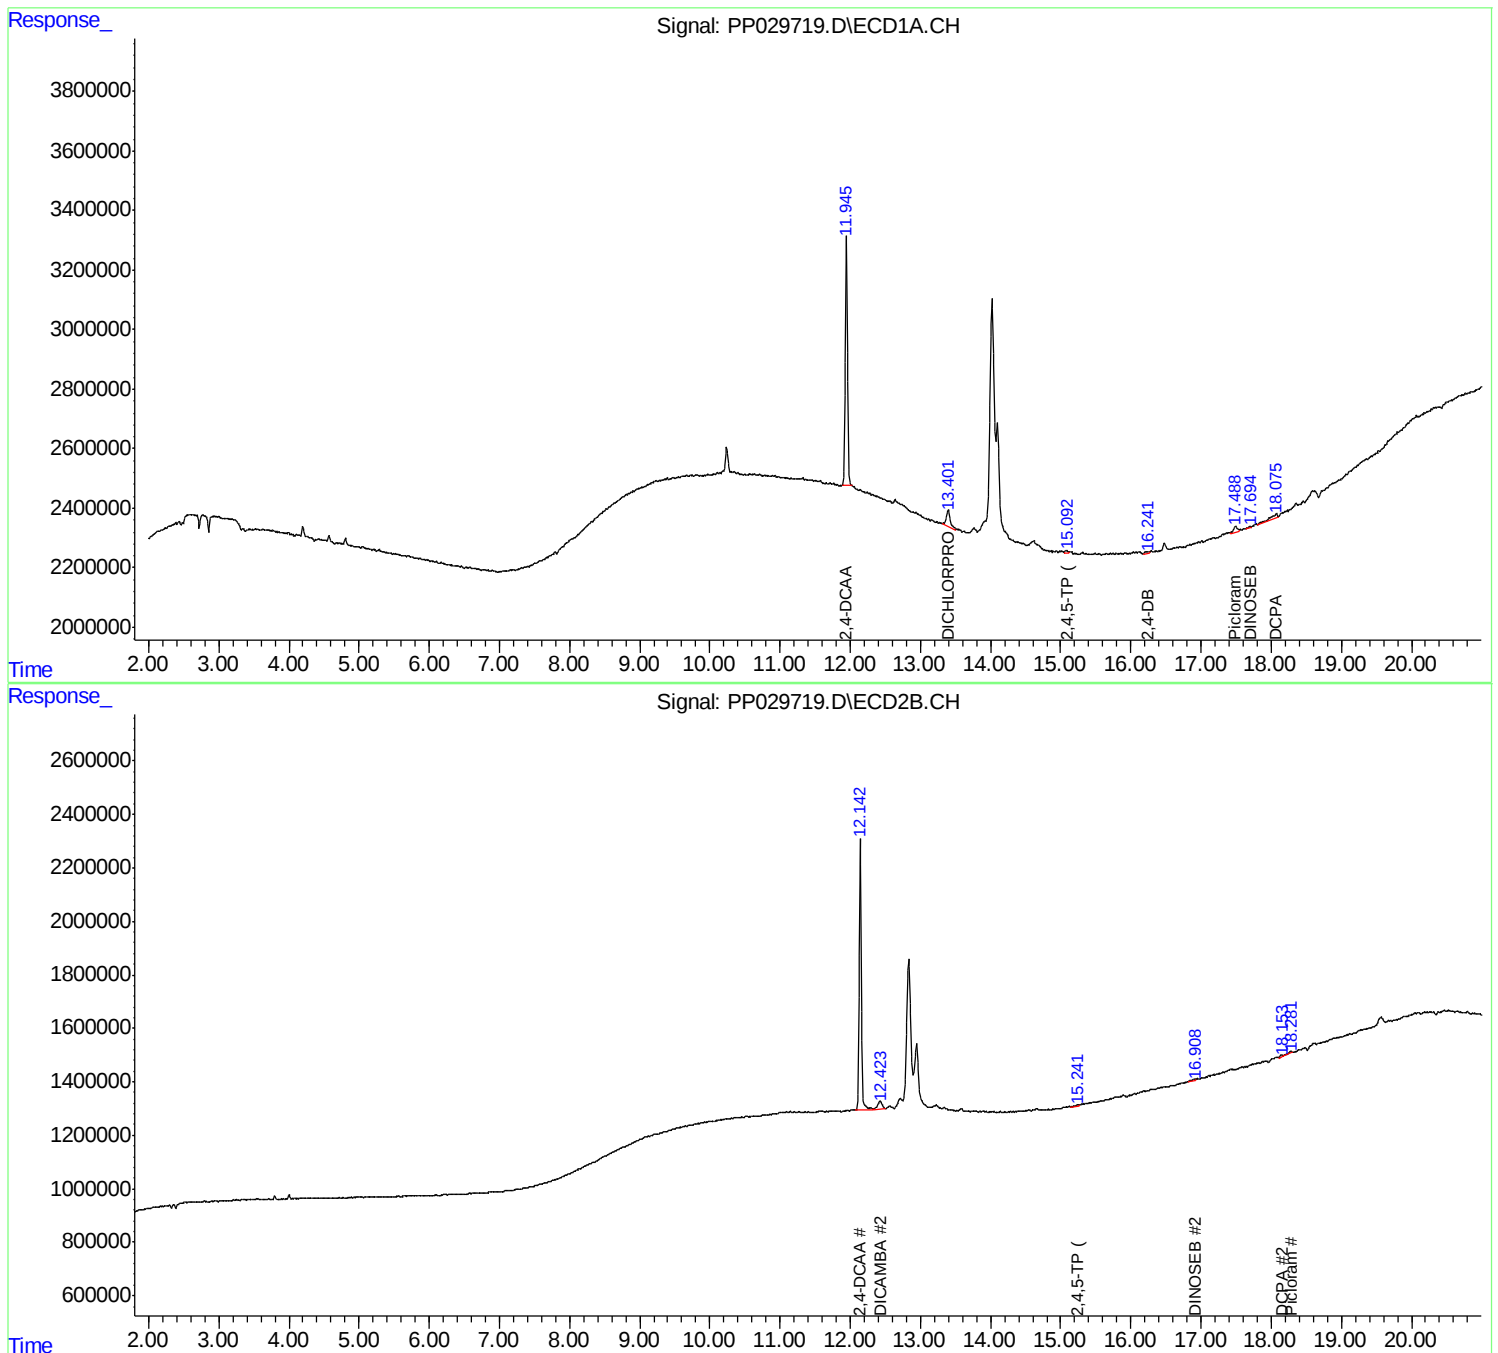


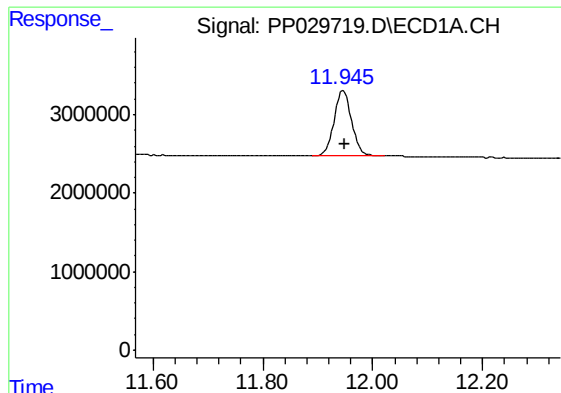

#4 2,4-DCAA


R.T.: 11.946 min
Delta R.T.: -0.003 min
Response: 18380028
Conc: 567.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

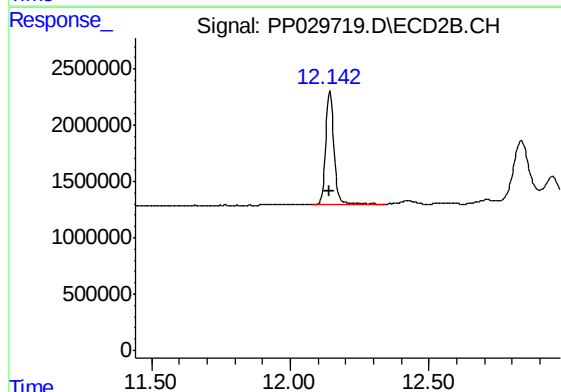


#4 2,4-DCAA

R.T.: 12.143 min
Delta R.T.: 0.000 min
Response: 21291891
Conc: 519.27 ng/ml

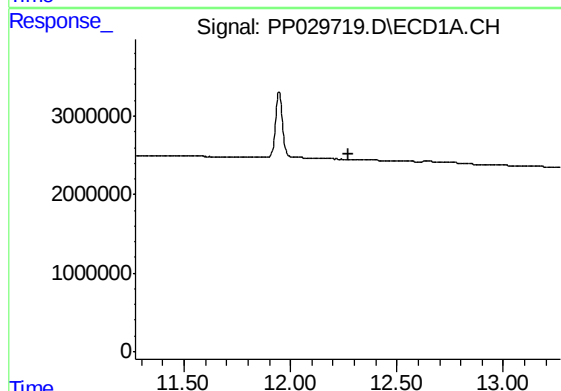


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.270 min
Response: 0
Conc: N.D.

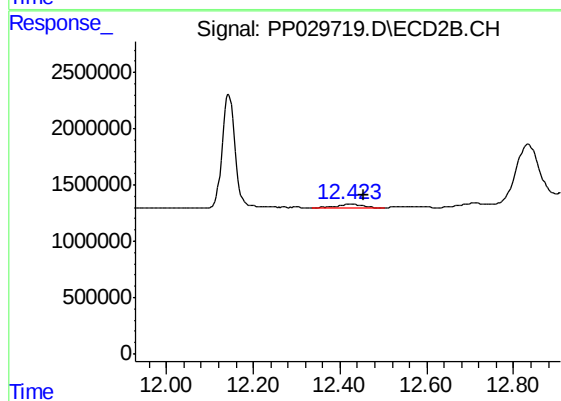

#5 DICAMBA


R.T.: 12.424 min
Delta R.T.: -0.031 min
Response: 1197836
Conc: 8.48 ng/ml

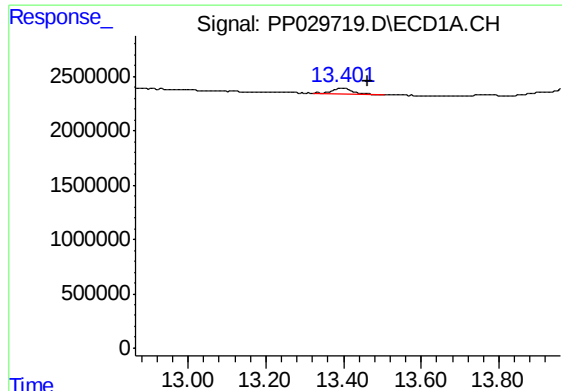

#8 DICHLORPROP


R.T.: 13.399 min
Delta R.T.: -0.062 min
Response: 1906572
Conc: 42.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

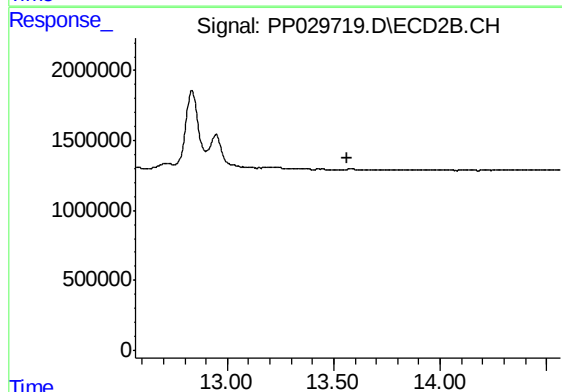


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.566 min
Response: 0
Conc: N.D.

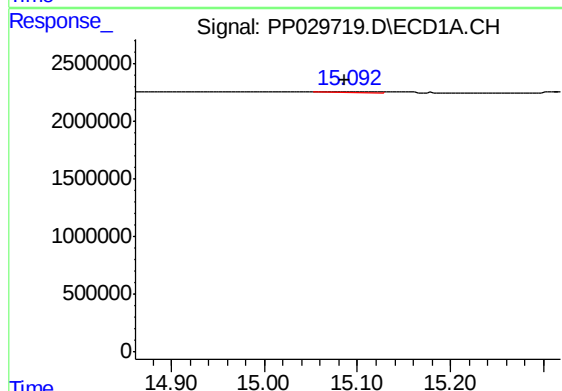


#11 2,4,5-TP (SILVEX)

R.T.: 15.093 min
Delta R.T.: 0.007 min
Response: 293020
Conc: 1.00 ng/ml

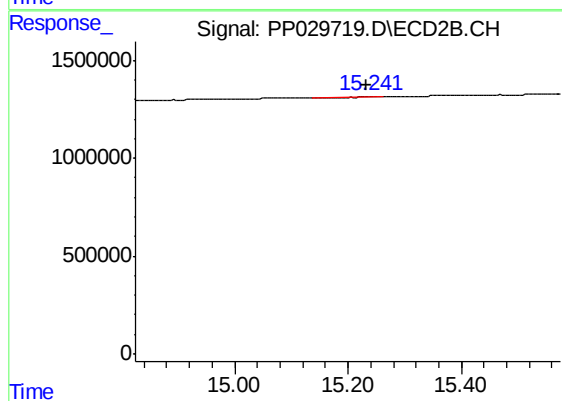

#11 2,4,5-TP (SILVEX)


R.T.: 15.244 min
Delta R.T.: 0.012 min
Response: 123846
Conc: 0.59 ng/ml

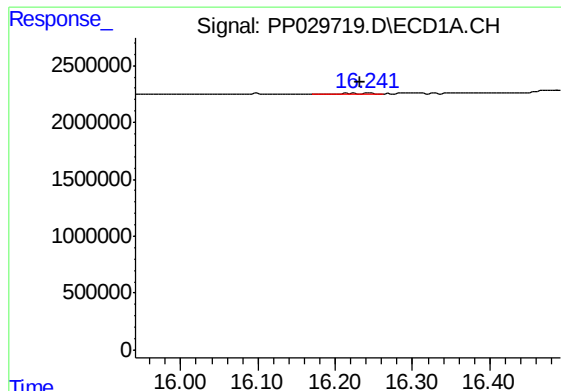

#13 2,4-DB


R.T.: 16.244 min
Delta R.T.: 0.012 min
Response: 275590
Conc: 10.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

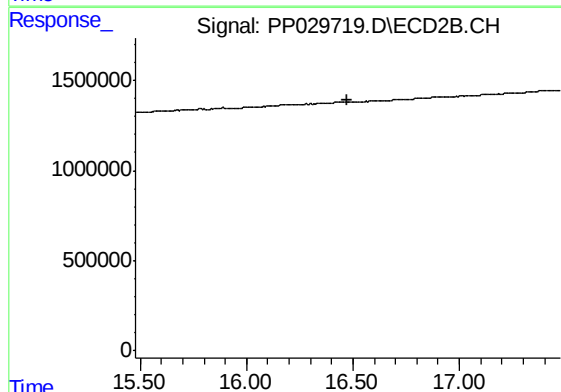


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.476 min
Response: 0
Conc: N.D.

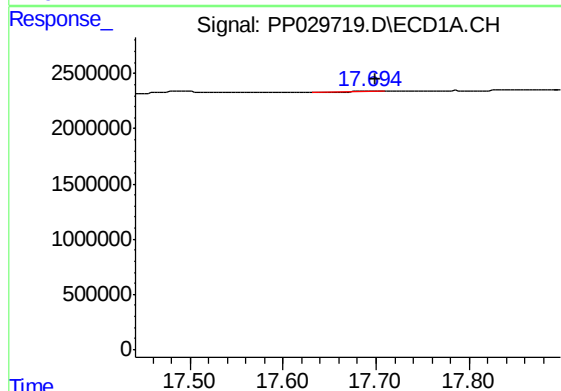


#14 DINOSEB

R.T.: 17.694 min
Delta R.T.: -0.005 min
Response: 86267
Conc: 0.44 ng/ml

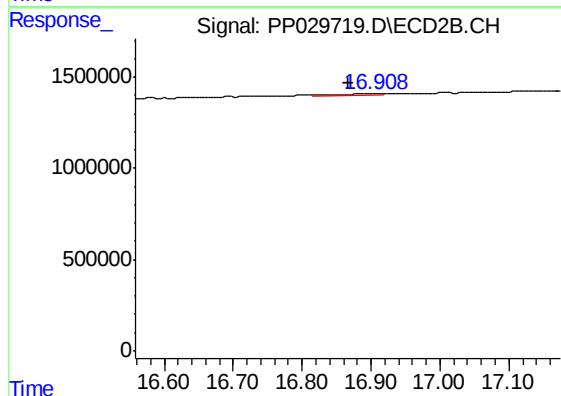

#14 DINOSEB


R.T.: 16.909 min
Delta R.T.: 0.042 min
Response: 246376
Conc: 1.63 ng/ml

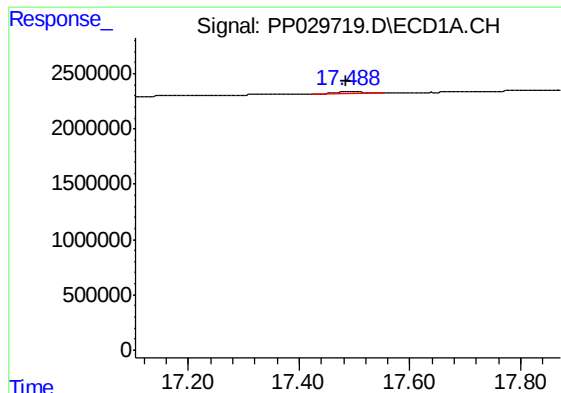

#15 Picloram


R.T.: 17.491 min
Delta R.T.: 0.006 min
Response: 726302
Conc: 2.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

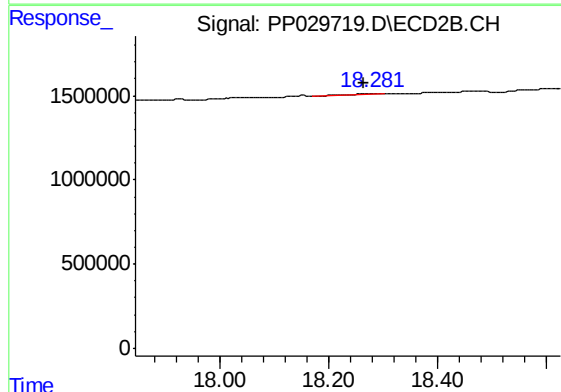


#15 Picloram

R.T.: 18.281 min
Delta R.T.: 0.016 min
Response: 244182
Conc: 1.08 ng/ml

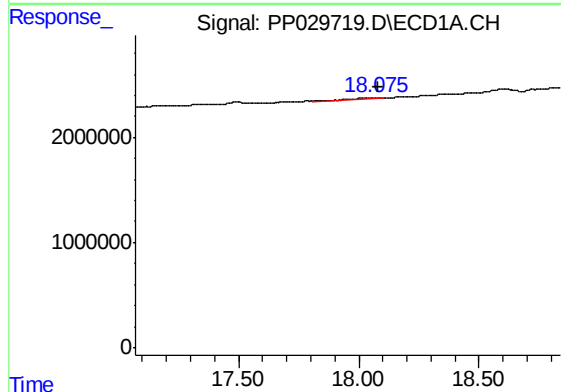

#16 DCPA

R.T.: 18.078 min
Delta R.T.: -0.003 min
Response: 1013473
Conc: 2.70 ng/ml

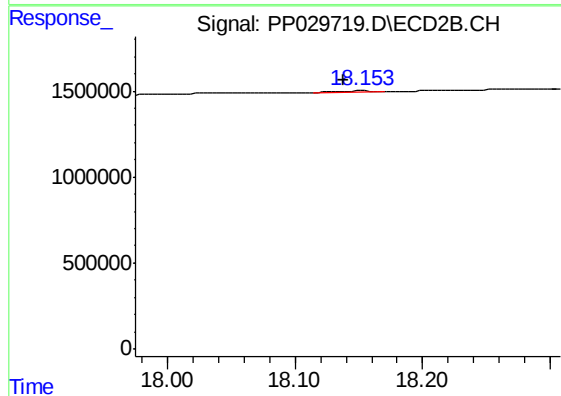

#16 DCPA

R.T.: 18.150 min
Delta R.T.: 0.012 min
Response: 206112
Conc: 0.76 ng/ml