

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040519\
 Data File : PP029742.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2019 16:54
 Operator : EI\MA
 Sample : K2199-02
 Misc : hexane
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 17:52:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 05 15:13:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.170	12.355	36659858	42682136	1104.597	926.380
Target Compounds							
6) T	MCP	0.000	12.791	0	11074423	N.D.	163.897 #
8) T	DICHLORPROP	0.000	13.811	0	3047530	N.D.	69.232 #
9) T	2,4-D	14.076	0.000	7913109	0	183.059	N.D. #
11) T	2,4,5-TP ...	15.258	0.000	14570749	0	54.516	N.D. #
12) T	2,4,5-T	0.000	16.116	0	16746509	N.D.	96.468 #
13) T	2,4-DB	16.517	0.000	31145427	0	1310.305	N.D. #
14) T	DINOSEB	17.963	17.115	4573448	3207363	29.275	23.852
15) T	Picloram	17.749	18.521	7828662	361362	29.325	1.739 #
16) T	DCPA	18.294	0.000	10145130	0	30.940	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040519\
Data File : PP029742.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2019 16:54
Operator : EI\MA
Sample : K2199-02
Misc : hexane
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 17:52:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040519.M
Quant Title : 8080.M
QLast Update : Fri Apr 05 15:13:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

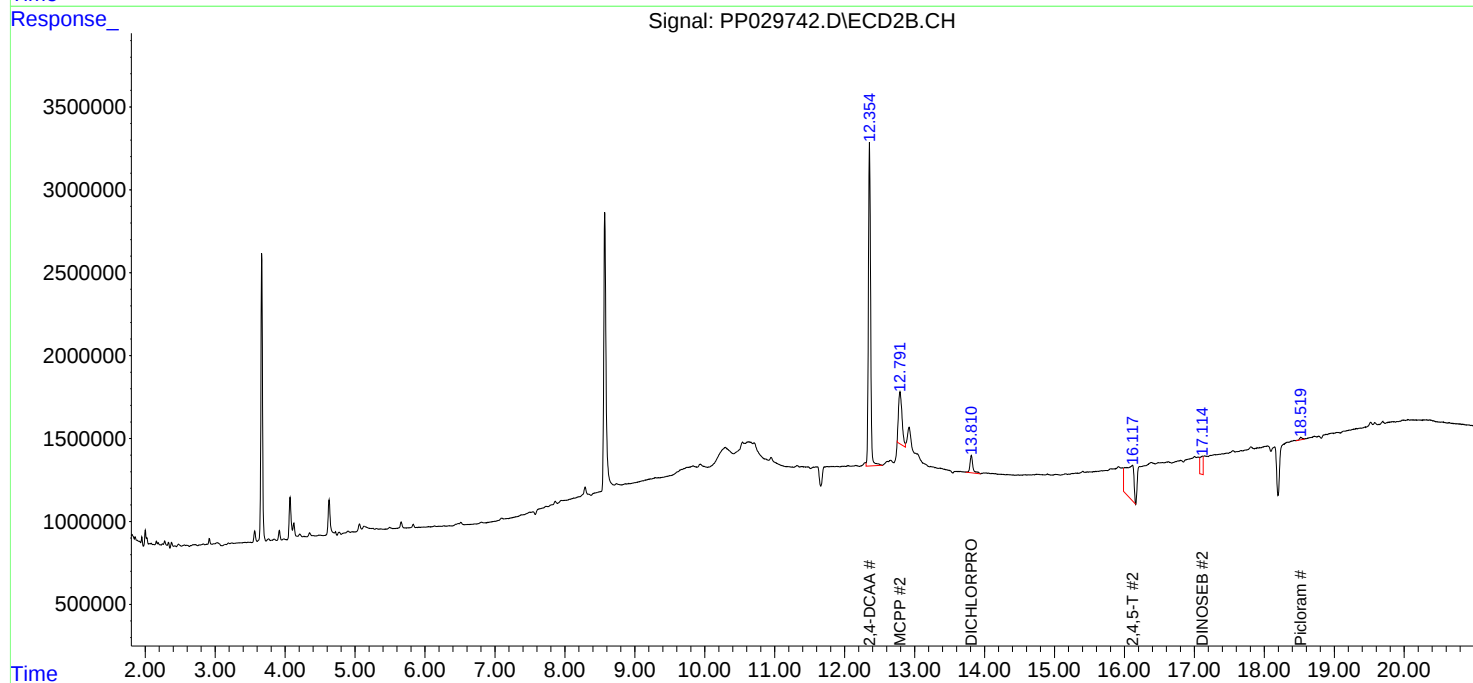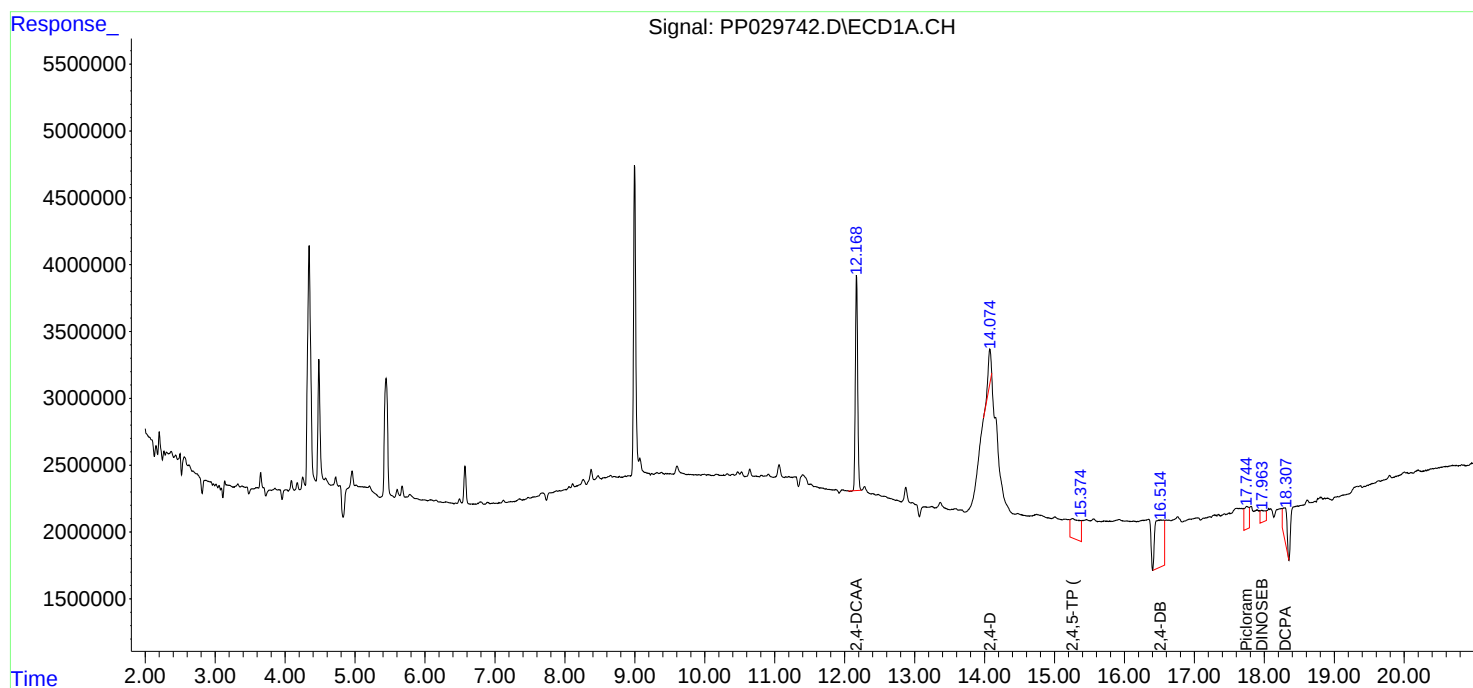


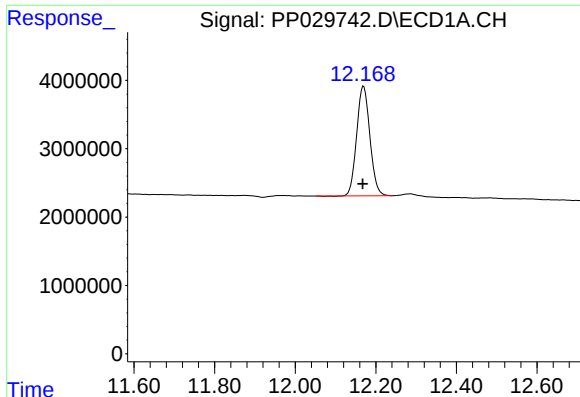

#4 2,4-DCAA


R.T.: 12.170 min
Delta R.T.: 0.002 min
Response: 36659858
Conc: 1104.60 ng/ml

Instrument :
ECD_P
ClientSampleId :

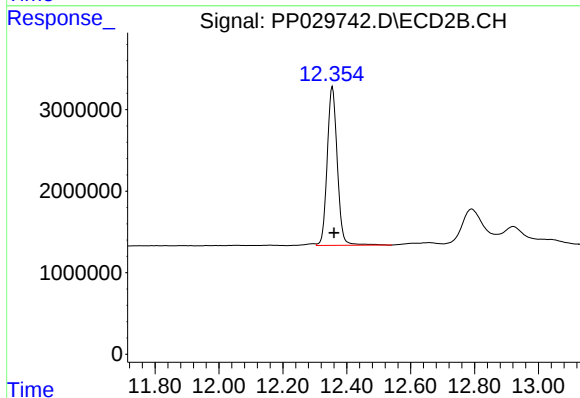


#4 2,4-DCAA

R.T.: 12.355 min
Delta R.T.: -0.005 min
Response: 42682136
Conc: 926.38 ng/ml

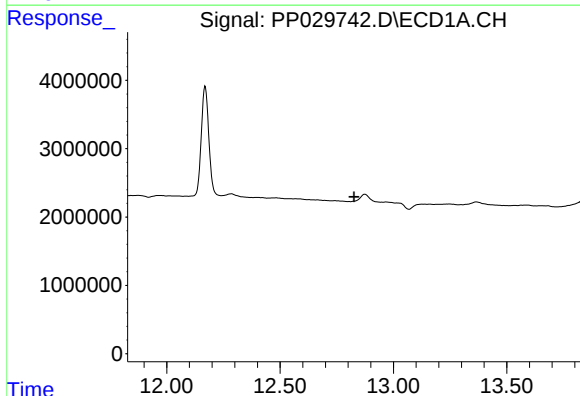


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.827 min
Response: 0
Conc: N.D.

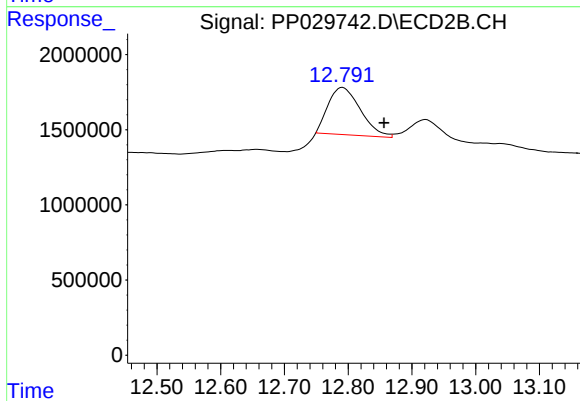

#6 MCP


R.T.: 12.791 min
Delta R.T.: -0.065 min
Response: 11074423
Conc: 163.90 ug/ml

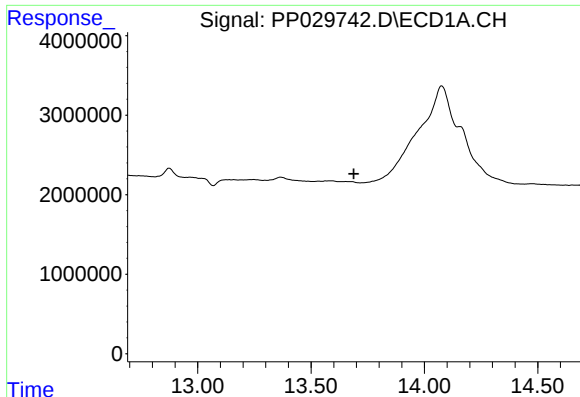

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.689 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

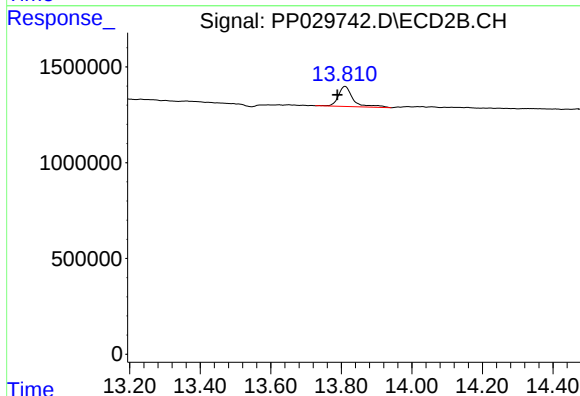


#8 DICHLORPROP

R.T.: 13.811 min
Delta R.T.: 0.022 min
Response: 3047530
Conc: 69.23 ng/ml

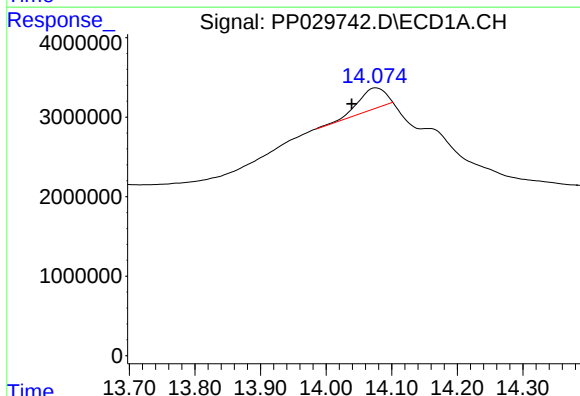


#9 2,4-D

R.T.: 14.076 min
Delta R.T.: 0.037 min
Response: 7913109
Conc: 183.06 ng/ml

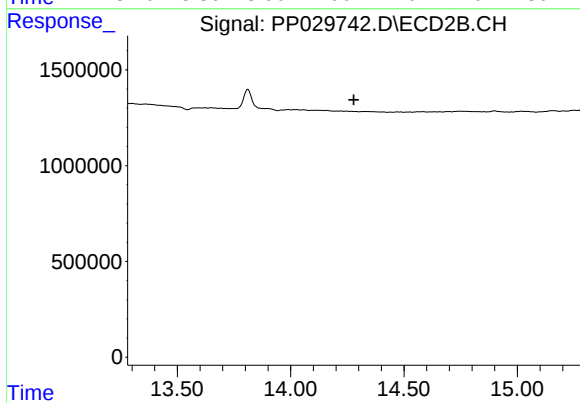

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 14.278 min
Response: 0
Conc: N.D.

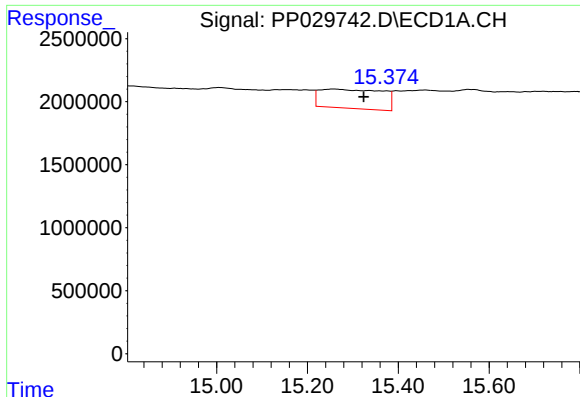

#11 2,4,5-TP (SILVEX)


R.T.: 15.258 min
Delta R.T.: -0.066 min
Response: 14570749
Conc: 54.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

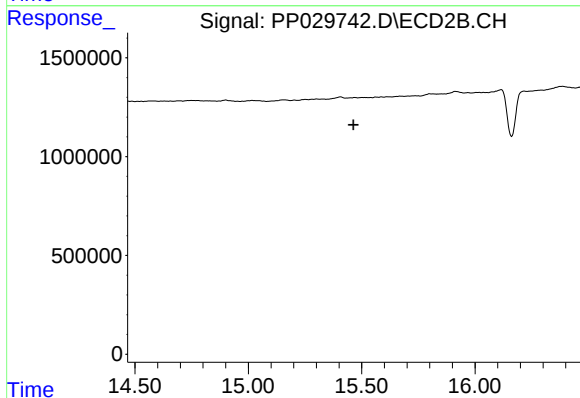


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.464 min
Response: 0
Conc: N.D.

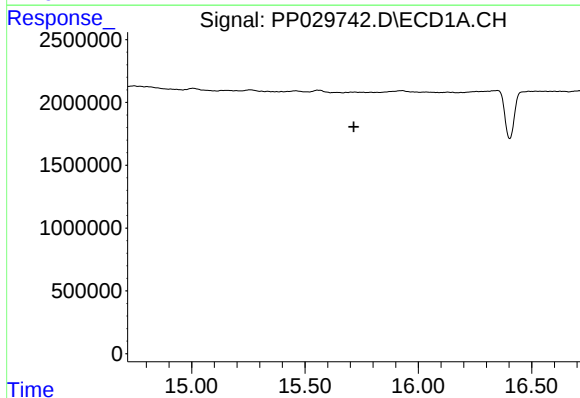


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.715 min
Response: 0
Conc: N.D.

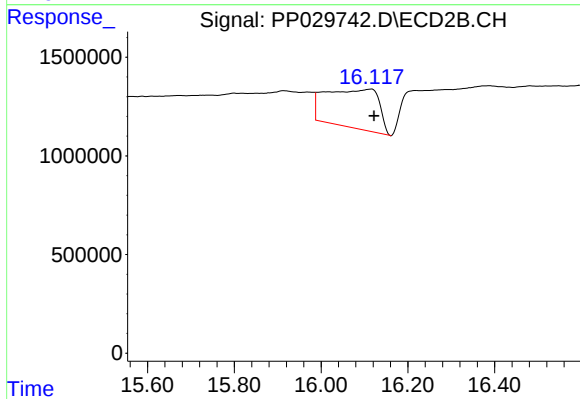

#12 2,4,5-T


R.T.: 16.116 min
Delta R.T.: -0.007 min
Response: 16746509
Conc: 96.47 ng/ml

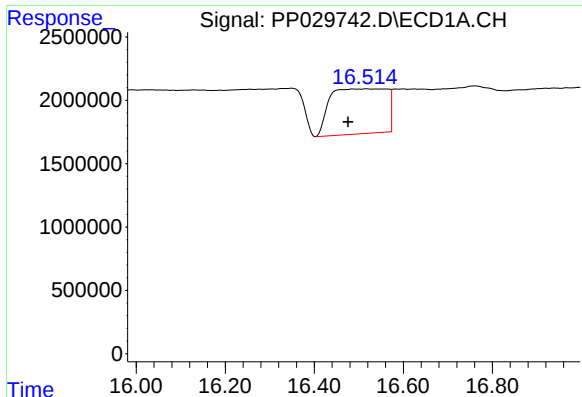

#13 2,4-DB


R.T.: 16.517 min
Delta R.T.: 0.041 min
Response: 31145427
Conc: 1310.30 ng/ml

Instrument :
ECD_P
ClientSampleId :

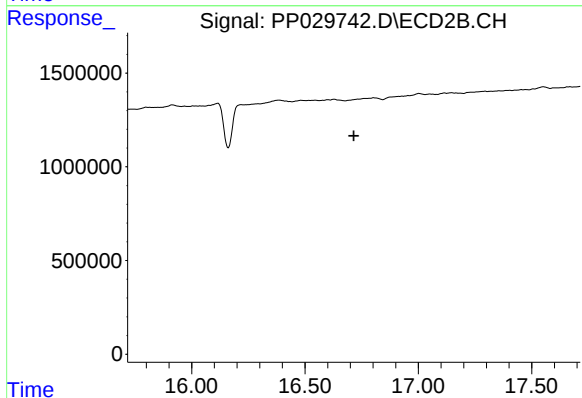


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 16.715 min
Response: 0
Conc: N.D.

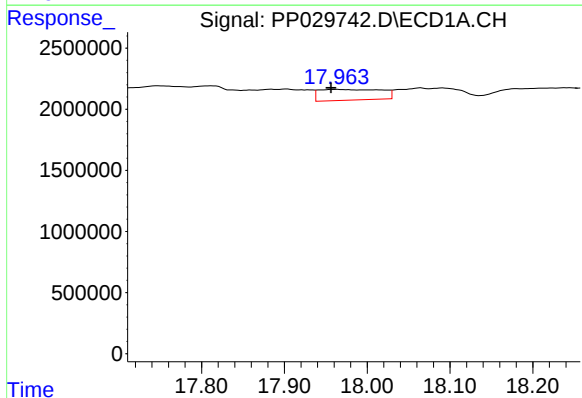


#14 DINOSEB

R.T.: 17.963 min
Delta R.T.: 0.006 min
Response: 4573448
Conc: 29.28 ng/ml

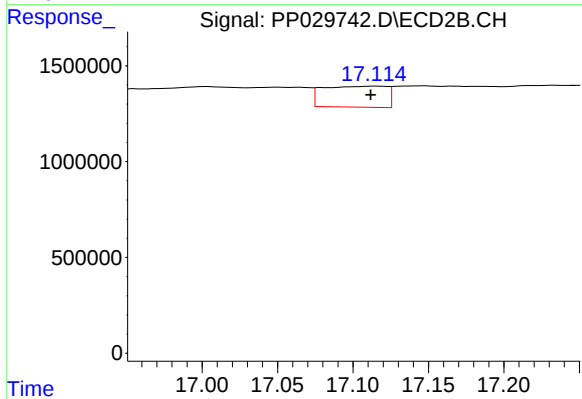

#14 DINOSEB


R.T.: 17.115 min
Delta R.T.: 0.003 min
Response: 3207363
Conc: 23.85 ng/ml

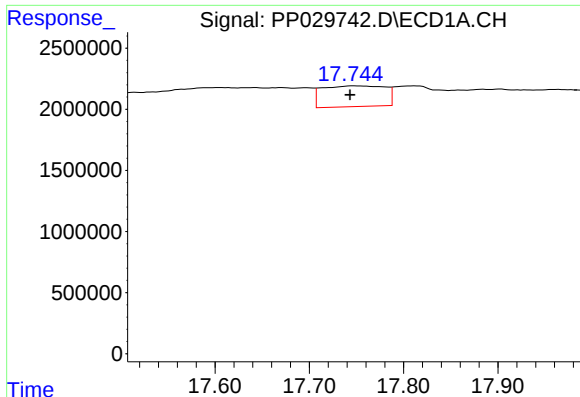

#15 Picloram


R.T.: 17.749 min
Delta R.T.: 0.005 min
Response: 7828662
Conc: 29.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

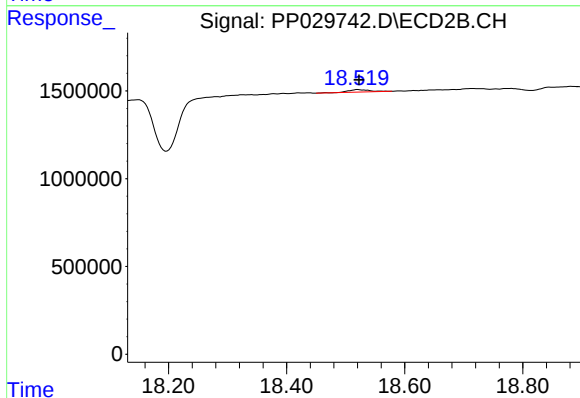


#15 Picloram

R.T.: 18.521 min
Delta R.T.: -0.002 min
Response: 361362
Conc: 1.74 ng/ml

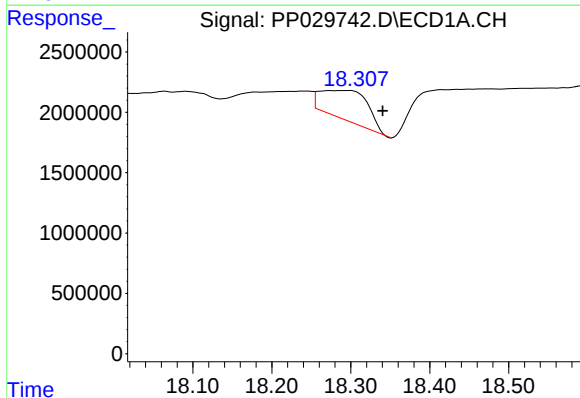

#16 DCPA

R.T.: 18.294 min
Delta R.T.: -0.046 min
Response: 10145130
Conc: 30.94 ng/ml

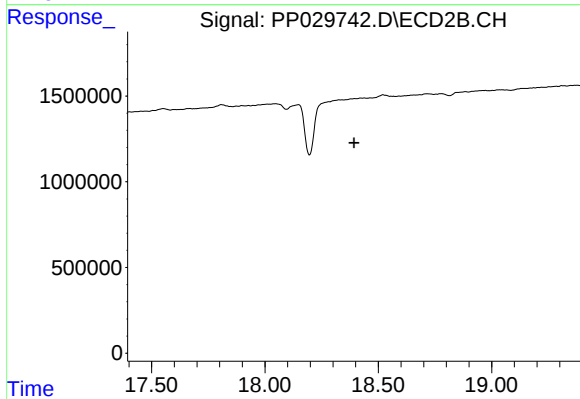

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.393 min
Response: 0
Conc: N.D.