

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040819\
 Data File : PP029788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 9:58
 Operator : EI\MA
 Sample : I.BLK
 Misc : hexane
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 10:25:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 05 15:13:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.169	12.355	16313430	19069648	491.540	413.891
Target Compounds							
2) T	3,5-DICHL...	10.620	0.000	113466	0	1.534	N.D. #
3) T	4-Nitroph...	11.761	0.000	713172	0	8.861	N.D. #
5) T	DICAMBA	12.485	12.658	-110176	516235	N.D.	3.323
6) T	MCP	0.000	12.812	0	925929	N.D.	29.234 #
11) T	2,4,5-TP ...	15.305	0.000	135038	0	0.505	N.D. #
12) T	2,4,5-T	15.704	0.000	379861	0	1.600	N.D. #
13) T	2,4-DB	16.462	0.000	107936	0	4.541	N.D. #
15) T	Picloram	17.674	0.000	103365	0	0.387	N.D. #
16) T	DCPA	18.313	0.000	228626	0	0.697	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040819\
Data File : PP029788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 9:58
Operator : EI\MA
Sample : I.BLK
Misc : hexane
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 10:25:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040519.M
Quant Title : 8080.M
QLast Update : Fri Apr 05 15:13:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

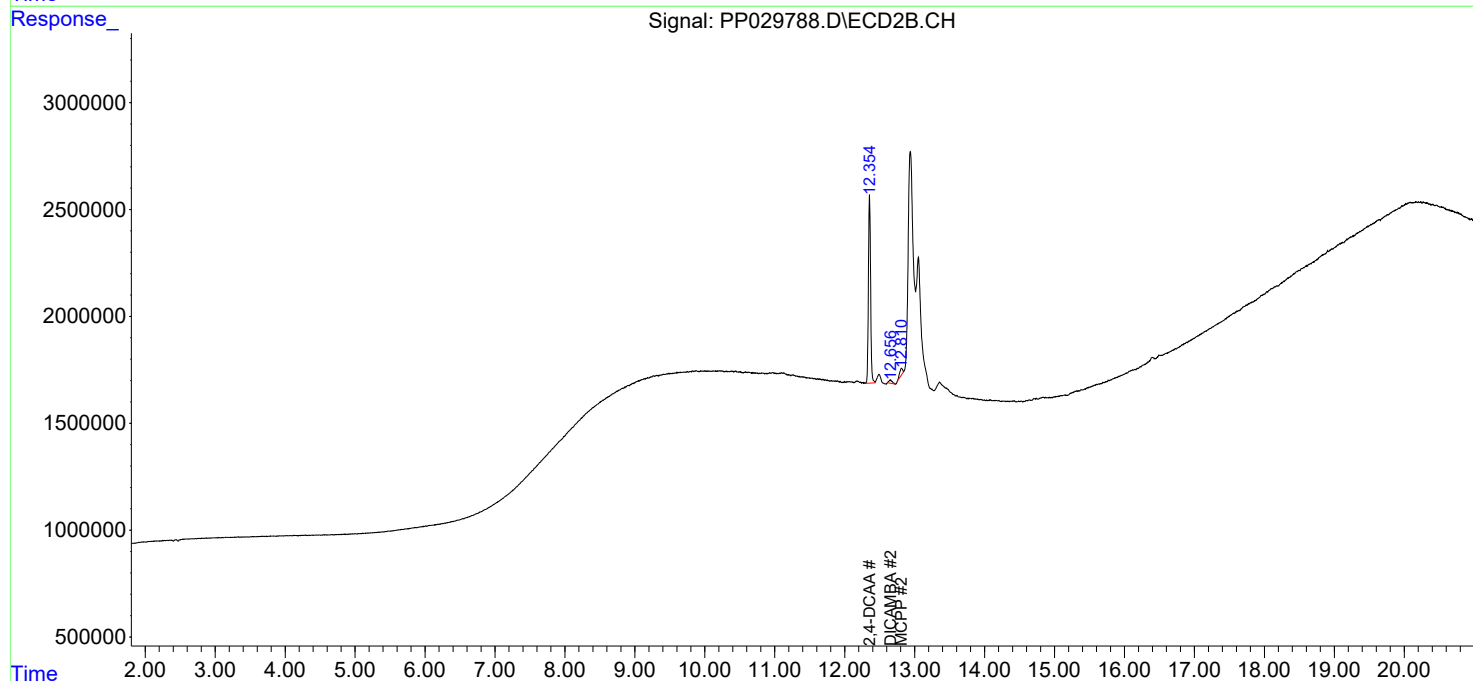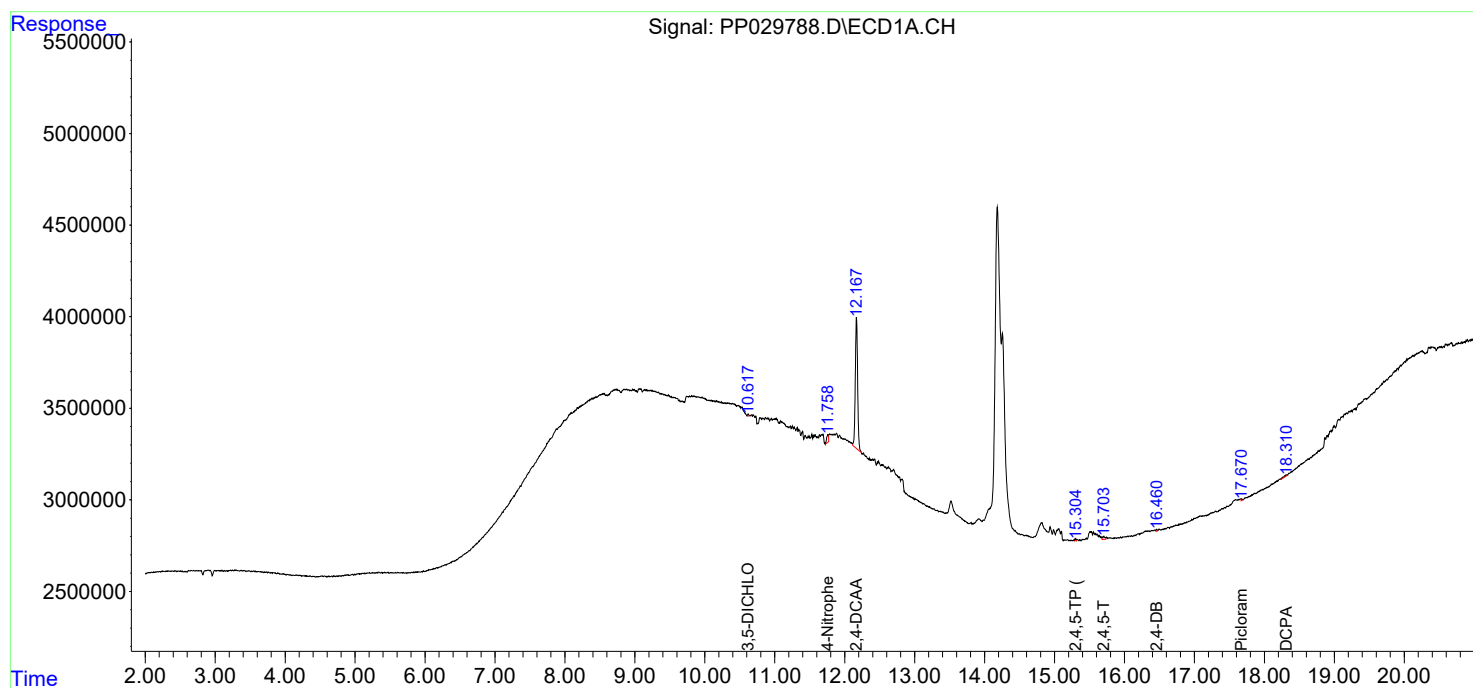


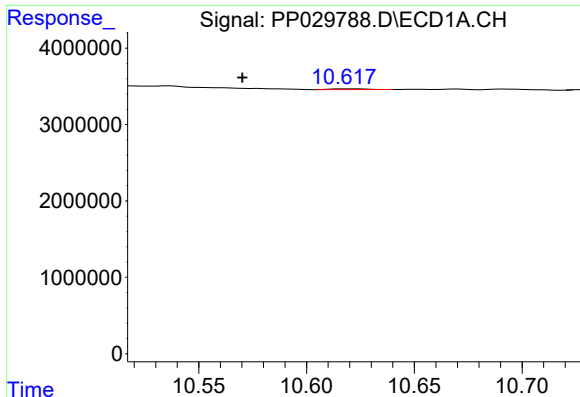

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 10.620 min
Delta R.T.: 0.050 min
Response: 113466
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

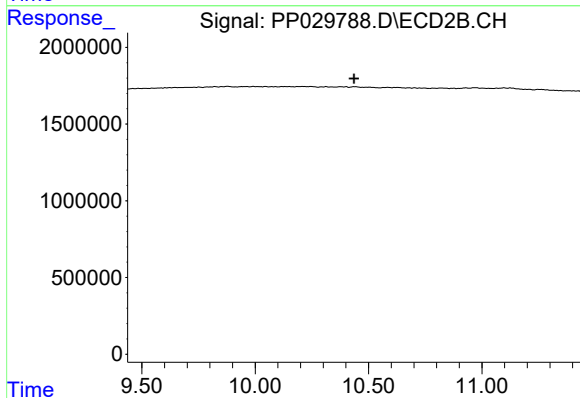


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.437 min
Response: 0
Conc: N.D.

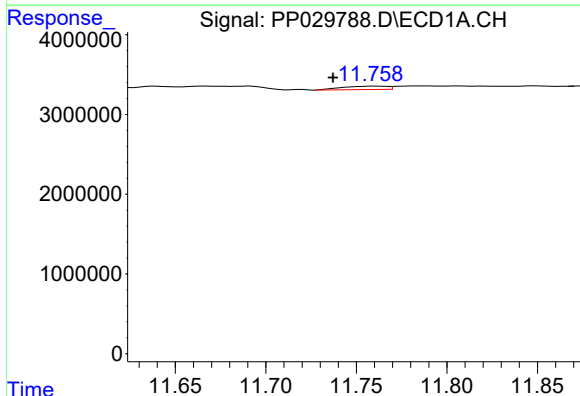


#3 4-Nitrophenol

R.T.: 11.761 min
Delta R.T.: 0.024 min
Response: 713172
Conc: 8.86 ng/ml

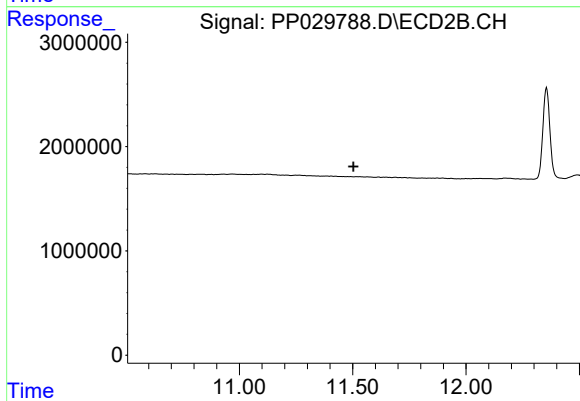

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 11.504 min
Response: 0
Conc: N.D.

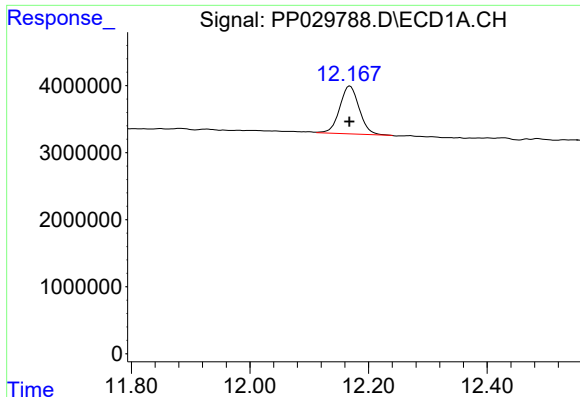

#4 2,4-DCAA


R.T.: 12.169 min
Delta R.T.: 0.001 min
Response: 16313430
Conc: 491.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

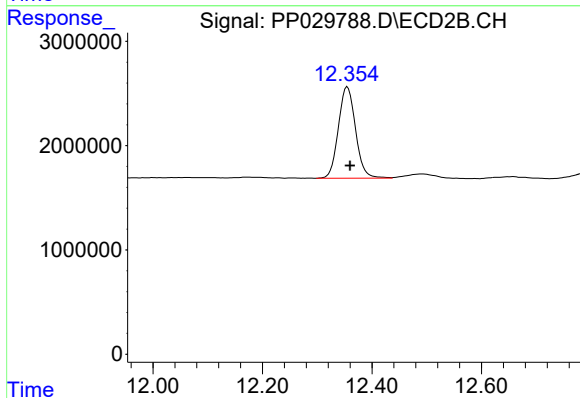


#4 2,4-DCAA

R.T.: 12.355 min
Delta R.T.: -0.005 min
Response: 19069648
Conc: 413.89 ng/ml

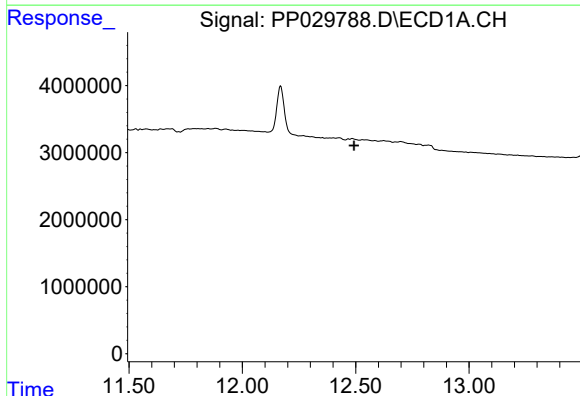


#5 DICAMBA

R.T.: 12.485 min
Delta R.T.: -0.009 min
Response: -110176
Conc: N.D.

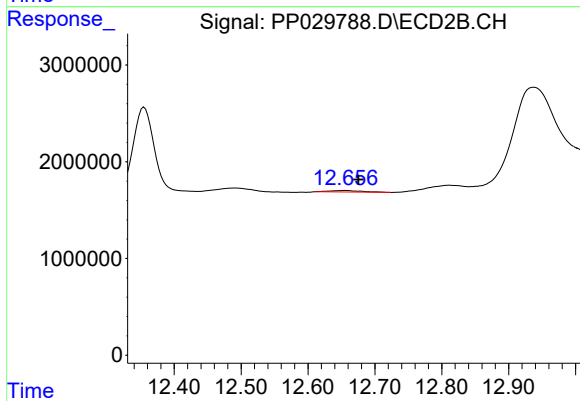

#5 DICAMBA


R.T.: 12.658 min
Delta R.T.: -0.018 min
Response: 516235
Conc: 3.32 ng/ml

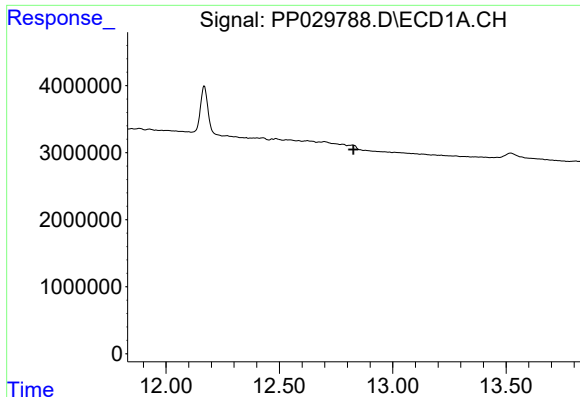

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 12.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

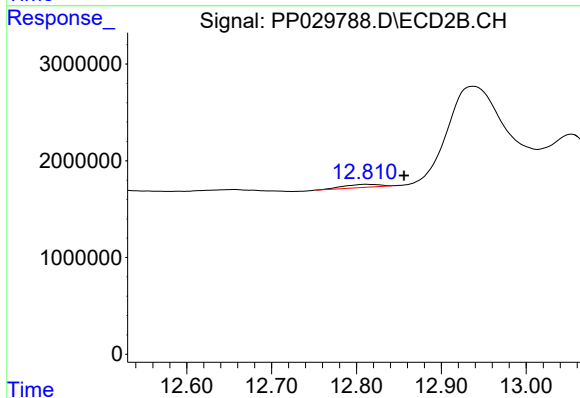


#6 MCPP

R.T.: 12.812 min
Delta R.T.: -0.044 min
Response: 925929
Conc: 29.23 ug/ml

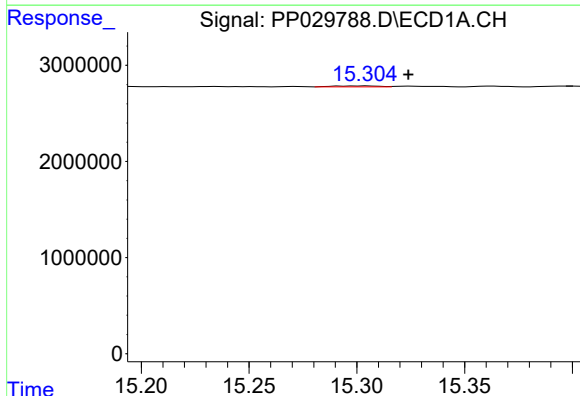


#11 2,4,5-TP (SILVEX)

R.T.: 15.305 min
Delta R.T.: -0.019 min
Response: 135038
Conc: 0.51 ng/ml

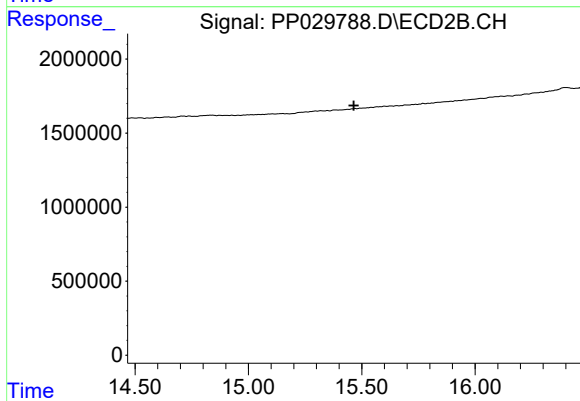

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

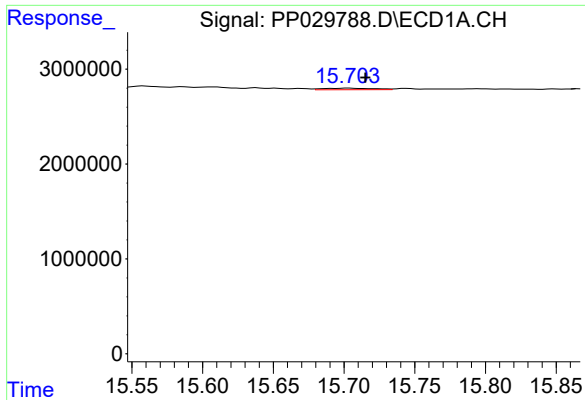

#12 2,4,5-T


R.T.: 15.704 min
Delta R.T.: -0.011 min
Response: 379861
Conc: 1.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

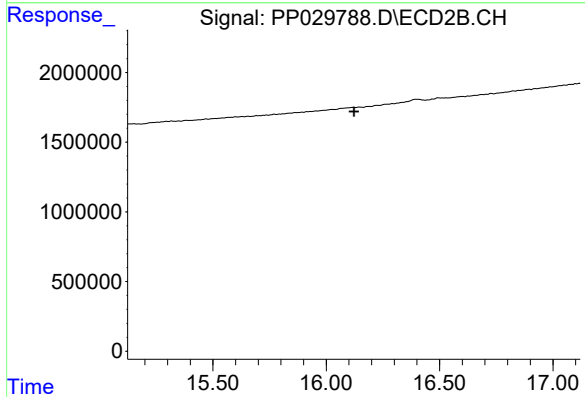


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 16.122 min
Response: 0
Conc: N.D.

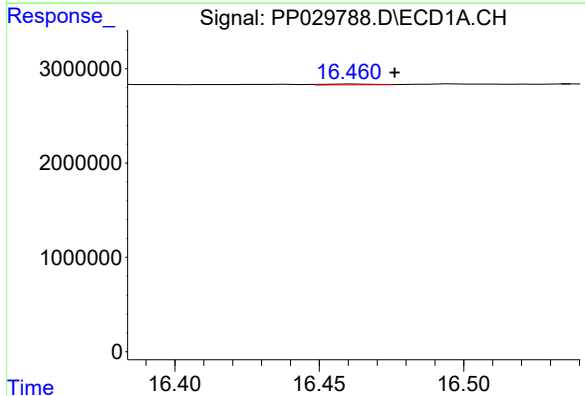


#13 2,4-DB

R.T.: 16.462 min
Delta R.T.: -0.014 min
Response: 107936
Conc: 4.54 ng/ml

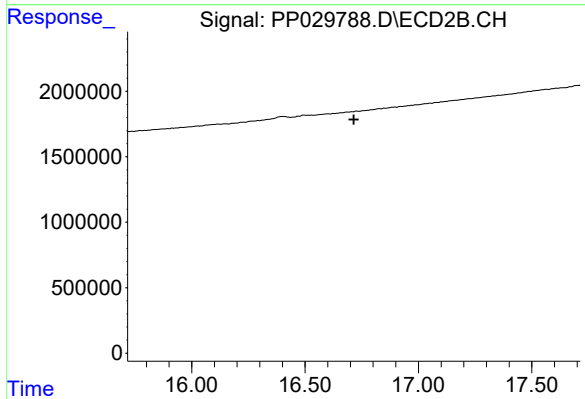

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 16.715 min
Response: 0
Conc: N.D.

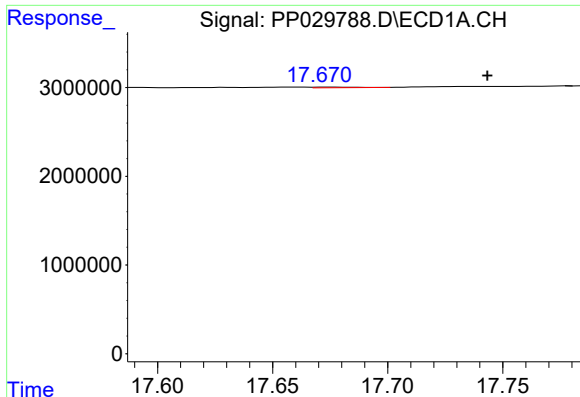

#15 Picloram


R.T.: 17.674 min
Delta R.T.: -0.070 min
Response: 103365
Conc: 0.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

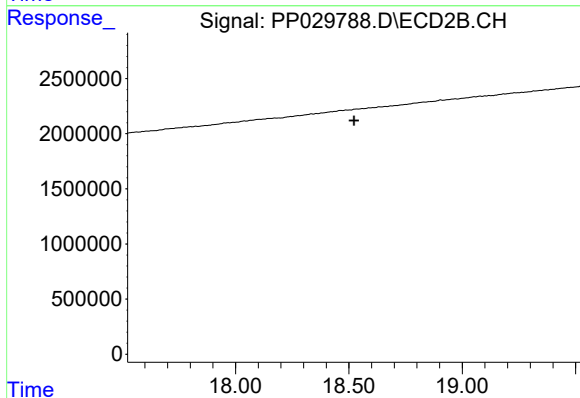


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.523 min
Response: 0
Conc: N.D.

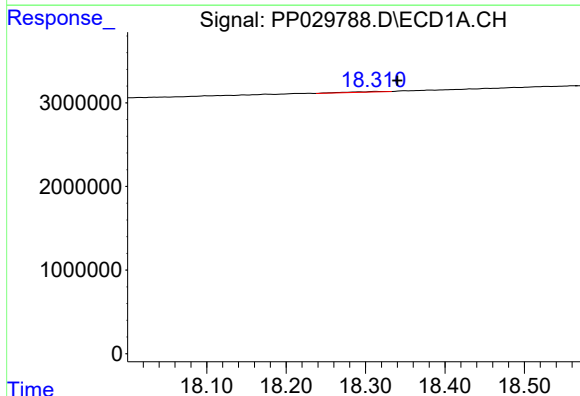

#16 DCPA

R.T.: 18.313 min
Delta R.T.: -0.027 min
Response: 228626
Conc: 0.70 ng/ml

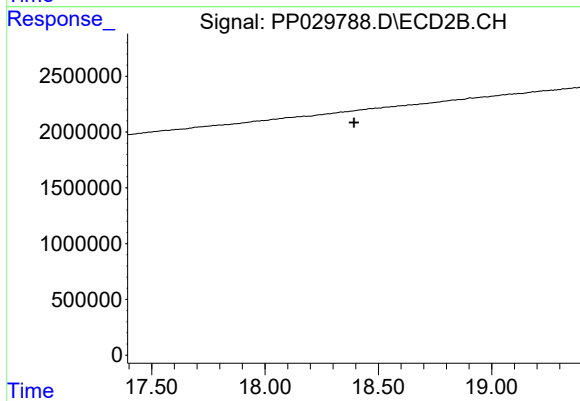

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.393 min
Response: 0
Conc: N.D.