

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041319\
 Data File : PP029846.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 7:12
 Operator : EI/SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 15:29:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041319.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 12 14:33:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.016	0.000	5785518	0	202.457	N.D. #
Target Compounds							
5) T	DICAMBA	12.362	0.000	10314876	0	72.382	N.D. #
15) T	Picloram	17.553	0.000	1085351	0	4.249	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041319\
Data File : PP029846.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 7:12
Operator : EI/SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 15:29:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041319.M
Quant Title : 8080.M
QLast Update : Fri Apr 12 14:33:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

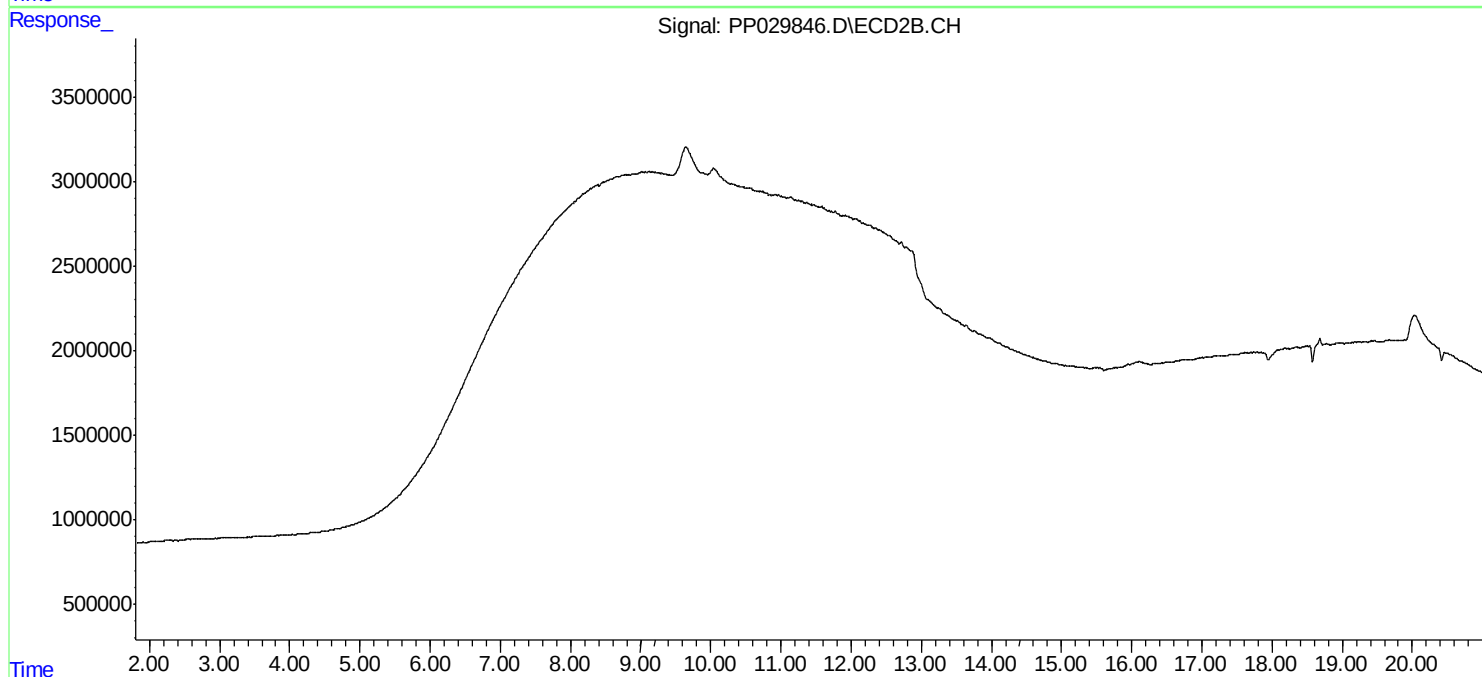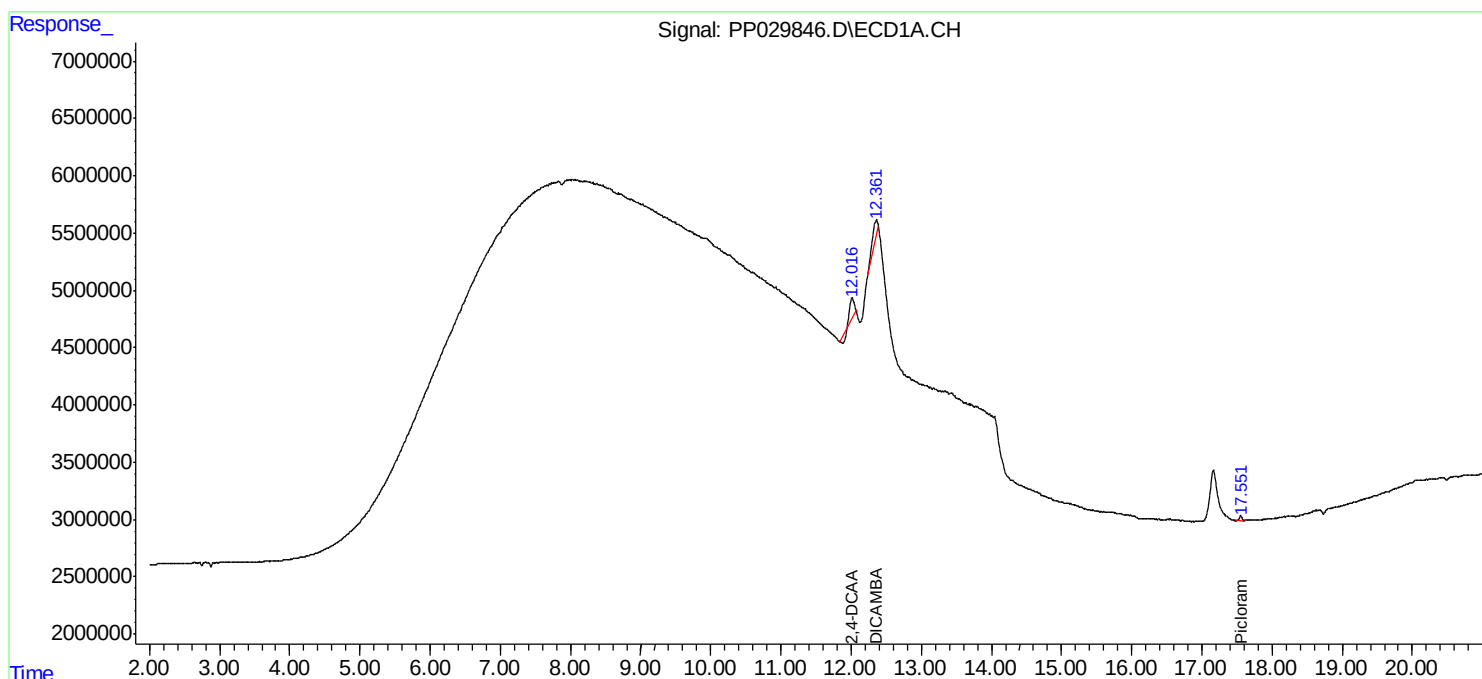


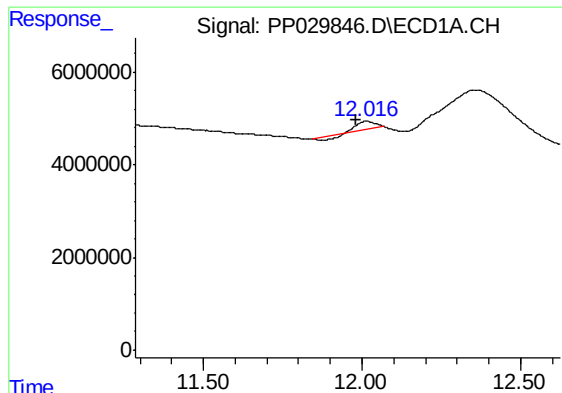

#4 2,4-DCAA


R.T.: 12.016 min
Delta R.T.: 0.036 min
Response: 5785518
Conc: 202.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

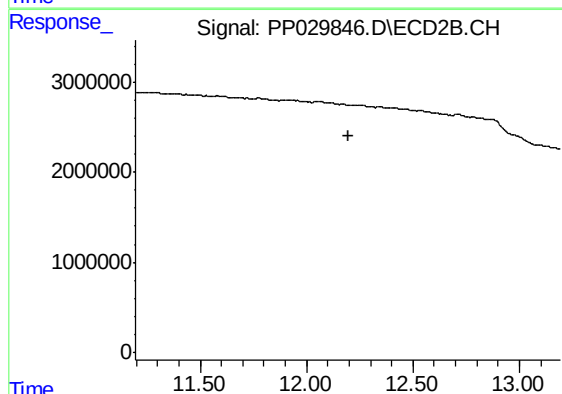


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 12.195 min
Response: 0
Conc: N.D.

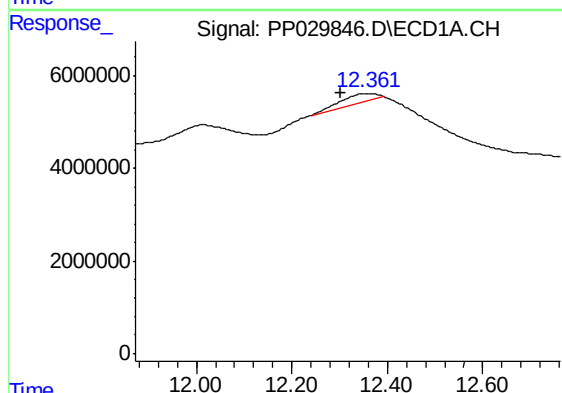


#5 DICAMBA

R.T.: 12.362 min
Delta R.T.: 0.059 min
Response: 10314876
Conc: 72.38 ng/ml

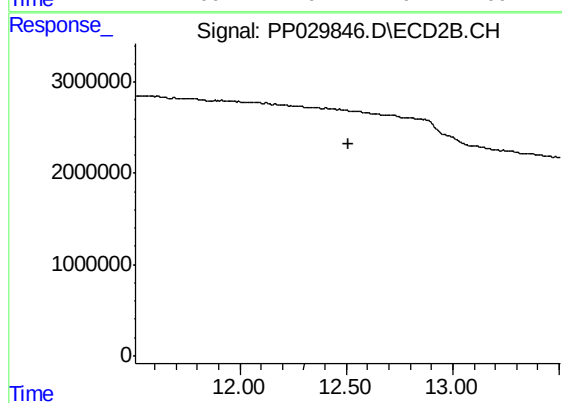

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 12.508 min
Response: 0
Conc: N.D.

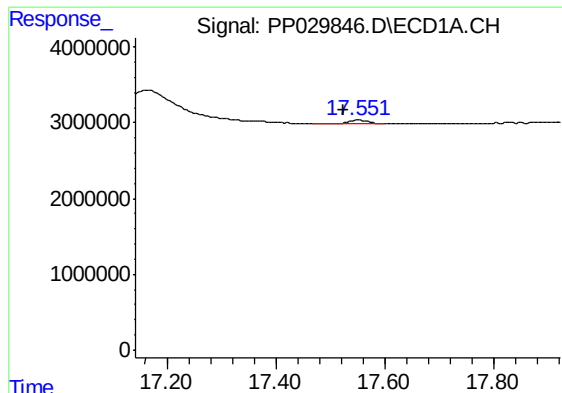

#15 Picloram

R.T.: 17.553 min
Delta R.T.: 0.028 min
Response: 1085351
Conc: 4.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

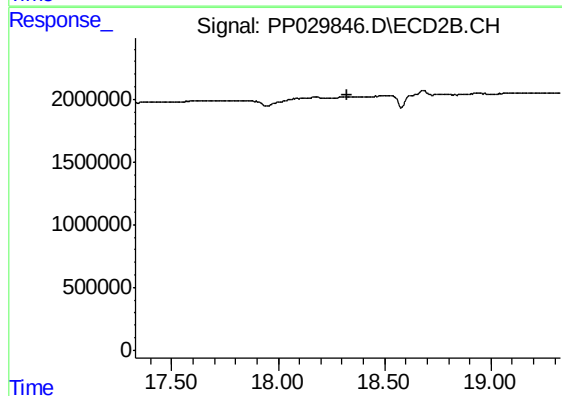

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.326 min
Response: 0
Conc: N.D.