

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042322\
 Data File : PP046558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2022 15:47
 Operator : YP\AJ
 Sample : N2514-07
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-16-1A-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/25/2022
 Supervised By :mohammad ahmed 04/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:37:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.867	3.137	34596588	63421432	14.332m	19.334m#
2) SA Decachlor...	9.967	8.472f	28006583	41233579	19.033	17.286

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042322\
Data File : PP046558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2022 15:47
Operator : YP\AJ
Sample : N2514-07
Misc :
ALS Vial : 83 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-16-1A-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2022
Supervised By :mohammad ahmed 04/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:37:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

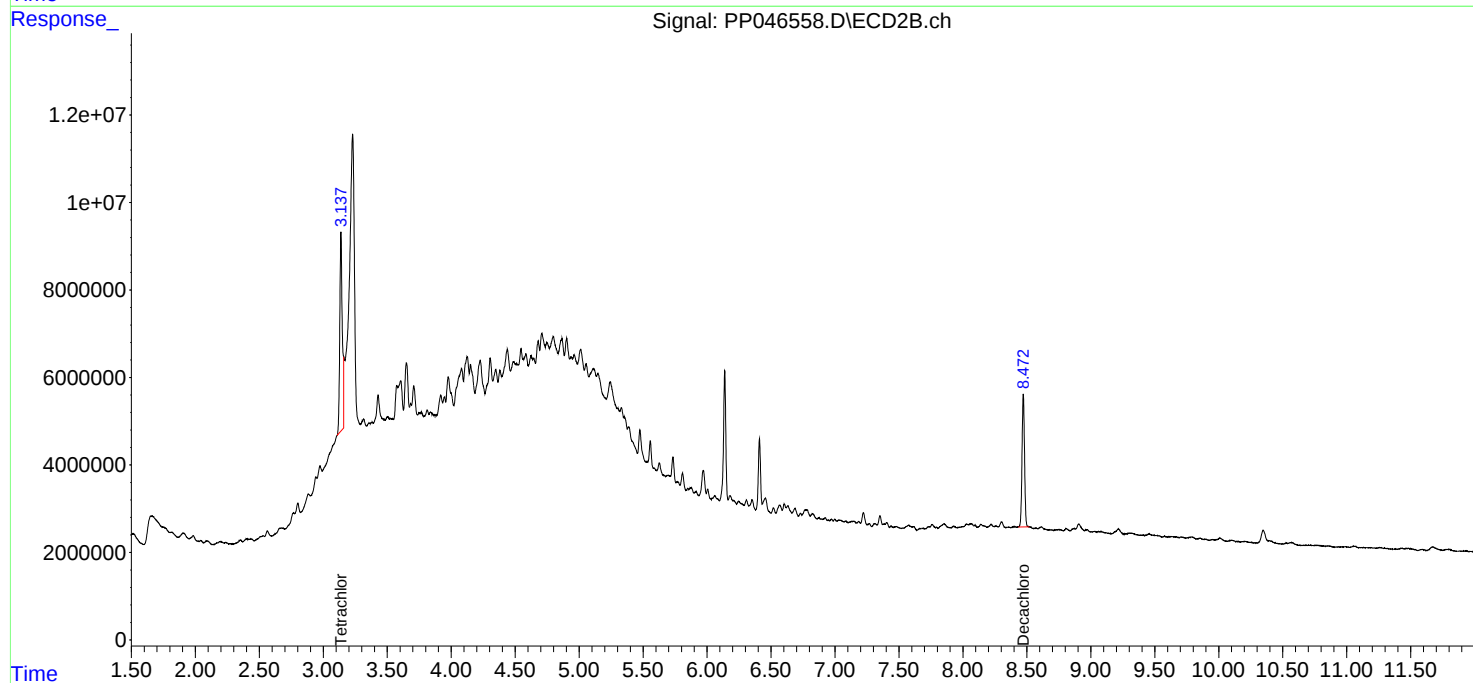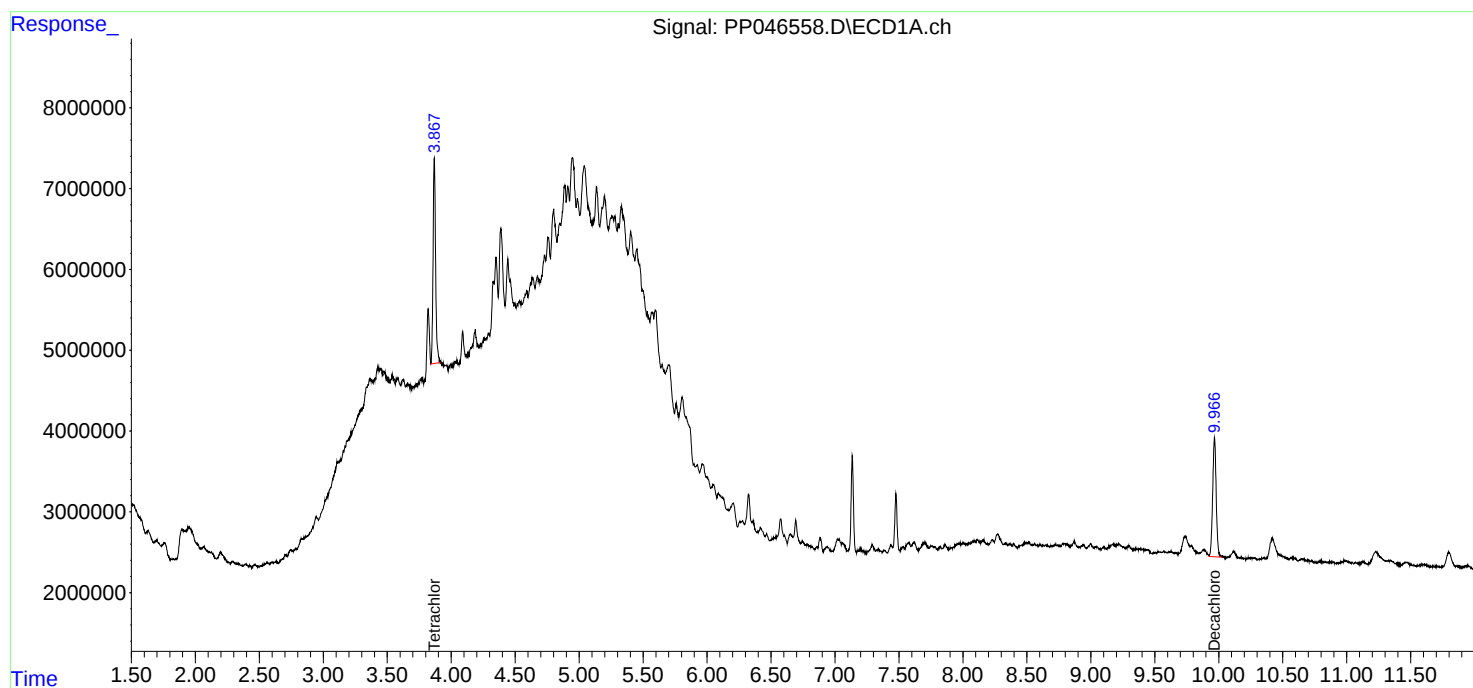

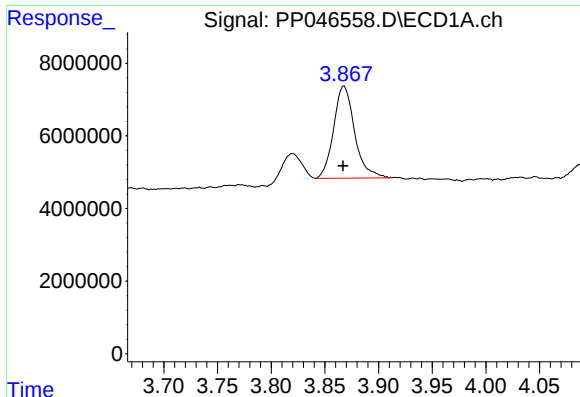


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 34596588
Conc: 14.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-16-1A-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2022
Supervised By :mohammad ahmed 04/25/2022

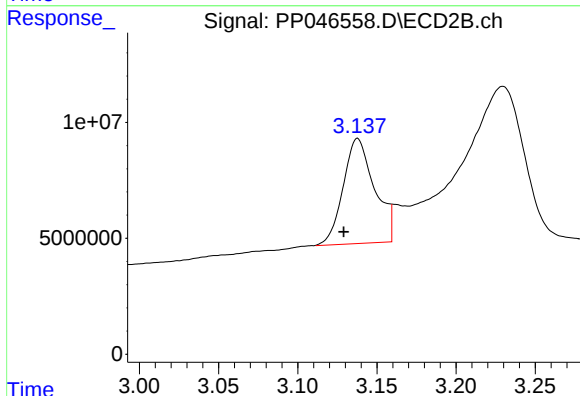


#1 Tetrachloro-m-xylene

R.T.: 3.137 min
Delta R.T.: 0.008 min
Response: 63421432
Conc: 19.33 ng/ml m

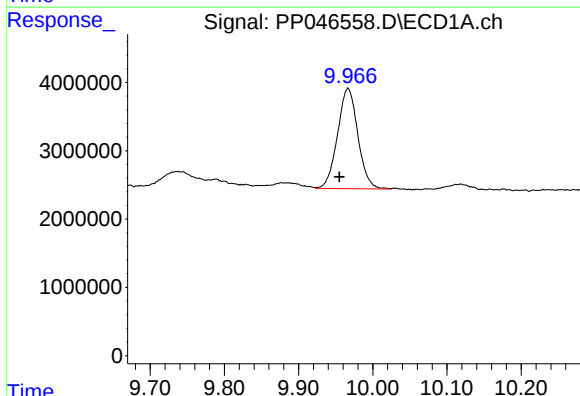

#2 Decachlorobiphenyl

R.T.: 9.967 min
Delta R.T.: 0.012 min
Response: 28006583
Conc: 19.03 ng/ml

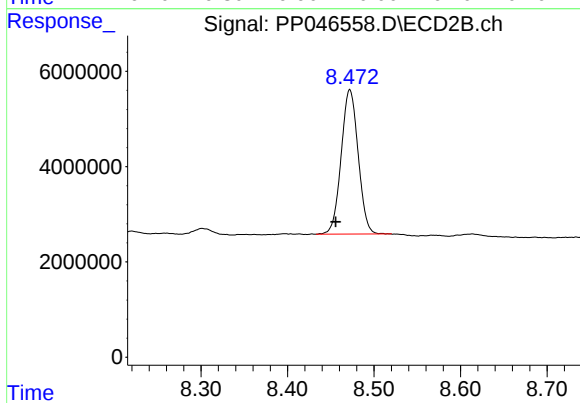

#2 Decachlorobiphenyl

R.T.: 8.472 min
Delta R.T.: 0.016 min
Response: 41233579
Conc: 17.29 ng/ml