

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050424\
 Data File : PP064811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2024 04:29
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 23:06:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP043024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 01 05:01:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.377	3.453	26136280	40122546	14.850	17.017
2) SA Decachlor...	10.067	8.350	21393352	36428792	24.045	19.529
Target Compounds						
9) L2 AR-1221-2	4.682	3.745	428257	553321	32.103	26.832
20) L4 AR-1242-5	0.000	5.322f	0	630670	N.D.	12.551 #
24) L5 AR-1248-4	6.397f	0.000	5453053	0	110.110	N.D. #
25) L5 AR-1248-5	0.000	5.322f	0	630670	N.D.	9.762 #
26) L6 AR-1254-1	6.397	5.322f	5453053	630670	91.330	5.349 #
28) L6 AR-1254-3	6.977	0.000	27317040	0	322.014	N.D. #
30) L6 AR-1254-5	7.679	0.000	258379	0	4.685	N.D. #
32) L7 AR-1260-2	0.000	6.137f	0	2057870	N.D.	15.735 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050424\
Data File : PP064811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2024 04:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 23:06:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP043024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 01 05:01:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

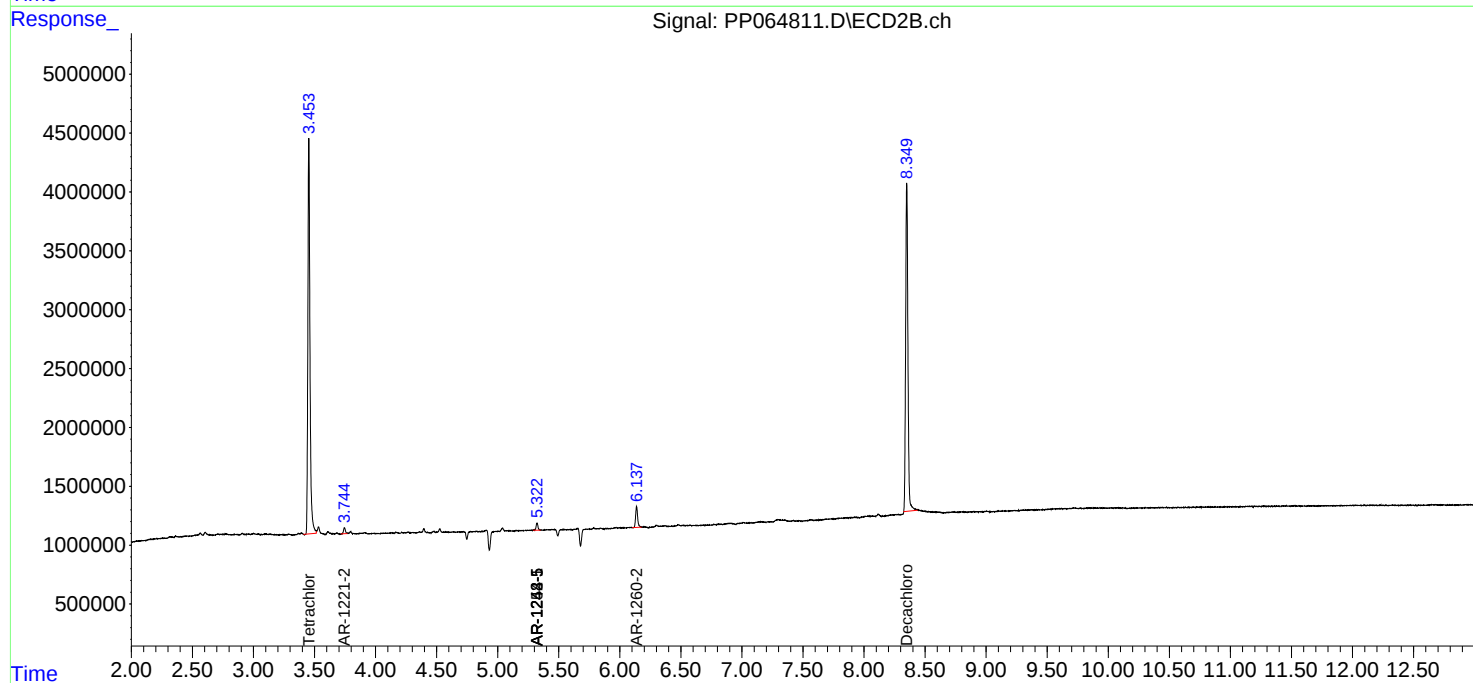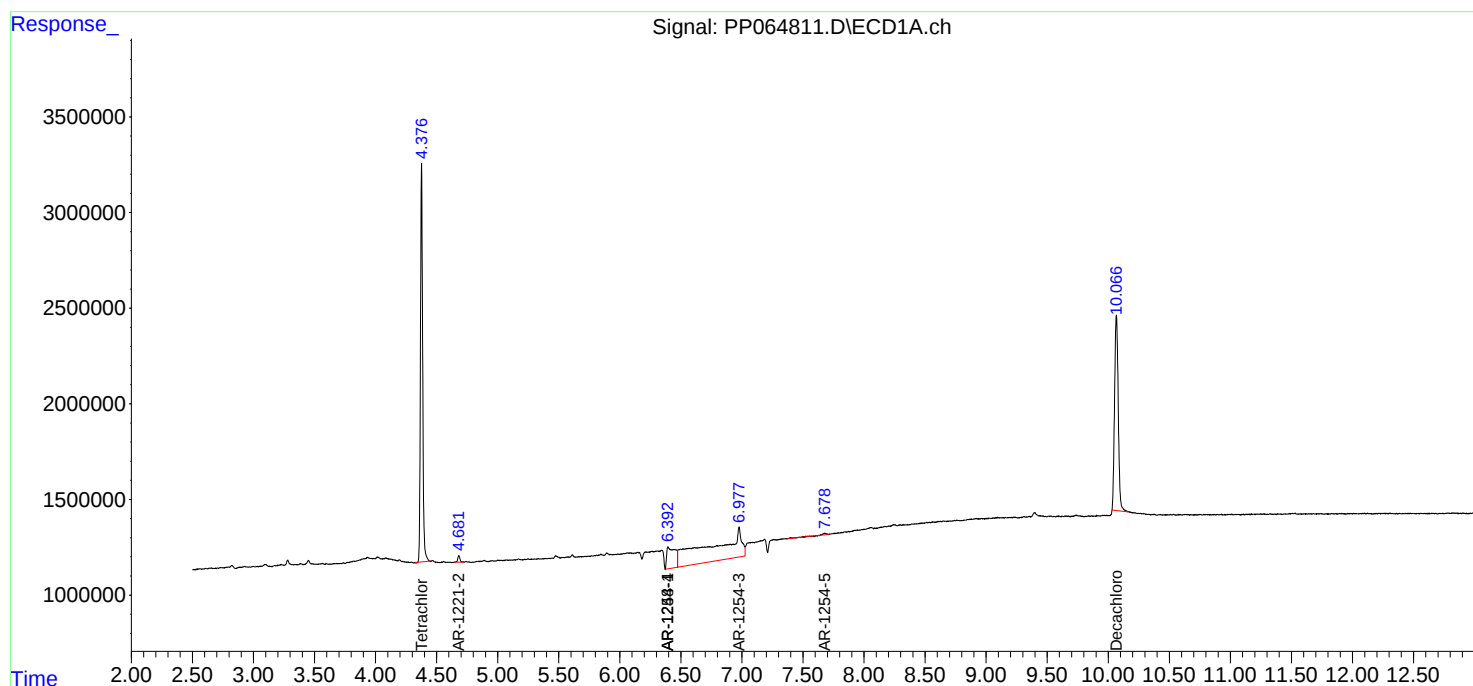


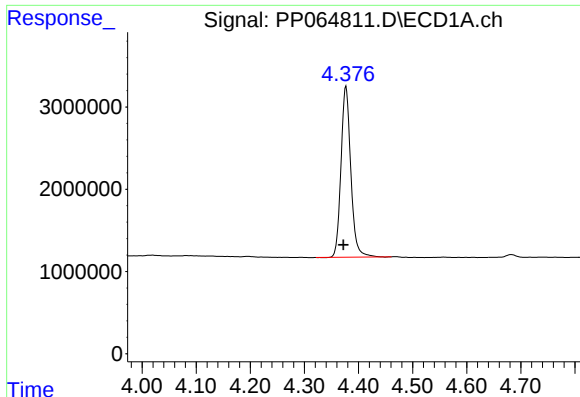

#1 Tetrachloro-m-xylene


R.T.: 4.377 min
Delta R.T.: 0.005 min
Response: 26136280
Conc: 14.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

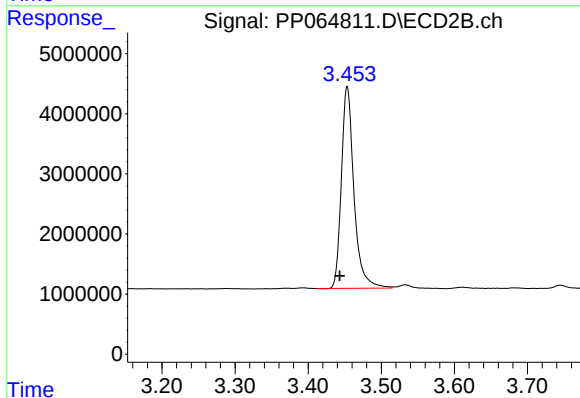


#1 Tetrachloro-m-xylene

R.T.: 3.453 min
Delta R.T.: 0.010 min
Response: 40122546
Conc: 17.02 ng/ml

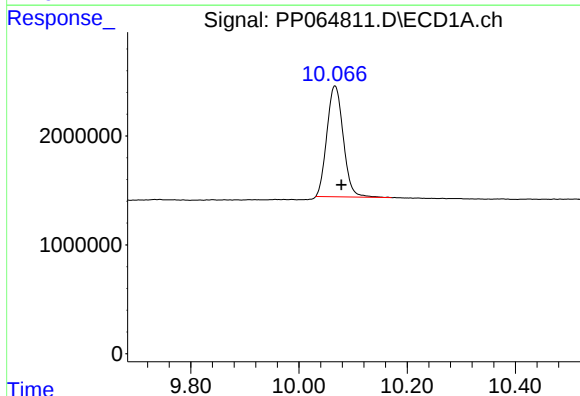


#2 Decachlorobiphenyl

R.T.: 10.067 min
Delta R.T.: -0.012 min
Response: 21393352
Conc: 24.05 ng/ml

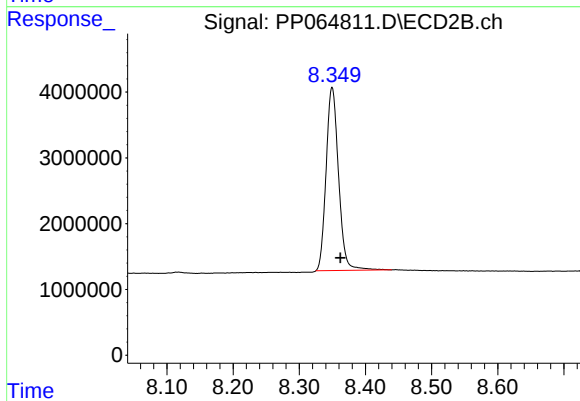

#2 Decachlorobiphenyl


R.T.: 8.350 min
Delta R.T.: -0.012 min
Response: 36428792
Conc: 19.53 ng/ml

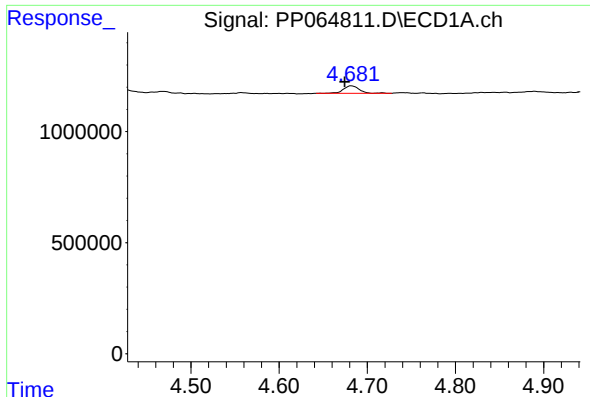

#9 AR-1221-2


R.T.: 4.682 min
Delta R.T.: 0.008 min
Response: 428257
Conc: 32.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

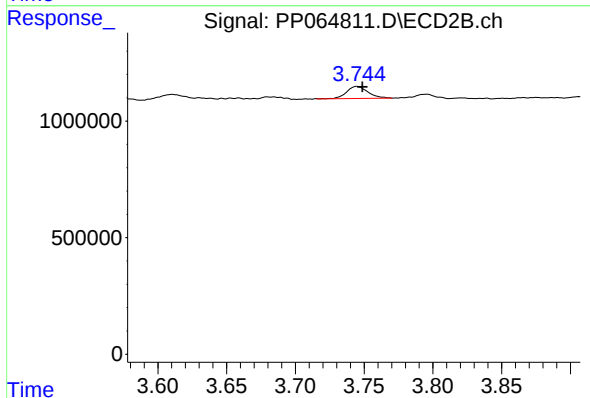


#9 AR-1221-2

R.T.: 3.745 min
Delta R.T.: -0.004 min
Response: 553321
Conc: 26.83 ng/ml

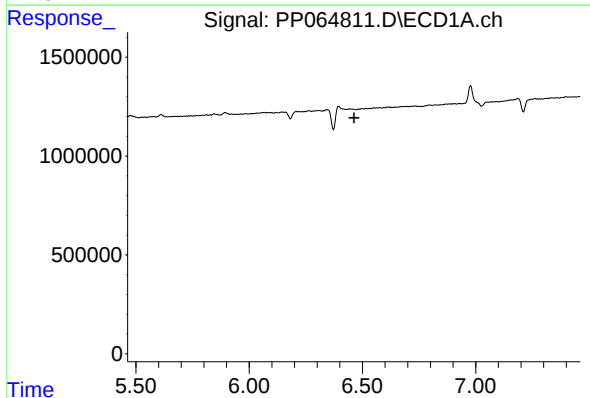


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

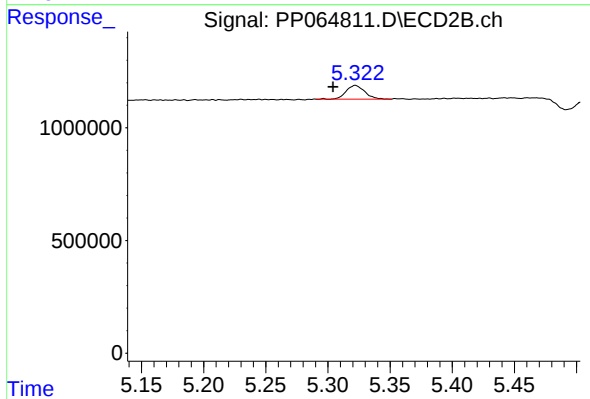

#20 AR-1242-5


R.T.: 5.322 min
Delta R.T.: 0.018 min
Response: 630670
Conc: 12.55 ng/ml

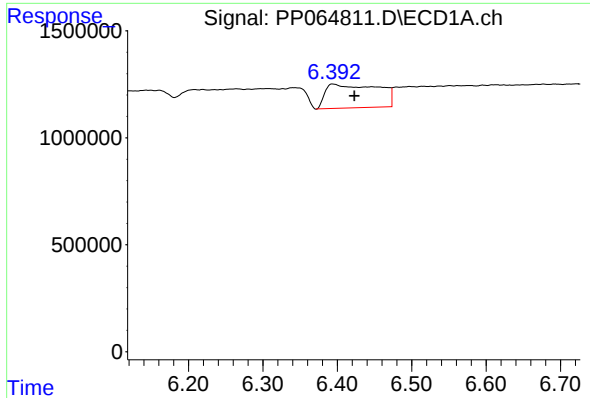

#24 AR-1248-4


R.T.: 6.397 min
Delta R.T.: -0.026 min
Response: 5453053
Conc: 110.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

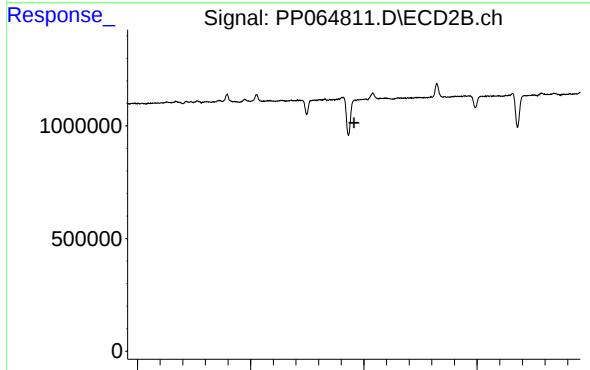


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

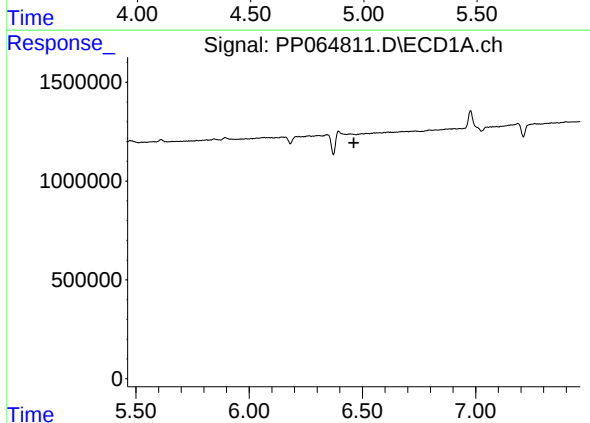


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.

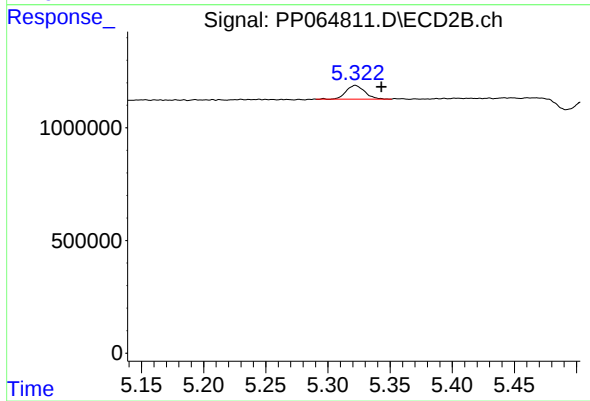

#25 AR-1248-5


R.T.: 5.322 min
Delta R.T.: -0.021 min
Response: 630670
Conc: 9.76 ng/ml

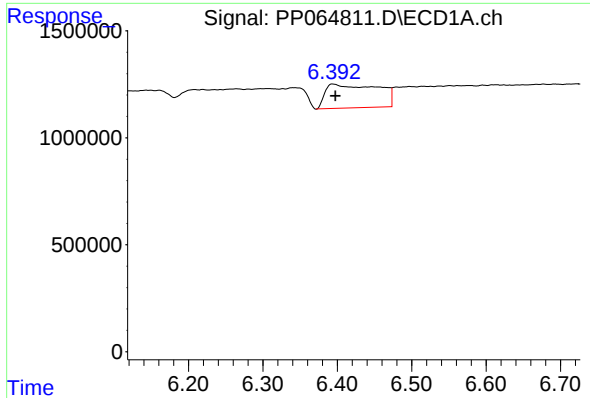

#26 AR-1254-1


R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 5453053
Conc: 91.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

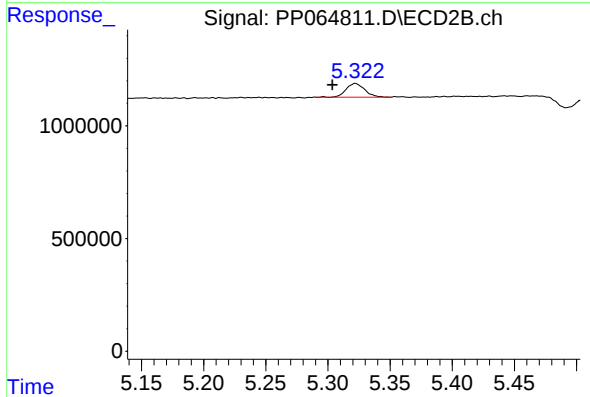


#26 AR-1254-1

R.T.: 5.322 min
Delta R.T.: 0.018 min
Response: 630670
Conc: 5.35 ng/ml

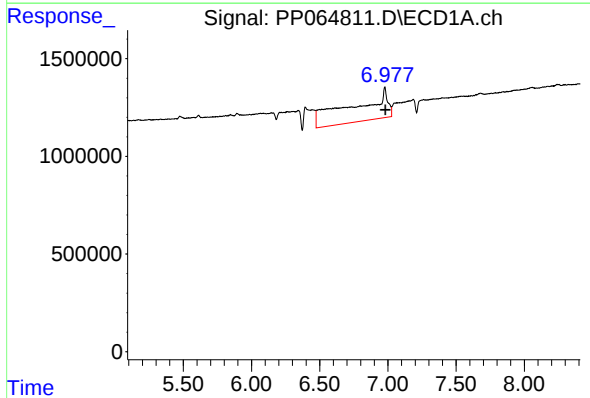


#28 AR-1254-3

R.T.: 6.977 min
Delta R.T.: -0.005 min
Response: 27317040
Conc: 322.01 ng/ml

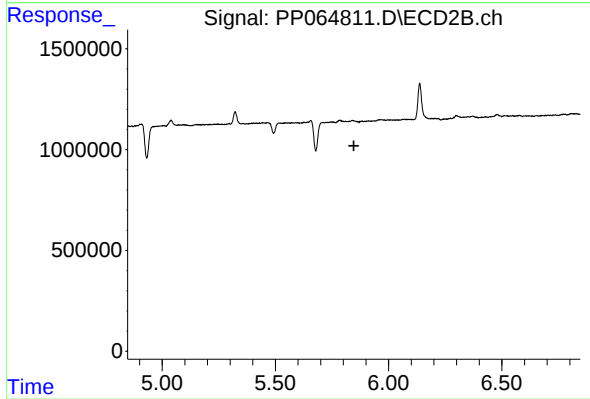

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 5.847 min
Response: 0
Conc: N.D.

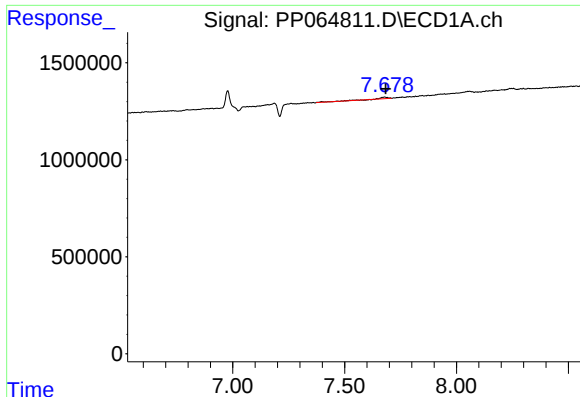

#30 AR-1254-5


R.T.: 7.679 min
Delta R.T.: -0.006 min
Response: 258379
Conc: 4.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

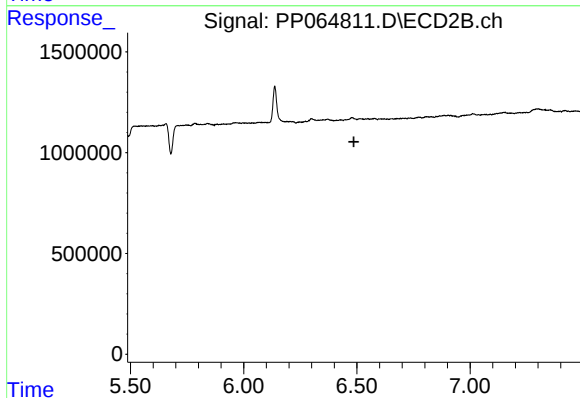


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.487 min
Response: 0
Conc: N.D.

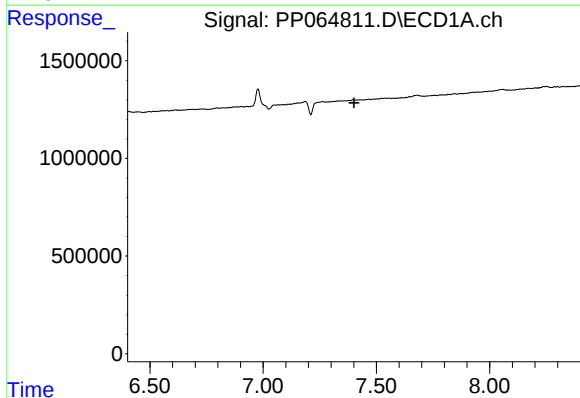

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.401 min
Response: 0
Conc: N.D.

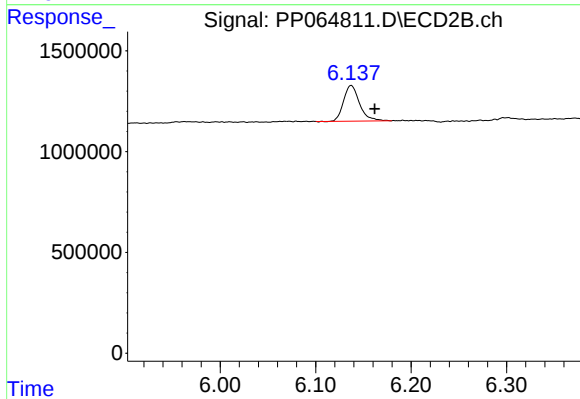

#32 AR-1260-2

R.T.: 6.137 min
Delta R.T.: -0.025 min
Response: 2057870
Conc: 15.74 ng/ml