

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050522\
 Data File : PP047048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2022 14:30
 Operator : YP\AJ
 Sample : N2651-07 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CL-57-05-02-22-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/09/2022
 Supervised By :mohammad ahmed 05/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 15:59:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 05 11:06:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.854	3.122	4109786	5997002	1.703m	1.828
2) SA Decachlor...	9.921	8.431	3719144	5071468	2.527m	2.126

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050522\
Data File : PP047048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2022 14:30
Operator : YP\AJ
Sample : N2651-07 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CL-57-05-02-22-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 15:59:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 05 11:06:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

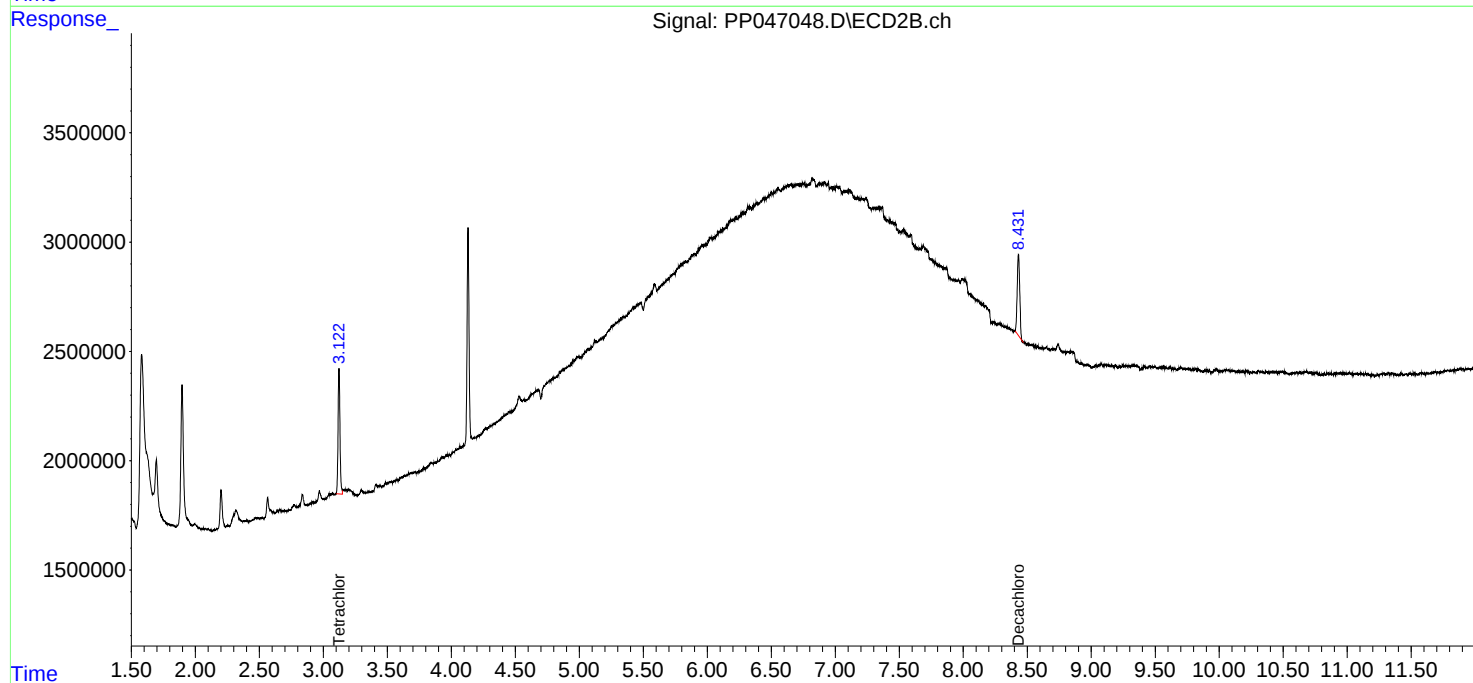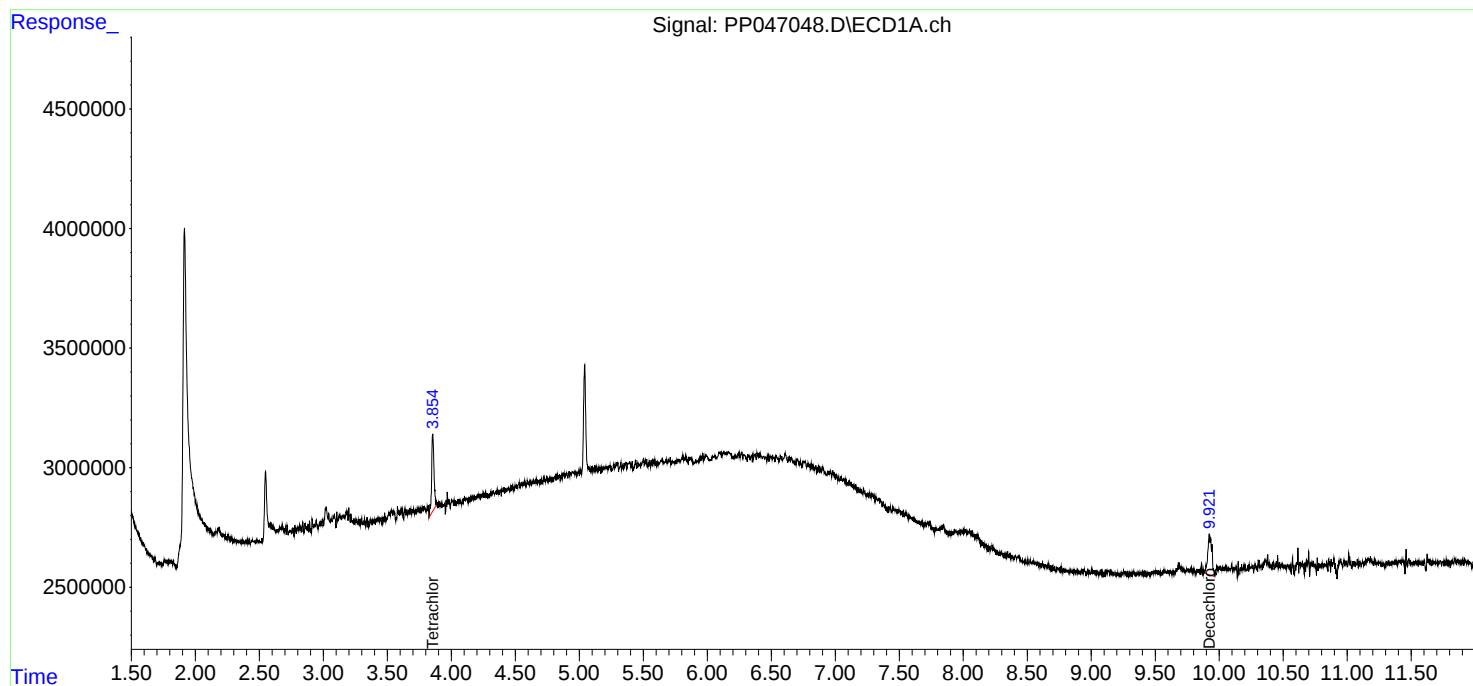

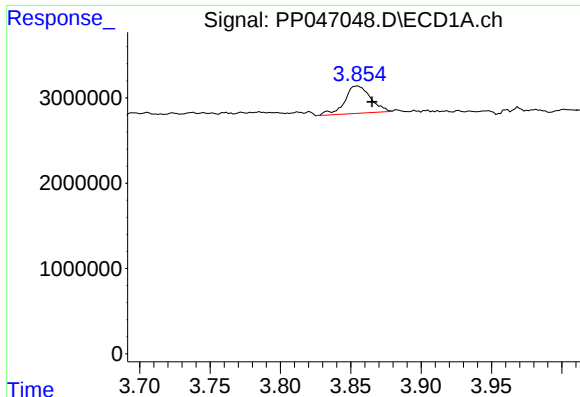


#1 Tetrachloro-m-xylene

R.T.: 3.854 min
Delta R.T.: -0.011 min
Response: 4109786
Conc: 1.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-57-05-02-22-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/09/2022

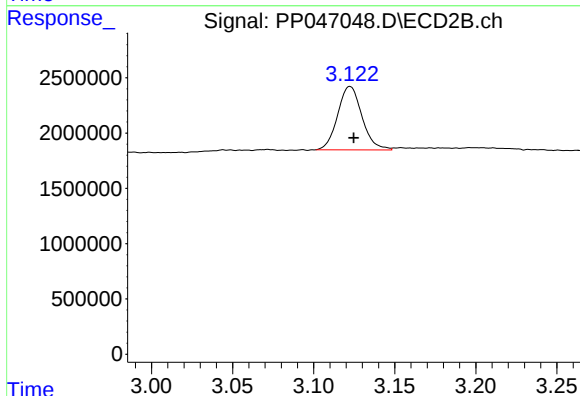


#1 Tetrachloro-m-xylene

R.T.: 3.122 min
Delta R.T.: -0.002 min
Response: 5997002
Conc: 1.83 ng/ml

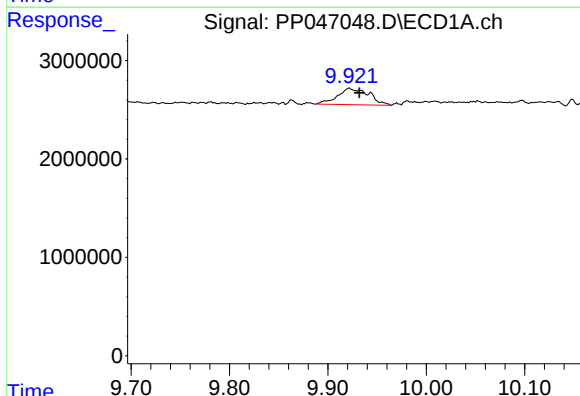

#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.011 min
Response: 3719144
Conc: 2.53 ng/ml m

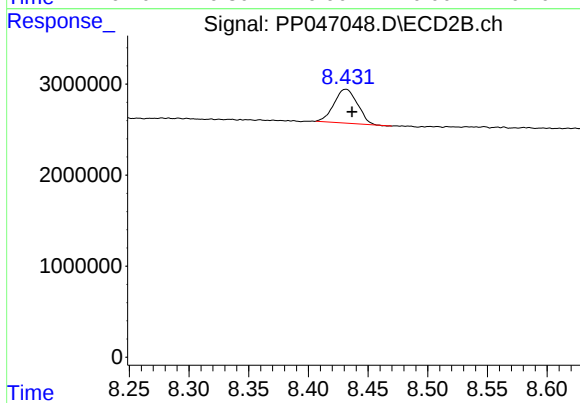

#2 Decachlorobiphenyl

R.T.: 8.431 min
Delta R.T.: -0.005 min
Response: 5071468
Conc: 2.13 ng/ml